

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020122\
 Data File : BM033955.D
 Acq On : 02 Feb 2022 01:02
 Operator : CG/JU
 Sample : N1307-06
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0Q04

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 02/02/2022
 Supervised By :Yogesh Patel 02/04/2022

Quant Time: Feb 02 01:52:55 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Feb 01 02:16:28 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.925	152	122139	20.000	ng/u1	0.00
20) Naphthalene-d8	10.736	136	512464	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.566	164	313395	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.301	188	596103	20.000	ng/u1	0.00
79) Chrysene-d12	21.459	240	516602	20.000	ng/u1	0.00
88) Perylene-d12	23.847	264	517293	20.000	ng/u1	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.290	96	12463	4.024	ng/uL	0.00
4) Pyridine-d5	3.731	84	21734	2.514	ng/u1	0.01
7) Phenol-d5	7.084	99	65855	6.436	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.248	67	192979	30.935	ng/u1	0.00
11) 2-Chlorophenol-d4	7.454	132	198975	24.271	ng/u1	0.00
15) 4-Methylphenol-d8	8.631	113	123308	15.208	ng/u1	-0.01
21) Nitrobenzene-d5	9.089	128	126213	30.694	ng/u1	0.00
24) 2-Nitrophenol-d4	9.813	143	130748	29.444	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.354	165	205862	25.619	ng/u1	0.00
31) 4-Chloroaniline-d4	10.872	131	157290	14.175	ng/u1	0.00
46) Dimethylphthalate-d6	13.971	166	829423	35.417	ng/u1	0.00
49) Acenaphthylene-d8	14.254	160	923837	32.202	ng/u1	0.00
54) 4-Nitrophenol-d4	14.754	143	17970m	4.491	ng/u1	0.00
60) Fluorene-d10	15.554	176	677358	34.639	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.665	200	114196	30.515	ng/u1	0.00
73) Anthracene-d10	17.395	188	1078689	37.786	ng/u1	0.00
81) Pyrene-d10	19.683	212	1157144	37.940	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.694	264	1039287	38.251	ng/u1	-0.01
Target Compounds						
71) Pentachlorophenol	16.954	266	84079	17.800	ng/u1	Qvalue 97

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020122\
Data File : BM033955.D
Acq On : 02 Feb 2022 01:02
Operator : CG/JU
Sample : N1307-06
Misc :
ALS Vial : 25 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
C0Q04

Quant Time: Feb 02 01:52:55 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Feb 01 02:16:28 2022
Response via : Initial Calibration

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 02/02/2022
Supervised By :Yogesh Patel 02/04/2022

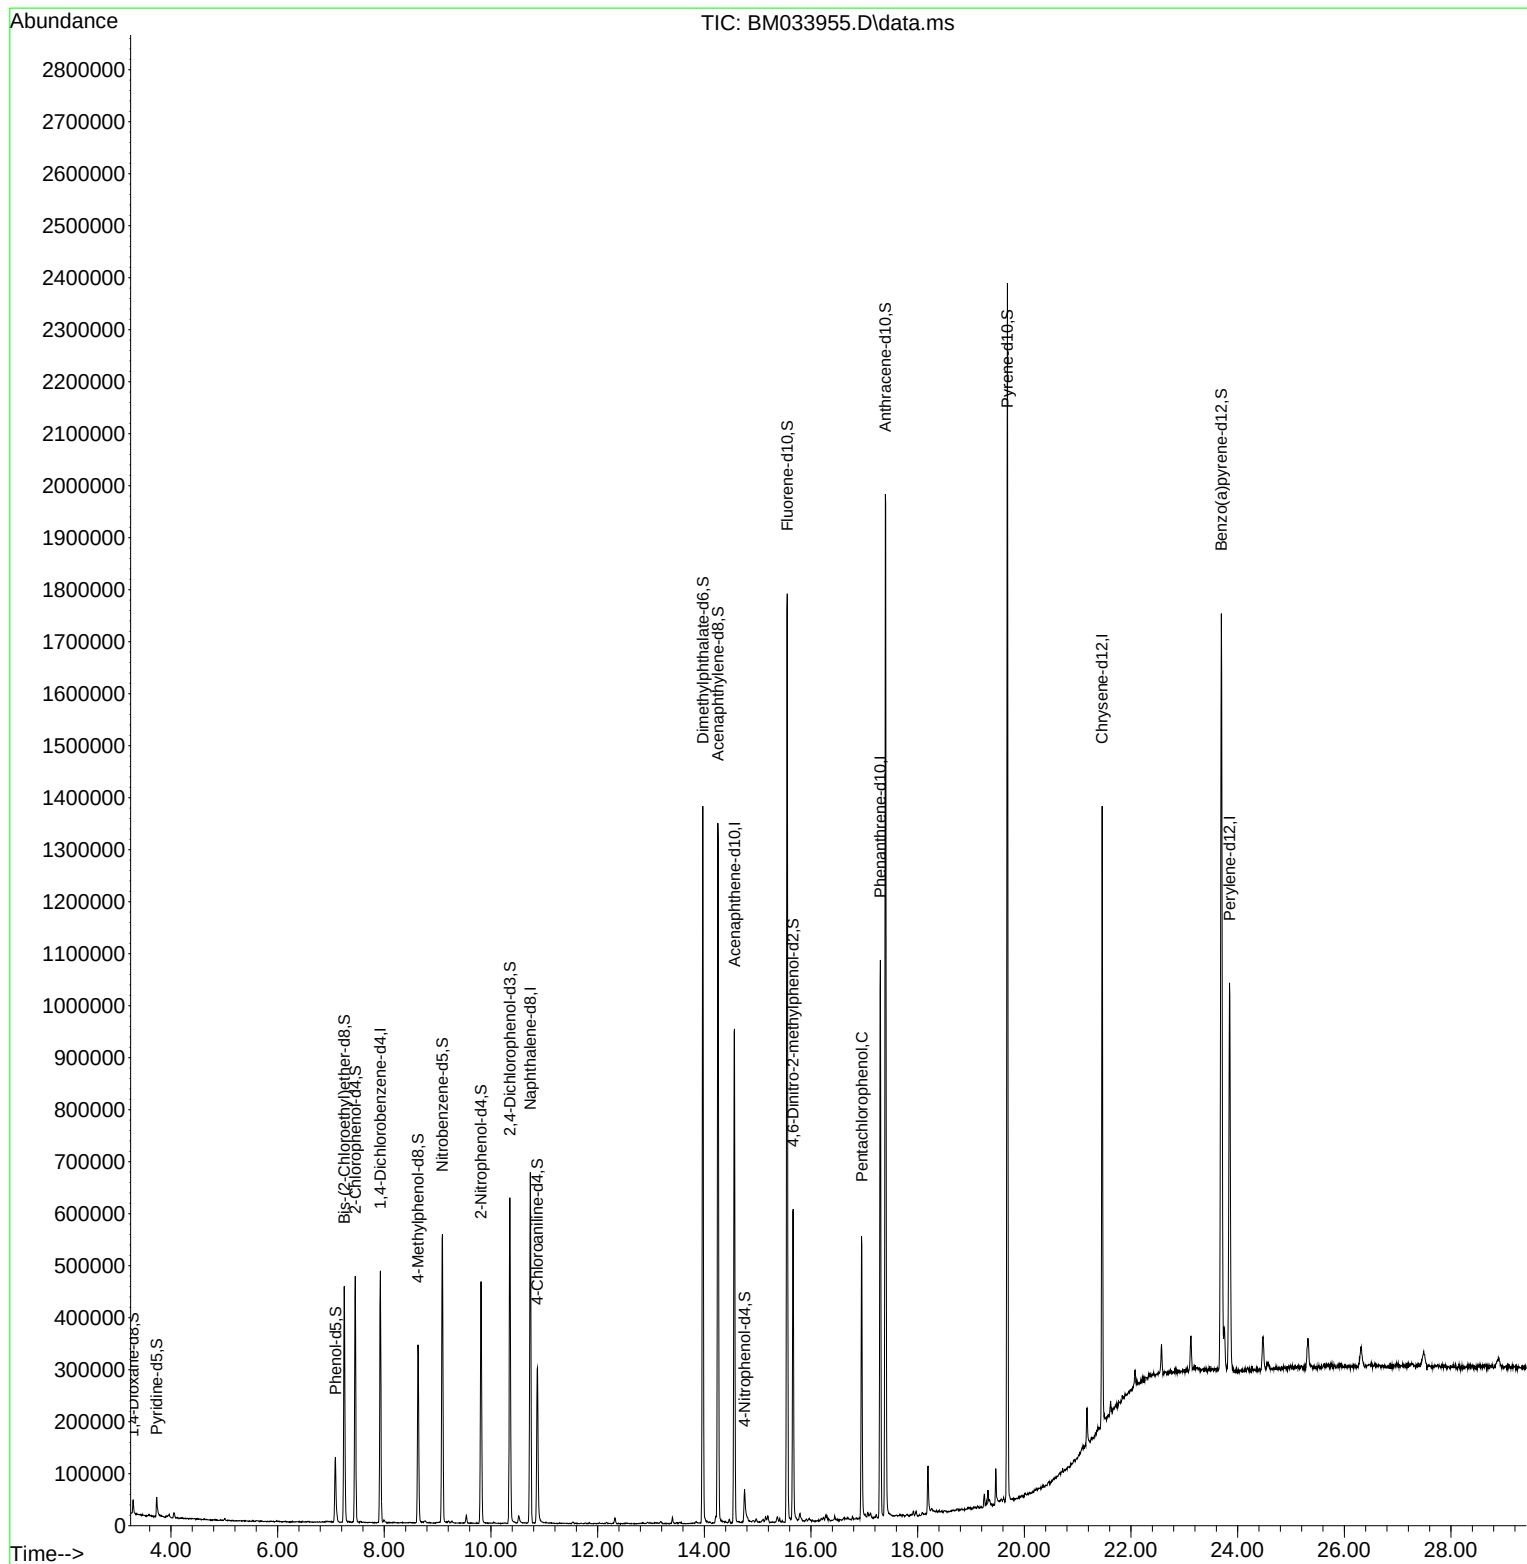

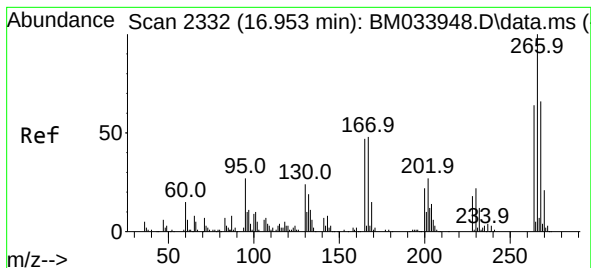

#71

Pentachlorophenol

Concen: 17.800 ng/ul

RT: 16.954 min Scan# 21

Delta R.T. -0.000 min

Lab File: BM033955.D


Acq: 02 Feb 2022 01:02

Instrument :

BNA_M

ClientSampleId :

C0Q04

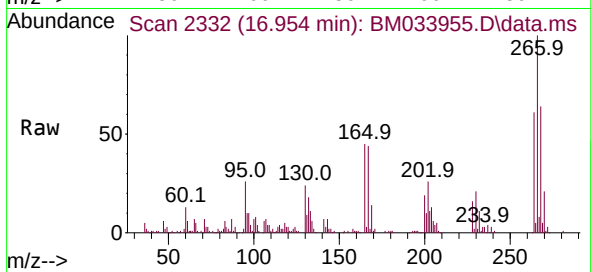

Tgt Ion:266 Resp: 84079

Ion Ratio Lower Upper

266 100

264 61.0 49.1 73.7

268 63.5 47.8 71.8

Manual Integrations

APPROVED

Reviewed By :Jagrut Upadhyay 02/02/2022

Supervised By :Yogesh Patel 02/04/2022

