

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020122\
 Data File : BM033961.D
 Acq On : 02 Feb 2022 04:36
 Operator : CG/JU
 Sample : N1307-03
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0Q31

Quant Time: Feb 02 05:59:54 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Feb 01 02:16:28 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.925	152	117396	20.000	ng/u1	0.00
20) Naphthalene-d8	10.736	136	535875	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.560	164	367367	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.301	188	782767	20.000	ng/u1	0.00
79) Chrysene-d12	21.459	240	691951	20.000	ng/u1	0.00
88) Perylene-d12	23.847	264	579186	20.000	ng/u1	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.284	96	12849	4.317	ng/uL	0.00
4) Pyridine-d5	3.719	84	62862	7.566	ng/u1	0.00
7) Phenol-d5	7.084	99	61507	6.254	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.248	67	179448	29.928	ng/u1	0.00
11) 2-Chlorophenol-d4	7.454	132	181313	23.010	ng/u1	0.00
15) 4-Methylphenol-d8	8.631	113	121452	15.584	ng/u1	-0.01
21) Nitrobenzene-d5	9.089	128	121265	28.202	ng/u1	0.00
24) 2-Nitrophenol-d4	9.813	143	127525	27.464	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.354	165	208724	24.840	ng/u1	0.00
31) 4-Chloroaniline-d4	10.866	131	283862	24.464	ng/u1	0.00
46) Dimethylphthalate-d6	13.971	166	880404	32.070	ng/u1	0.00
49) Acenaphthylene-d8	14.254	160	969759	28.837	ng/u1	0.00
54) 4-Nitrophenol-d4	14.754	143	24554	5.235	ng/u1	0.00
60) Fluorene-d10	15.554	176	713326	31.119	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.665	200	128333	26.115	ng/u1	0.00
73) Anthracene-d10	17.395	188	1181781	31.525	ng/u1	0.00
81) Pyrene-d10	19.683	212	1354881	33.166	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.694	264	964388	31.701	ng/u1	-0.01
Target Compounds						
					Qvalue	
8) Phenol	7.107	94	18497	1.834	ng/u1#	84


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020122\
Data File : BM033961.D
Acq On : 02 Feb 2022 04:36
Operator : CG/JU
Sample : N1307-03
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0Q31

Quant Time: Feb 02 05:59:54 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Feb 01 02:16:28 2022
Response via : Initial Calibration

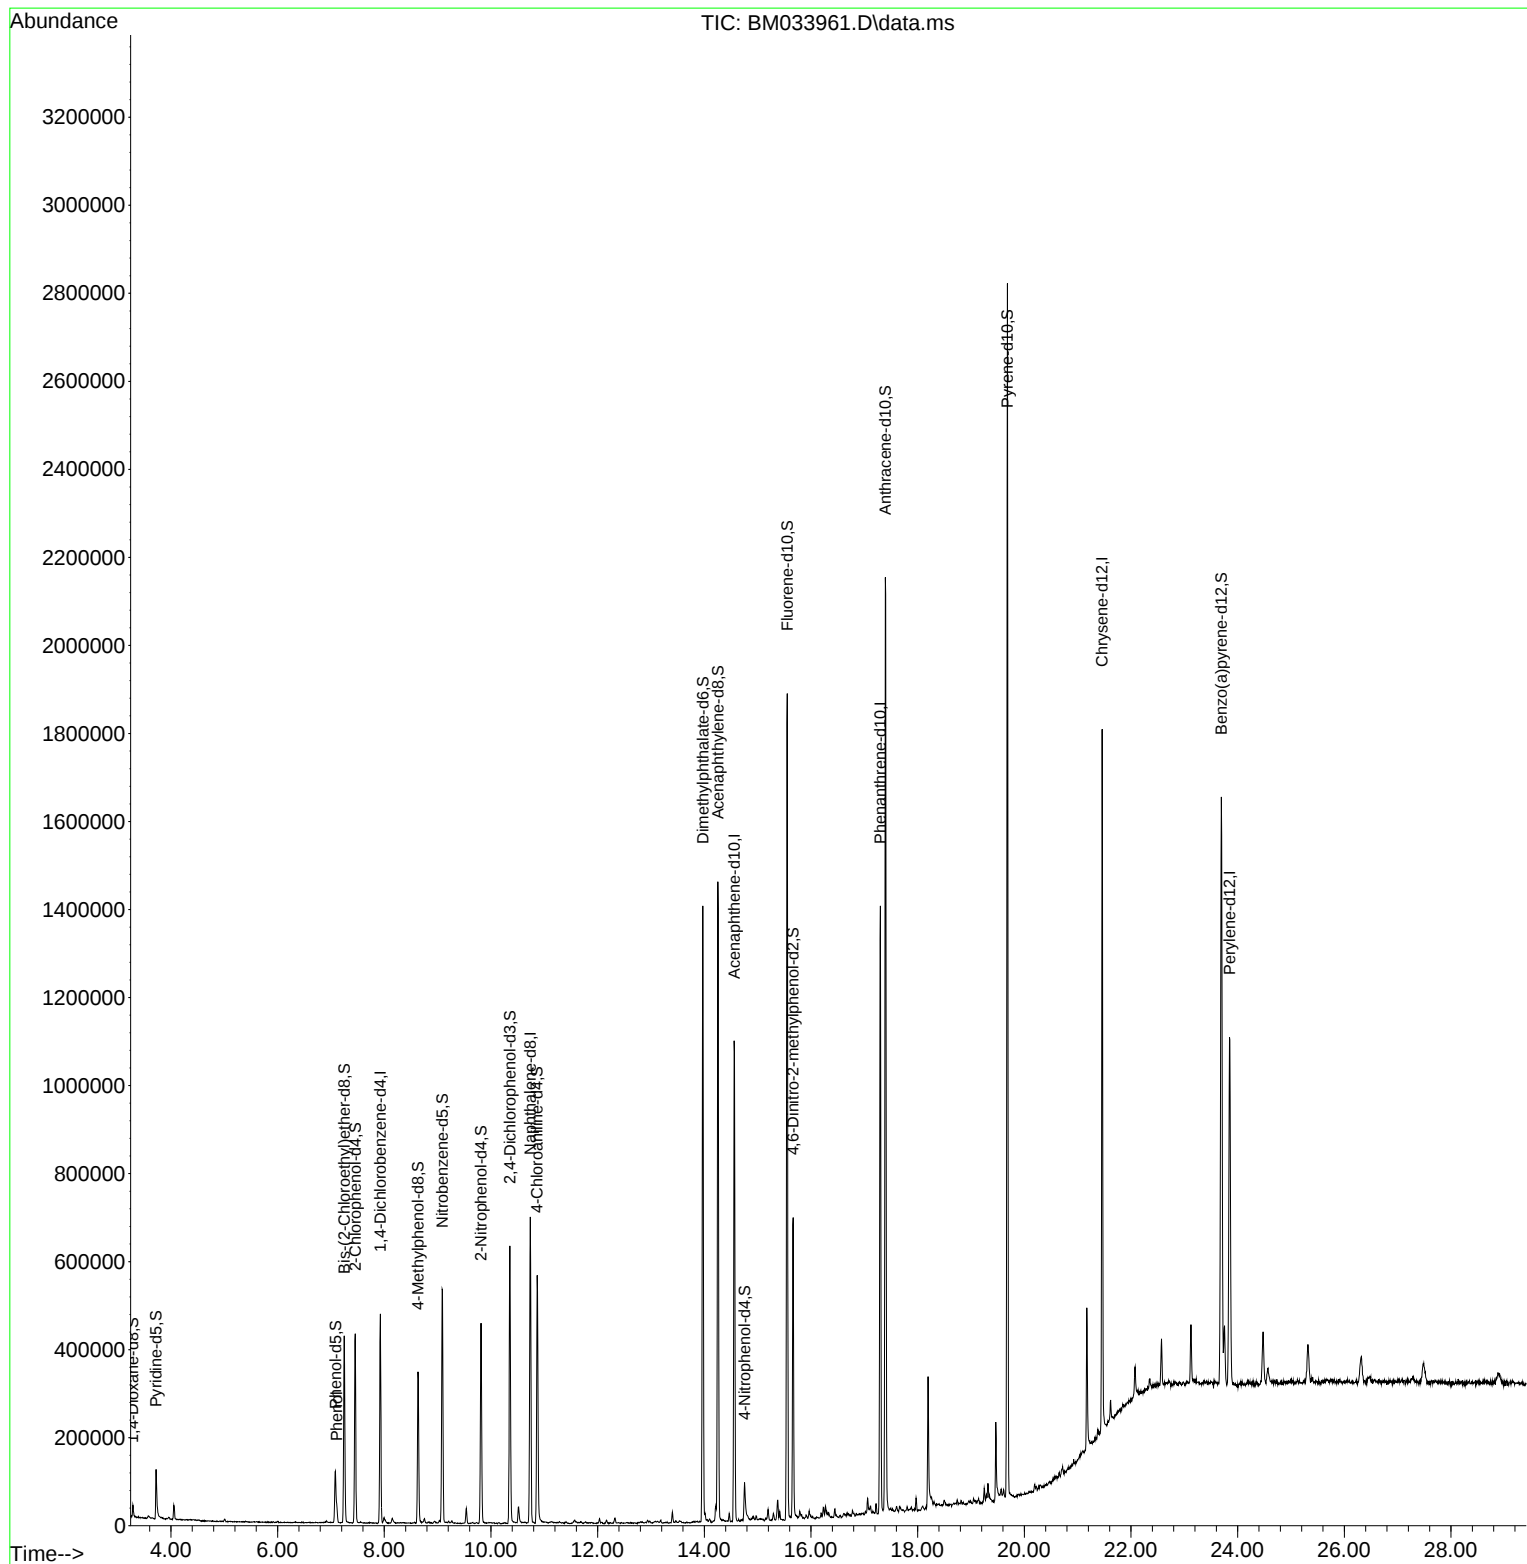

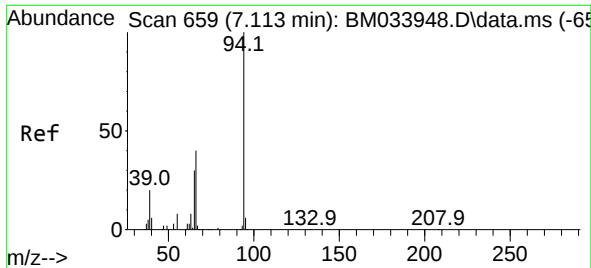

#8
Phenol
Concen: 1.834 ng/ul
RT: 7.107 min Scan# 61
Delta R.T. -0.006 min
Lab File: BM033961.D
Acq: 02 Feb 2022 04:36

Instrument :
BNA_M
ClientSampleId :
C0Q31

Tgt Ion: 94 Resp: 18497
Ion Ratio Lower Upper
94 100
65 28.5 31.7 47.5#
66 45.9 45.4 68.0

