

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020122\
 Data File : BM033968.D
 Acq On : 02 Feb 2022 10:55
 Operator : CG/JU
 Sample : N1273-17DL 5X
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0HL5DL

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 02/03/2022
 Supervised By :Yogesh Patel 02/04/2022

Quant Time: Feb 02 15:23:21 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Feb 01 02:16:28 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.925	152	115964	20.000	ng/u1	0.00
20) Naphthalene-d8	10.736	136	508896	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.560	164	361762	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.295	188	778583	20.000	ng/u1	-0.01
79) Chrysene-d12	21.459	240	615649	20.000	ng/u1	0.00
88) Perylene-d12	23.847	264	542014	20.000	ng/u1	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.354	96	313	0.106	ng/uL	0.06
4) Pyridine-d5	3.713	84	142	0.017	ng/u1	0.00
7) Phenol-d5	7.084	99	14033	1.444	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.248	67	54069	9.129	ng/u1	0.00
11) 2-Chlorophenol-d4	7.454	132	50885	6.538	ng/u1	0.00
15) 4-Methylphenol-d8	8.631	113	27729	3.602	ng/u1	-0.01
21) Nitrobenzene-d5	9.089	128	32807	8.034	ng/u1	0.00
24) 2-Nitrophenol-d4	9.813	143	31954	7.246	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.354	165	52723	6.607	ng/u1	0.00
31) 4-Chloroaniline-d4	10.872	131	11471	1.041	ng/u1	0.00
46) Dimethylphthalate-d6	13.971	166	262313	9.703	ng/u1	0.00
49) Acenaphthylene-d8	14.254	160	257850	7.786	ng/u1	0.00
54) 4-Nitrophenol-d4	14.771	143	2054	0.445	ng/u1	0.02
60) Fluorene-d10	15.548	176	214555	9.505	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.665	200	29272	5.989	ng/u1	0.00
73) Anthracene-d10	17.395	188	365762	9.810	ng/u1	0.00
81) Pyrene-d10	19.677	212	405184	11.148	ng/u1	-0.01
92) Benzo(a)pyrene-d12	23.694	264	284041	9.977	ng/u1	-0.01
Target Compounds						
2) 1,4-Dioxane	3.325	88	44306	13.808	ng/uL#	87

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020122\
Data File : BM033968.D
Acq On : 02 Feb 2022 10:55
Operator : CG/JU
Sample : N1273-17DL 5X
Misc :
ALS Vial : 39 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
C0HL5DL

Quant Time: Feb 02 15:23:21 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Feb 01 02:16:28 2022
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 02/03/2022
Supervised By :Yogesh Patel 02/04/2022

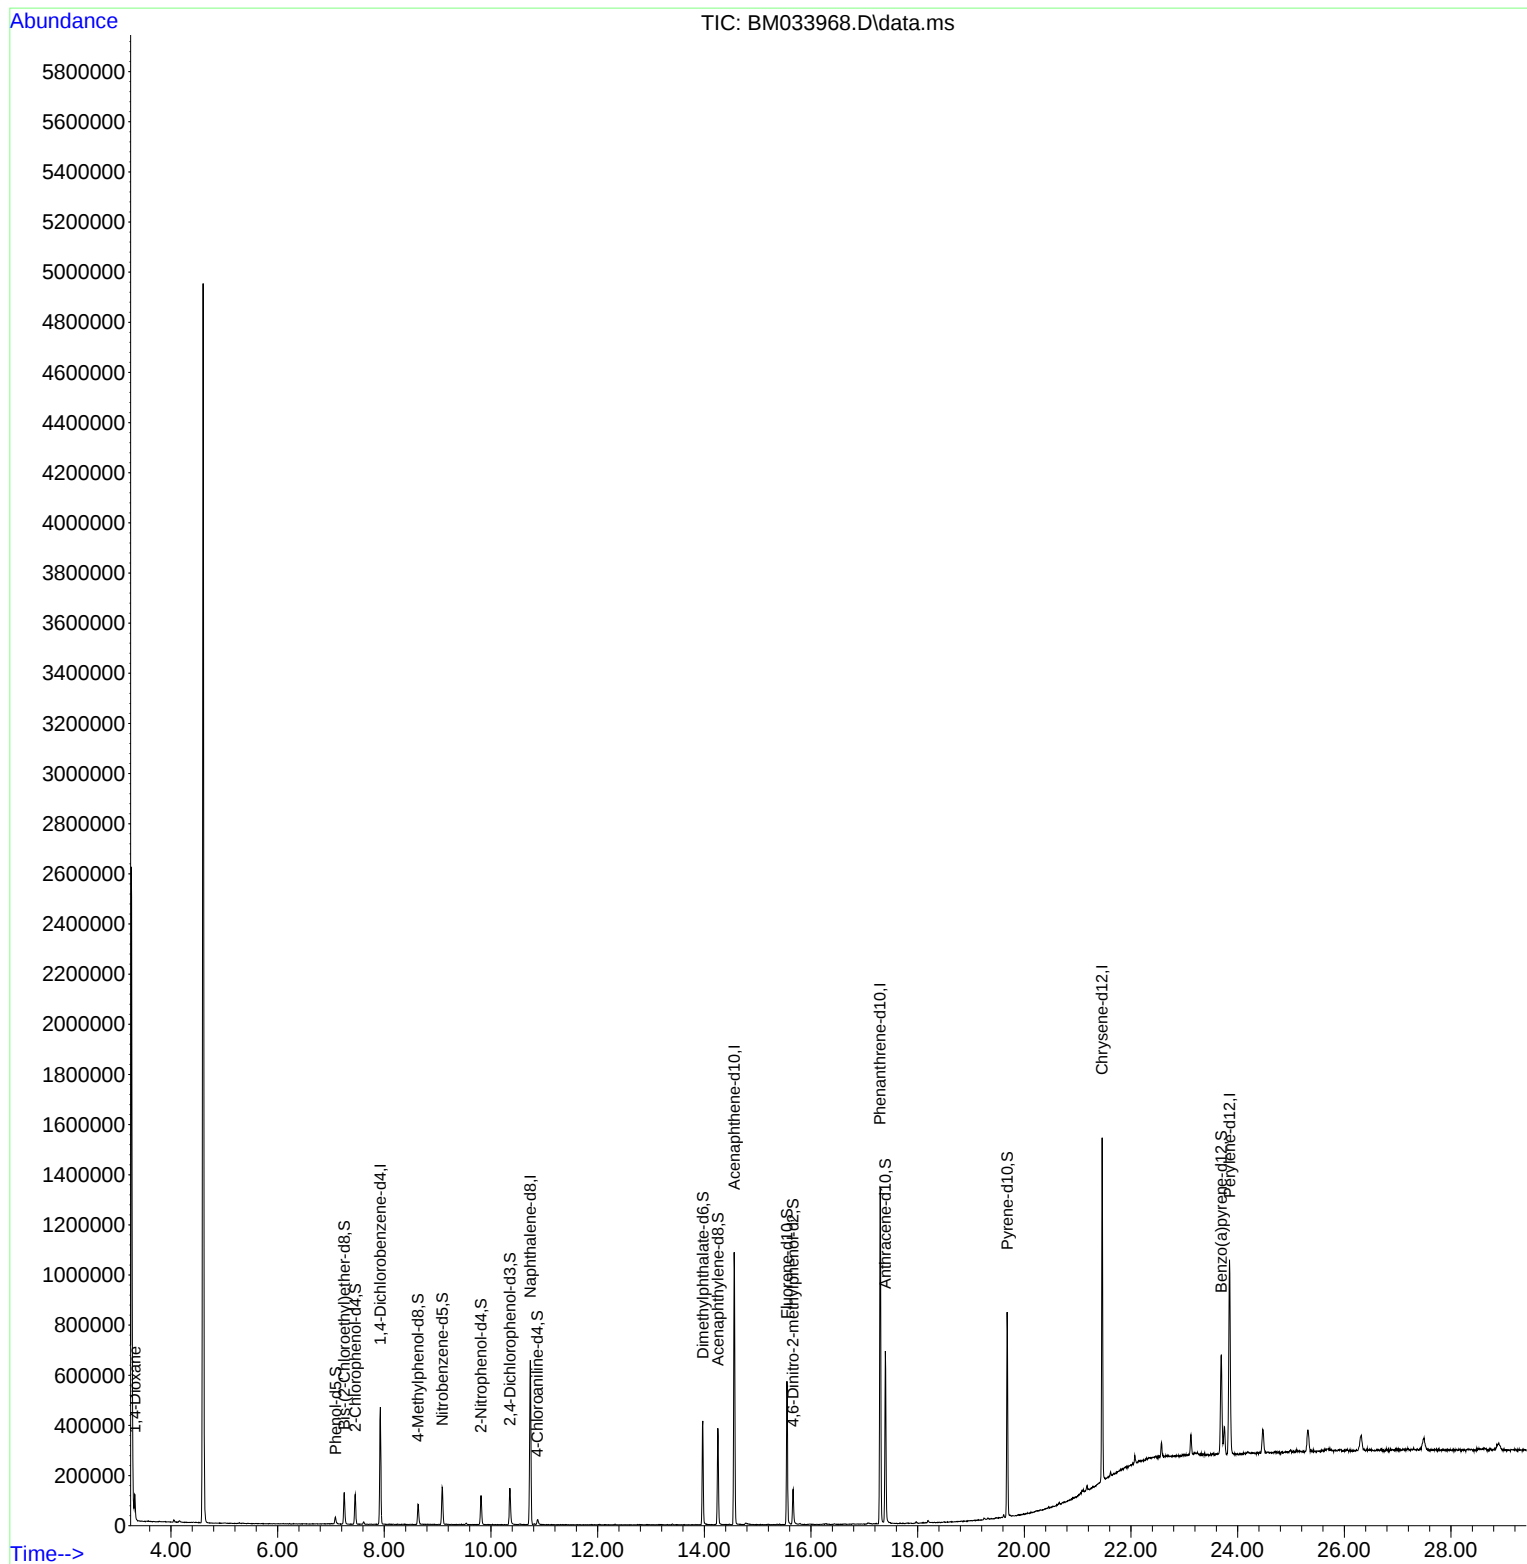

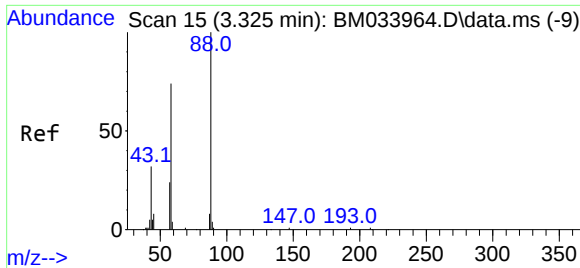

#2
 1,4-Dioxane
 Concen: 13.808 ng/uL
 RT: 3.325 min Scan# 11
 Delta R.T. 0.000 min
 Lab File: BM033968.D
 Acq: 02 Feb 2022 10:55

Instrument :
 BNA_M
 ClientSampleId :
 C0HL5DL

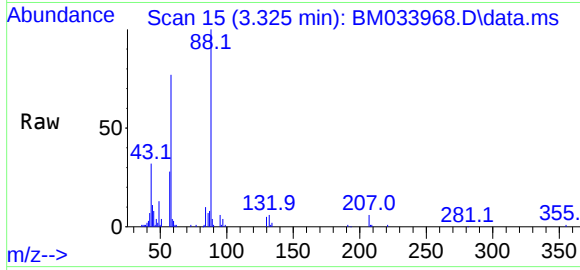

Tgt Ion: 88 Resp: 44300
 Ion Ratio Lower Upper
 88 100
 43 31.9 36.2 54.4
 58 77.2 68.5 102.7

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 02/03/2022
 Supervised By :Yogesh Patel 02/04/2022

