

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020122\
 Data File : BM033980.D
 Acq On : 02 Feb 2022 19:01
 Operator : CG/JU
 Sample : N1355-04
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 COVE5

Quant Time: Feb 03 00:14:25 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Feb 01 02:16:28 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.925	152	120214	20.000	ng/u1	0.00
20) Naphthalene-d8	10.736	136	533591	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.560	164	367691	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.295	188	723951	20.000	ng/u1	-0.01
79) Chrysene-d12	21.459	240	525619	20.000	ng/u1	0.00
88) Perylene-d12	23.847	264	483128	20.000	ng/u1	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.290	96	15309	5.022	ng/uL	0.00
4) Pyridine-d5	3.719	84	96859	11.385	ng/u1	0.00
7) Phenol-d5	7.078	99	267858	26.597	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.248	67	168532	27.448	ng/u1	0.00
11) 2-Chlorophenol-d4	7.454	132	217313	26.933	ng/u1	0.00
15) 4-Methylphenol-d8	8.631	113	225603	28.270	ng/u1	-0.01
21) Nitrobenzene-d5	9.084	128	110653	25.844	ng/u1	-0.01
24) 2-Nitrophenol-d4	9.813	143	121998	26.386	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.354	165	216486	25.874	ng/u1	0.00
31) 4-Chloroaniline-d4	10.866	131	295108	25.542	ng/u1	0.00
46) Dimethylphthalate-d6	13.972	166	771932	28.094	ng/u1	0.00
49) Acenaphthylene-d8	14.254	160	896433	26.633	ng/u1	0.00
54) 4-Nitrophenol-d4	14.748	143	95955	20.441	ng/u1	0.00
60) Fluorene-d10	15.548	176	630141	27.466	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.660	200	93783	20.635	ng/u1	-0.01
73) Anthracene-d10	17.395	188	939855	27.109	ng/u1	0.00
81) Pyrene-d10	19.677	212	956110	30.811	ng/u1	-0.01
92) Benzo(a)pyrene-d12	23.694	264	694603	27.373	ng/u1	-0.01
Target Compounds						
					Qvalue	
8) Phenol	7.107	94	15241	1.476	ng/u1	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020122\
Data File : BM033980.D
Acq On : 02 Feb 2022 19:01
Operator : CG/JU
Sample : N1355-04
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
COVE5

Quant Time: Feb 03 00:14:25 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Feb 01 02:16:28 2022
Response via : Initial Calibration

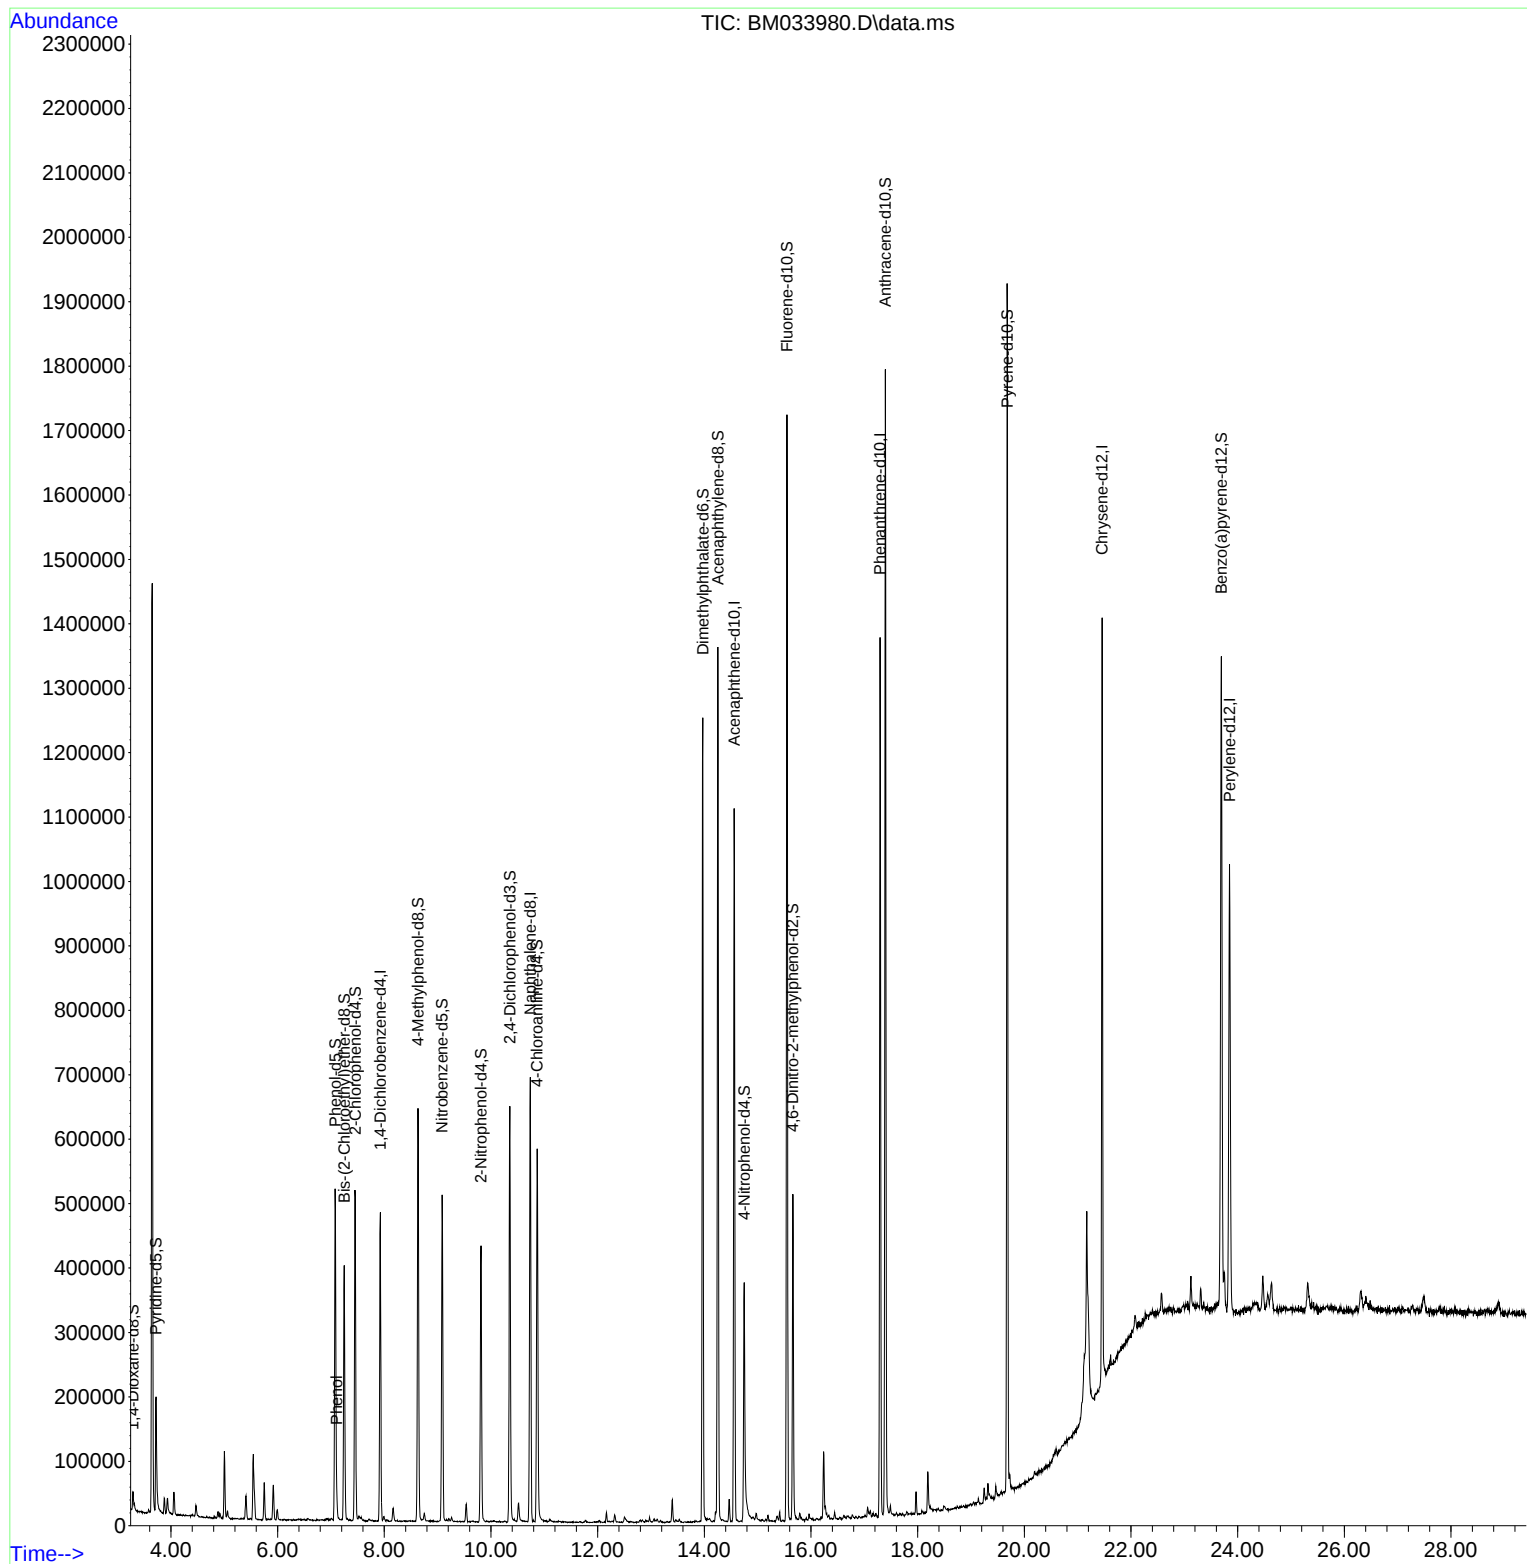

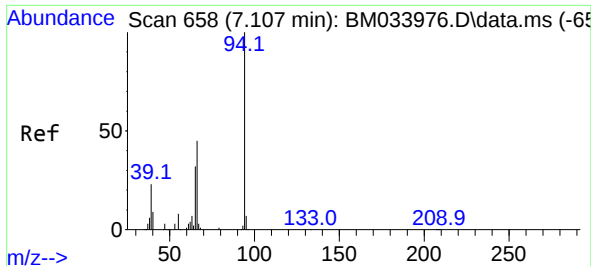

#8
Phenol
Concen: 1.476 ng/ul
RT: 7.107 min Scan# 61
Delta R.T. -0.006 min
Lab File: BM033980.D
Acq: 02 Feb 2022 19:01

Instrument :
BNA_M
ClientSampleId :
COVE5

Tgt Ion: 94 Resp: 15241
Ion Ratio Lower Upper
94 100
65 33.7 31.7 47.5
66 51.1 45.4 68.0

