

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020122\
 Data File : BM033981.D
 Acq On : 02 Feb 2022 19:37
 Operator : CG/JU
 Sample : N1355-05
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 COVE6

Quant Time: Feb 03 00:14:40 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Feb 01 02:16:28 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.925	152	116364	20.000	ng/ul	0.00
20) Naphthalene-d8	10.736	136	506491	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.560	164	332531	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.295	188	627884	20.000	ng/ul	-0.01
79) Chrysene-d12	21.459	240	477372	20.000	ng/ul	0.00
88) Perylene-d12	23.847	264	464709	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.290	96	15545	5.269	ng/uL	0.00
4) Pyridine-d5	3.725	84	59331	7.204	ng/ul	0.00
7) Phenol-d5	7.084	99	309766	31.775	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.248	67	185622	31.232	ng/ul	0.00
11) 2-Chlorophenol-d4	7.454	132	248306	31.792	ng/ul	0.00
15) 4-Methylphenol-d8	8.631	113	253801	32.855	ng/ul	-0.01
21) Nitrobenzene-d5	9.083	128	122698	30.191	ng/ul	-0.01
24) 2-Nitrophenol-d4	9.813	143	140482	32.010	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.354	165	247548	31.170	ng/ul	0.00
31) 4-Chloroaniline-d4	10.866	131	235668	21.488	ng/ul	0.00
46) Dimethylphthalate-d6	13.971	166	794241	31.963	ng/ul	0.00
49) Acenaphthylene-d8	14.254	160	935762	30.741	ng/ul	0.00
54) 4-Nitrophenol-d4	14.748	143	108537	25.566	ng/ul	0.00
60) Fluorene-d10	15.548	176	645795	31.124	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.660	200	101159	25.663	ng/ul	-0.01
73) Anthracene-d10	17.395	188	911439	30.311	ng/ul	0.00
81) Pyrene-d10	19.677	212	930900	33.030	ng/ul	-0.01
92) Benzo(a)pyrene-d12	23.694	264	734404	30.088	ng/ul	-0.01
Target Compounds					Qvalue	
8) Phenol	7.107	94	17194	1.720	ng/ul#	87
16) Acetophenone	8.748	105	35506	2.895	ng/ul#	88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020122\
Data File : BM033981.D
Acq On : 02 Feb 2022 19:37
Operator : CG/JU
Sample : N1355-05
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
COVE6

Quant Time: Feb 03 00:14:40 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Feb 01 02:16:28 2022
Response via : Initial Calibration




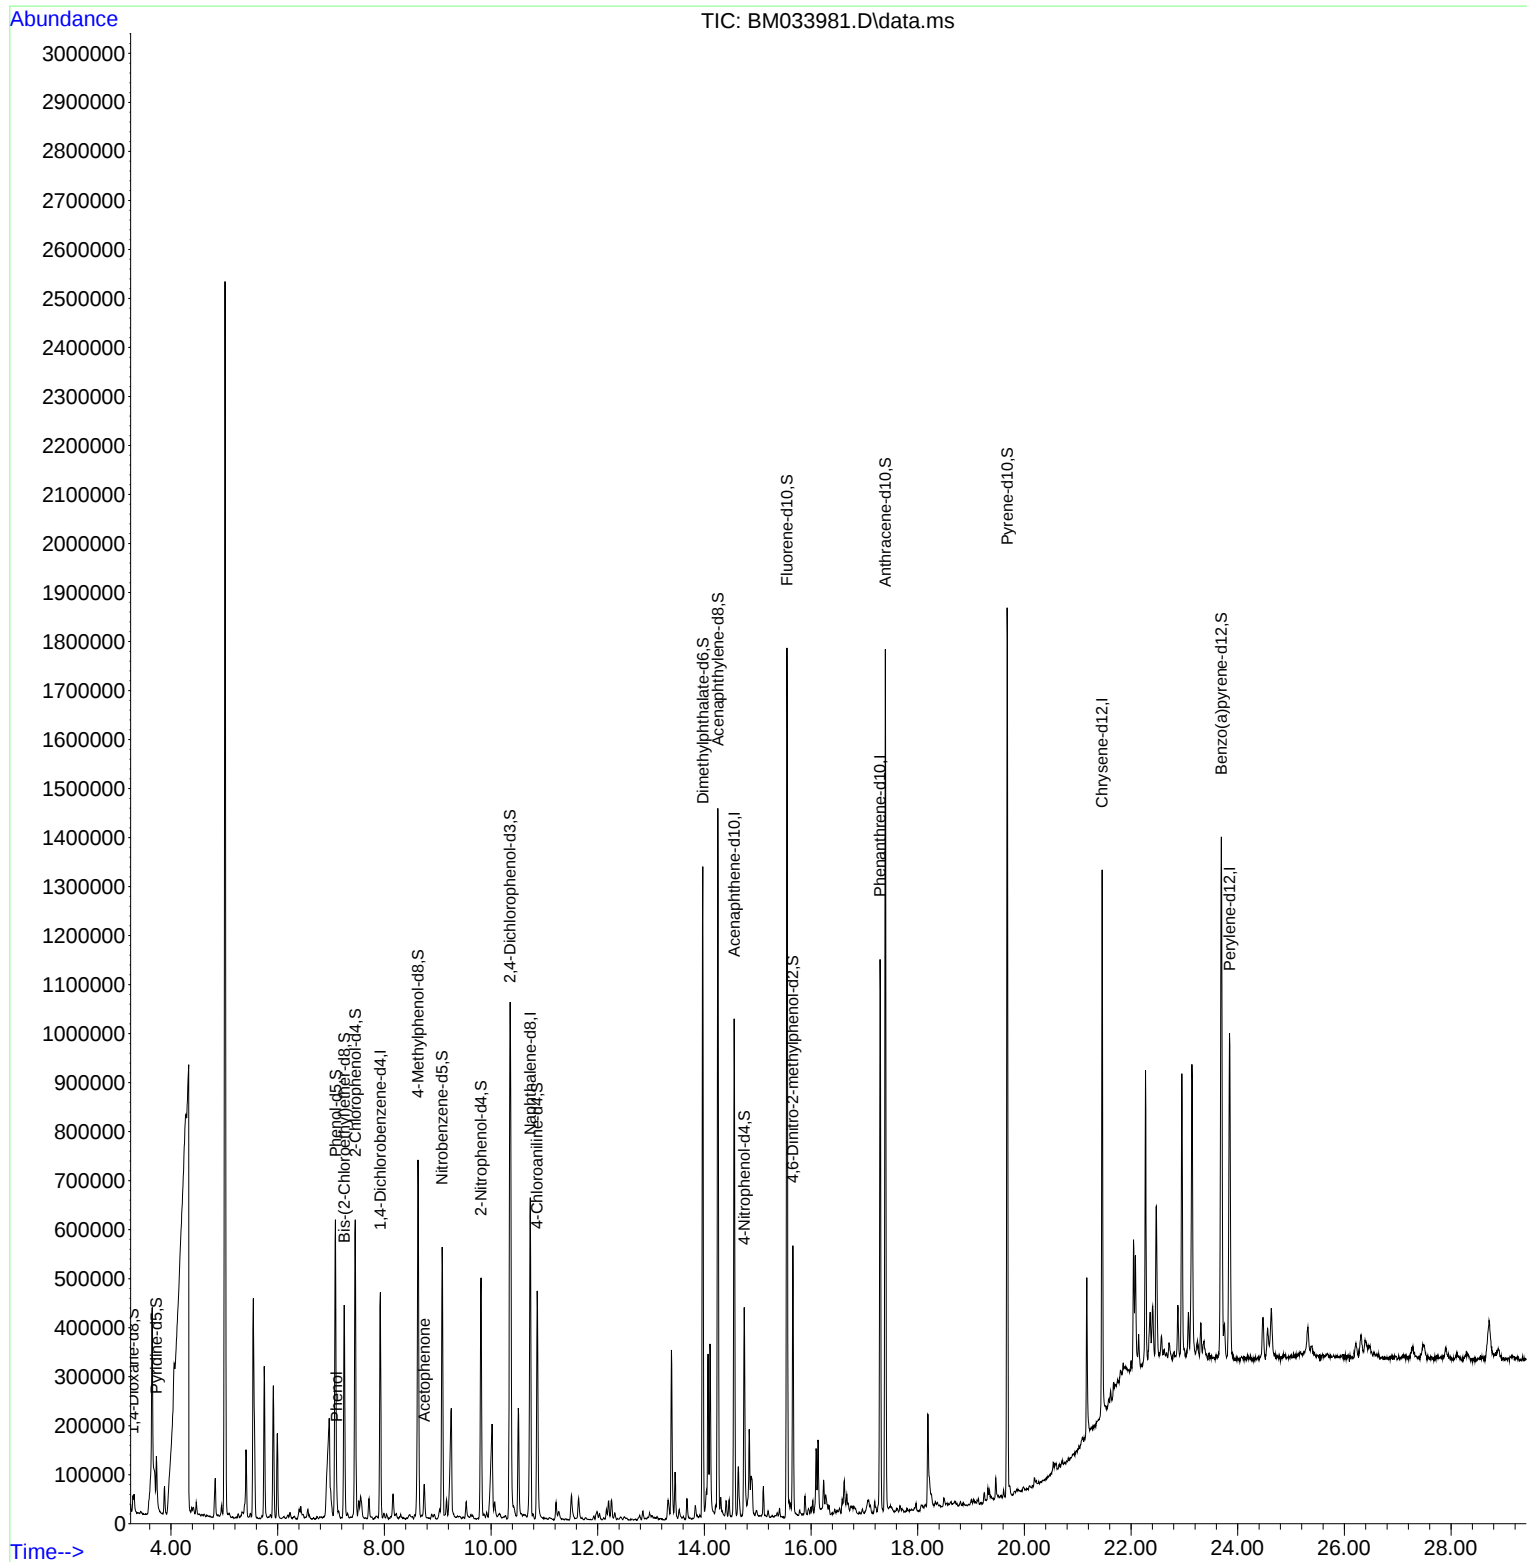


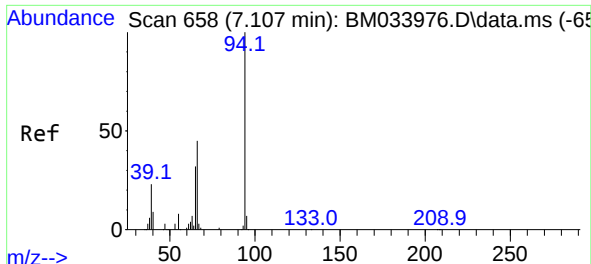

#8
Phenol
Concen: 1.720 ng/ul
RT: 7.107 min Scan# 61
Delta R.T. -0.006 min
Lab File: BM033981.D
Acq: 02 Feb 2022 19:37

Instrument :
BNA_M
ClientSampleId :
COVE6

Tgt Ion: 94 Resp: 17194
Ion Ratio Lower Upper
94 100
65 31.4 31.7 47.5#
66 47.6 45.4 68.0

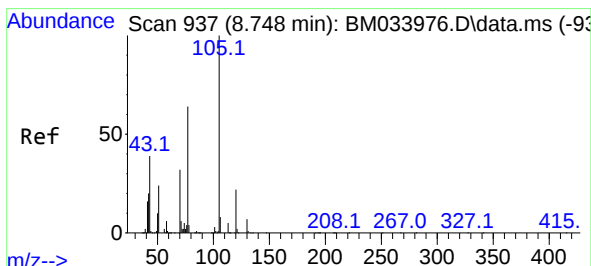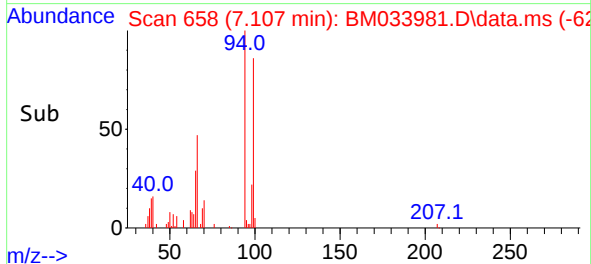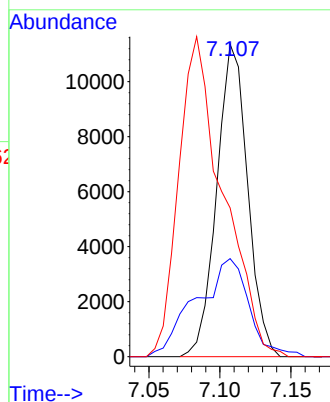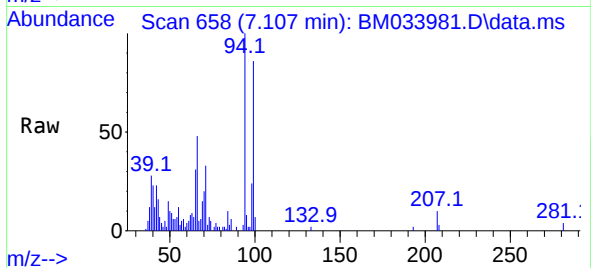

#16
Acetophenone
Concen: 2.895 ng/ul
RT: 8.748 min Scan# 937
Delta R.T. -0.006 min
Lab File: BM033981.D
Acq: 02 Feb 2022 19:37

Tgt Ion: 105 Resp: 35506
Ion Ratio Lower Upper
105 100
77 80.8 73.1 109.7
51 30.3 30.5 45.7#

