

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020122\
 Data File : BM033982.D
 Acq On : 02 Feb 2022 20:13
 Operator : CG/JU
 Sample : N1355-06
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 COVE8

Quant Time: Feb 03 00:14:57 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Feb 01 02:16:28 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.925	152	130874	20.000	ng/u1	0.00
20) Naphthalene-d8	10.736	136	565480	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.560	164	349358	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.295	188	606587	20.000	ng/u1	-0.01
79) Chrysene-d12	21.459	240	472232	20.000	ng/u1	0.00
88) Perylene-d12	23.853	264	487633	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.290	96	14152	4.265	ng/uL	0.00
4) Pyridine-d5	3.725	84	30279	3.269	ng/u1	0.00
7) Phenol-d5	7.084	99	293955	26.810	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.248	67	170418	25.495	ng/u1	0.00
11) 2-Chlorophenol-d4	7.454	132	235780	26.841	ng/u1	0.00
15) 4-Methylphenol-d8	8.631	113	237838	27.375	ng/u1	-0.01
21) Nitrobenzene-d5	9.084	128	113277	24.965	ng/u1	-0.01
24) 2-Nitrophenol-d4	9.813	143	127639	26.049	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.354	165	225869	25.473	ng/u1	0.00
31) 4-Chloroaniline-d4	10.866	131	214828	17.545	ng/u1	0.00
46) Dimethylphthalate-d6	13.971	166	640089	24.518	ng/u1	0.00
49) Acenaphthylene-d8	14.254	160	790709	24.725	ng/u1	0.00
54) 4-Nitrophenol-d4	14.748	143	74799	16.770	ng/u1	0.00
60) Fluorene-d10	15.548	176	528528	24.246	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.660	200	72096	18.932	ng/u1	-0.01
73) Anthracene-d10	17.395	188	700989	24.131	ng/u1	0.00
81) Pyrene-d10	19.677	212	708946	25.429	ng/u1	-0.01
92) Benzo(a)pyrene-d12	23.694	264	612764	23.924	ng/u1	-0.01
Target Compounds						
					Qvalue	
8) Phenol	7.107	94	16648	1.481	ng/u1	88
16) Acetophenone	8.748	105	41629	3.018	ng/u1#	78


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020122\
Data File : BM033982.D
Acq On : 02 Feb 2022 20:13
Operator : CG/JU
Sample : N1355-06
Misc :
ALS Vial : 53 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
COVE8

Quant Time: Feb 03 00:14:57 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Feb 01 02:16:28 2022
Response via : Initial Calibration




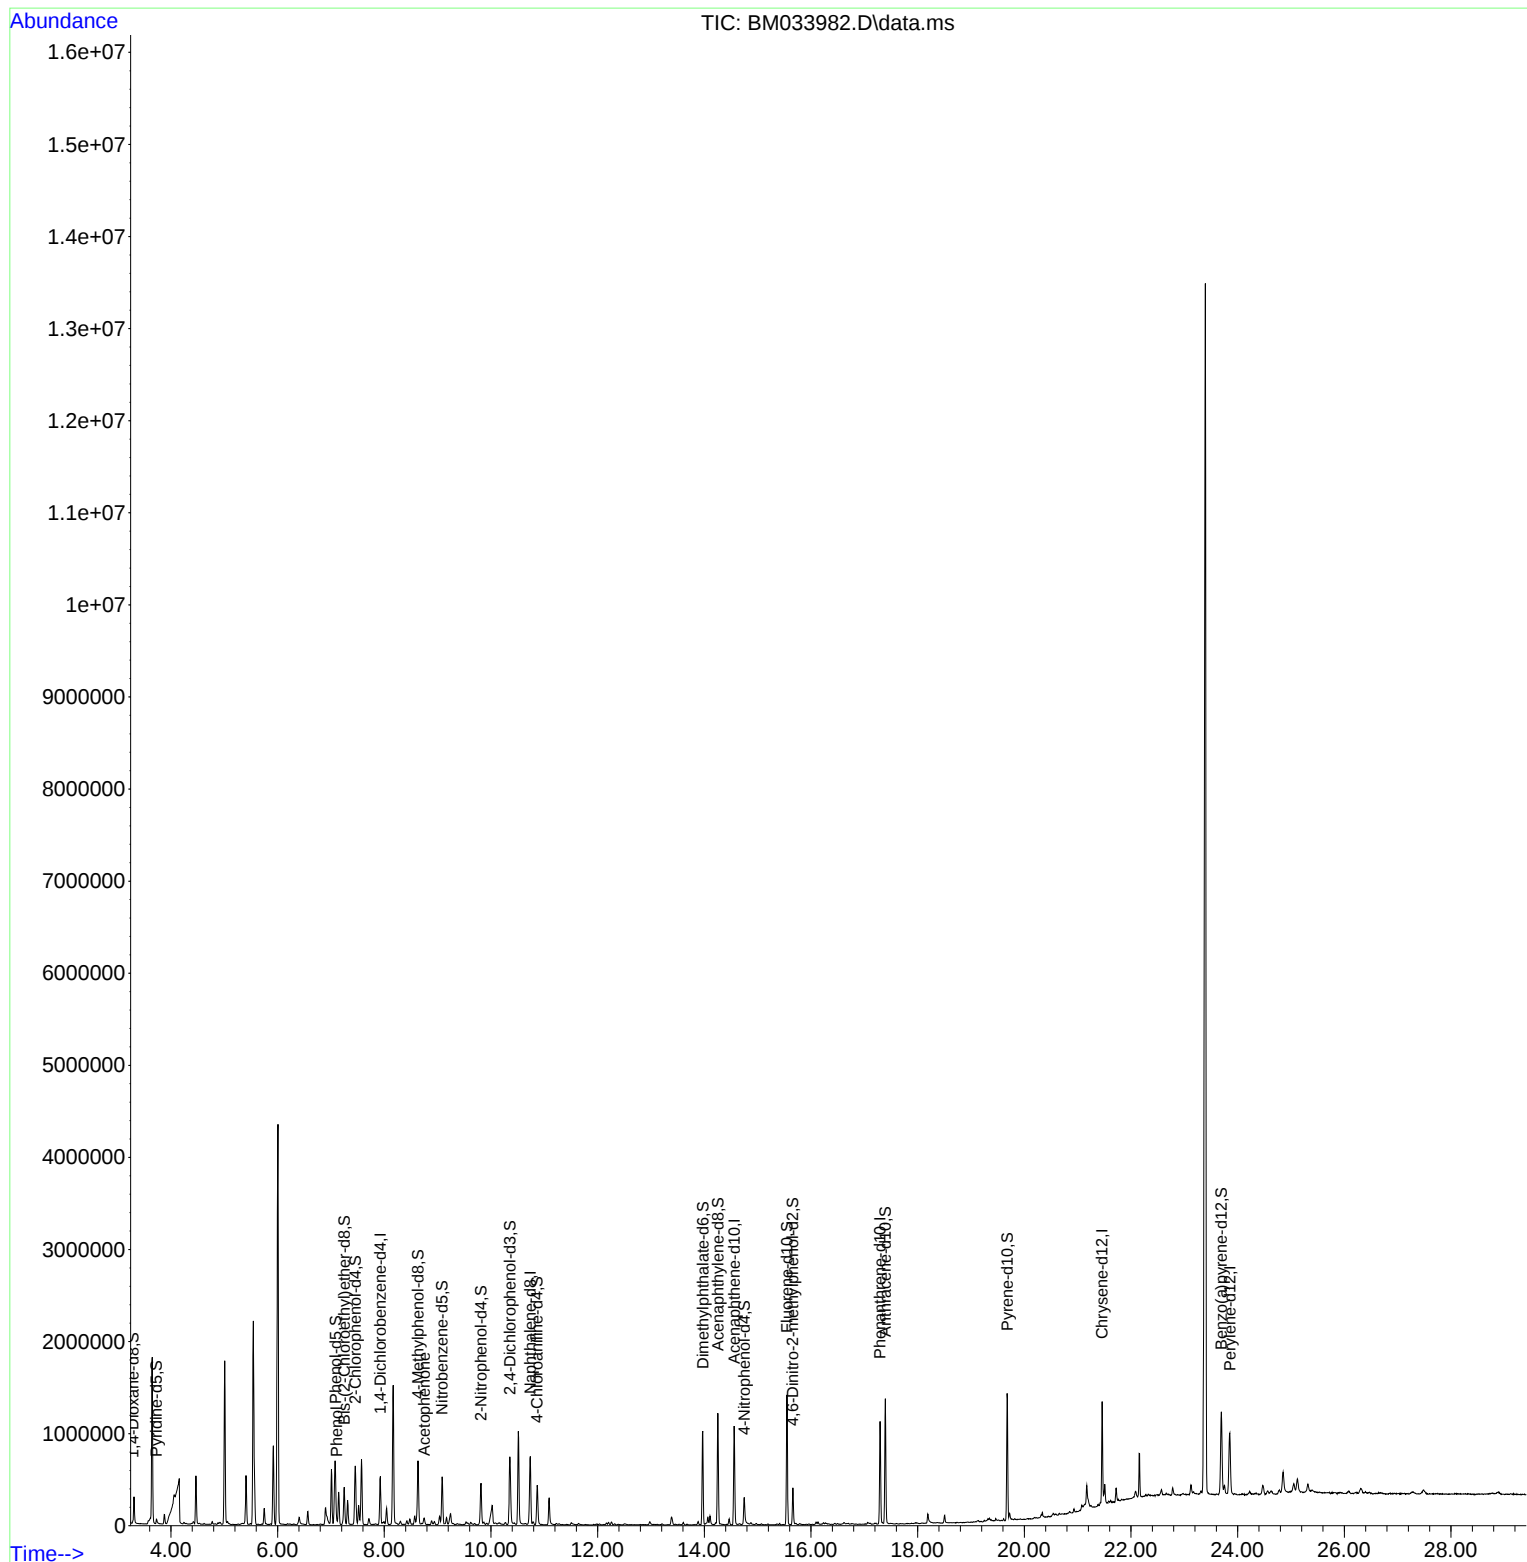


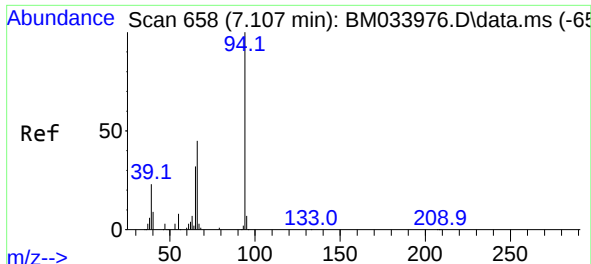

#8
Phenol
Concen: 1.481 ng/ul
RT: 7.107 min Scan# 658
Delta R.T. -0.006 min
Lab File: BM033982.D
Acq: 02 Feb 2022 20:13

Instrument :
BNA_M
ClientSampleId :
COVE8

Tgt Ion: 94 Resp: 16648
Ion Ratio Lower Upper
94 100
65 31.7 31.7 47.5
66 48.3 45.4 68.0

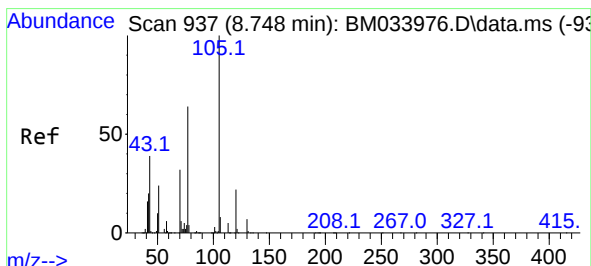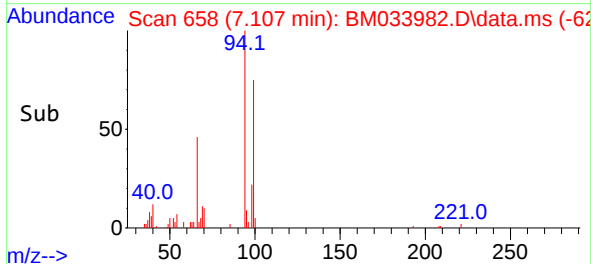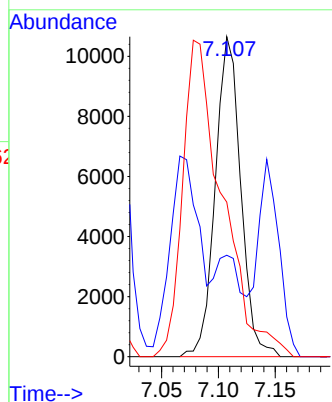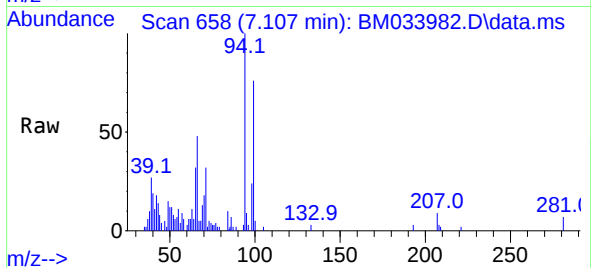

#16
Acetophenone
Concen: 3.018 ng/ul
RT: 8.748 min Scan# 937
Delta R.T. -0.006 min
Lab File: BM033982.D
Acq: 02 Feb 2022 20:13

Tgt Ion: 105 Resp: 41629
Ion Ratio Lower Upper
105 100
77 68.7 73.1 109.7#
51 26.9 30.5 45.7#

