

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020122\
 Data File : BM033983.D
 Acq On : 02 Feb 2022 20:48
 Operator : CG/JU
 Sample : N1355-08
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 COVF2

Quant Time: Feb 03 00:15:16 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Feb 01 02:16:28 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.925	152	116510	20.000	ng/ul	0.00
20) Naphthalene-d8	10.736	136	532821	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.560	164	372218	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.295	188	749866	20.000	ng/ul	-0.01
79) Chrysene-d12	21.459	240	535936	20.000	ng/ul	0.00
88) Perylene-d12	23.847	264	487766	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.284	96	10851	3.673	ng/uL	0.00
4) Pyridine-d5	3.725	84	19865	2.409	ng/ul	0.00
7) Phenol-d5	7.078	99	235019	24.078	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.248	67	146081	24.548	ng/ul	0.00
11) 2-Chlorophenol-d4	7.448	132	188780	24.140	ng/ul	-0.01
15) 4-Methylphenol-d8	8.631	113	197101	25.483	ng/ul	-0.01
21) Nitrobenzene-d5	9.084	128	98358	23.006	ng/ul	-0.01
24) 2-Nitrophenol-d4	9.813	143	106575	23.084	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.348	165	196378	23.505	ng/ul	-0.01
31) 4-Chloroaniline-d4	10.866	131	179005	15.515	ng/ul	0.00
46) Dimethylphthalate-d6	13.972	166	697874	25.090	ng/ul	0.00
49) Acenaphthylene-d8	14.254	160	807785	23.707	ng/ul	0.00
54) 4-Nitrophenol-d4	14.748	143	90140	18.969	ng/ul	0.00
60) Fluorene-d10	15.548	176	587071	25.277	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.660	200	84738	18.000	ng/ul	-0.01
73) Anthracene-d10	17.395	188	891550	24.827	ng/ul	0.00
81) Pyrene-d10	19.677	212	888275	28.074	ng/ul	-0.01
92) Benzo(a)pyrene-d12	23.694	264	623327	24.330	ng/ul	-0.01
Target Compounds						
					Qvalue	
8) Phenol	7.107	94	13809	1.380	ng/ul	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020122\
Data File : BM033983.D
Acq On : 02 Feb 2022 20:48
Operator : CG/JU
Sample : N1355-08
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
COVF2


Quant Time: Feb 03 00:15:16 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Feb 01 02:16:28 2022
Response via : Initial Calibration

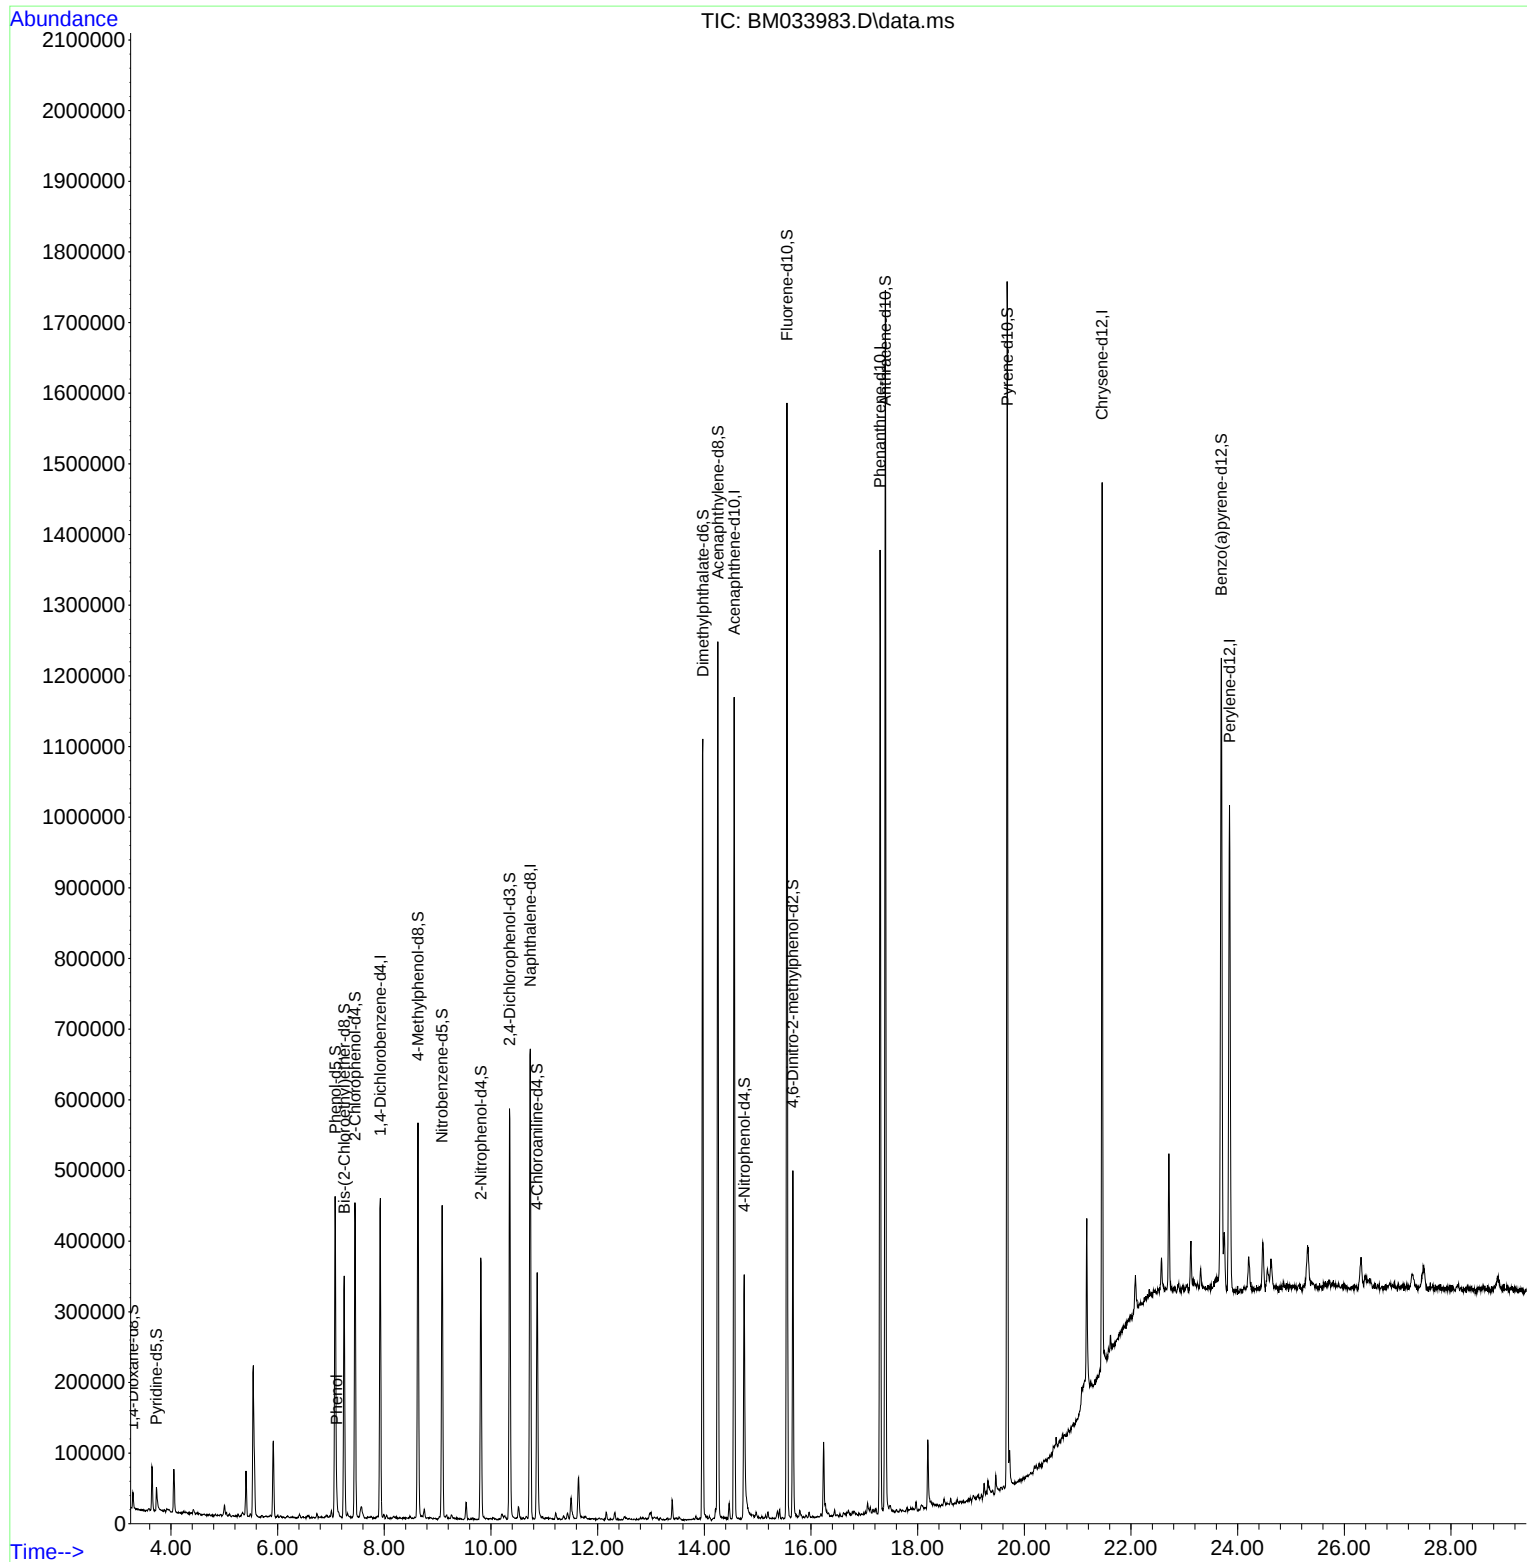

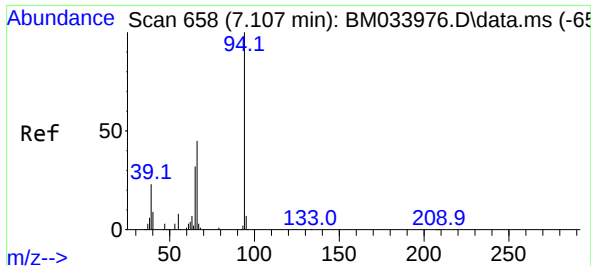

#8
Phenol
Concen: 1.380 ng/ul
RT: 7.107 min Scan# 61
Delta R.T. -0.006 min
Lab File: BM033983.D
Acq: 02 Feb 2022 20:48

Instrument :
BNA_M
ClientSampleId :
C0VF2

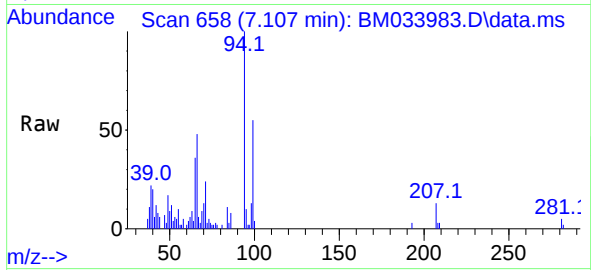

Tgt Ion: 94 Resp: 13809

Ion	Ratio	Lower	Upper
94	100		
65	36.0	31.7	47.5
66	48.5	45.4	68.0

