

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020122\
 Data File : BM033933.D
 Acq On : 01 Feb 2022 10:59
 Operator : CG/JU
 Sample : PB142371BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK371

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
 Title : SVOA CALIBRATION

Signal : TIC: BM033933.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.290	4	9	17	rVB	35282	49966	1.79%	0.164%
2	3.713	77	81	98	rBV	425073	656930	23.53%	2.161%
3	4.060	135	140	148	rVB	20055	29254	1.05%	0.096%
4	7.084	645	654	666	rBV	510705	786399	28.17%	2.587%
5	7.248	676	682	692	rVB	390220	611795	21.91%	2.013%
6	7.454	710	717	727	rVB	523467	808931	28.98%	2.661%
7	7.925	791	797	805	rVB	436262	689854	24.71%	2.270%
8	8.637	911	918	931	rBV	627315	988593	35.41%	3.252%
9	9.089	988	995	1004	rBV	512764	811419	29.07%	2.670%
10	9.819	1112	1119	1129	rBV	413132	693248	24.83%	2.281%
11	10.360	1202	1211	1227	rBV	603383	1013147	36.29%	3.333%
12	10.742	1268	1276	1283	rVB	614544	1038806	37.21%	3.418%
13	10.872	1290	1298	1311	rBV	612337	1062362	38.05%	3.495%
14	12.330	1541	1546	1553	rVB2	8898	14695	0.53%	0.048%
15	13.977	1819	1826	1837	rBV	1264396	1716830	61.50%	5.648%
16	14.260	1866	1874	1891	rBV	1299638	1874199	67.13%	6.166%
17	14.389	1893	1896	1901	rBV5	4143	6752	0.24%	0.022%
18	14.566	1920	1926	1935	rBV	1010089	1465504	52.49%	4.822%
19	14.754	1951	1958	1978	rBV	401490	766293	27.45%	2.521%
20	15.554	2088	2094	2104	rBV	1661829	2346421	84.05%	7.720%
21	15.666	2107	2113	2131	rVV	552635	778956	27.90%	2.563%
22	15.795	2131	2135	2138	rVB2	9944	12842	0.46%	0.042%
23	16.230	2204	2209	2212	rVB5	2098	3582	0.13%	0.012%
24	17.089	2351	2355	2361	rVB3	4297	5476	0.20%	0.018%
25	17.301	2384	2391	2400	rBV	1227147	1745694	62.53%	5.743%
26	17.401	2401	2408	2423	rVV	1918358	2624113	94.00%	8.633%
27	18.859	2654	2656	2659	rBV4	2603	3055	0.11%	0.010%
28	19.254	2717	2723	2727	rBV3	22732	37052	1.33%	0.122%
29	19.324	2731	2735	2739	rVV2	17786	25090	0.90%	0.083%
30	19.689	2791	2797	2804	rBV	2014021	2791714	100.00%	9.185%
31	21.465	3094	3099	3107	rBV	1223435	1566602	56.12%	5.154%
32	23.706	3473	3480	3488	rBV2	1045621	2049097	73.40%	6.742%
33	23.859	3500	3506	3515	rVB2	672637	1320210	47.29%	4.344%




Sum of corrected areas: 30394881

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020122\
Data File : BM033933.D
Acq On : 01 Feb 2022 10:59
Operator : CG/JU
Sample : PB142371BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK371

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

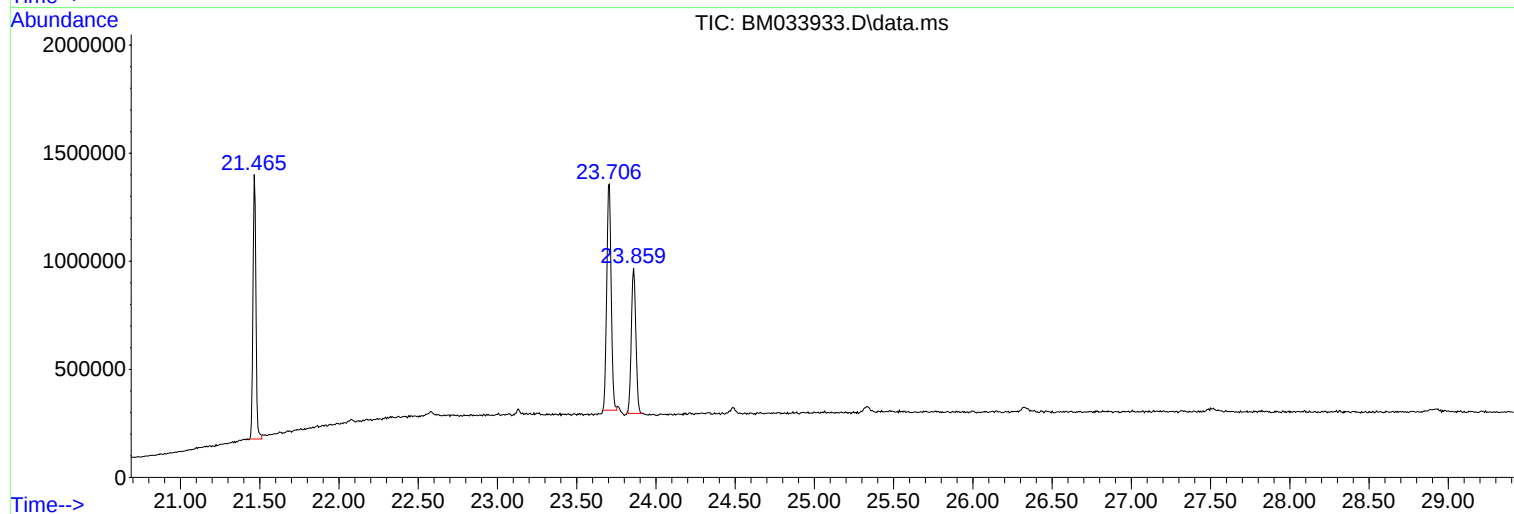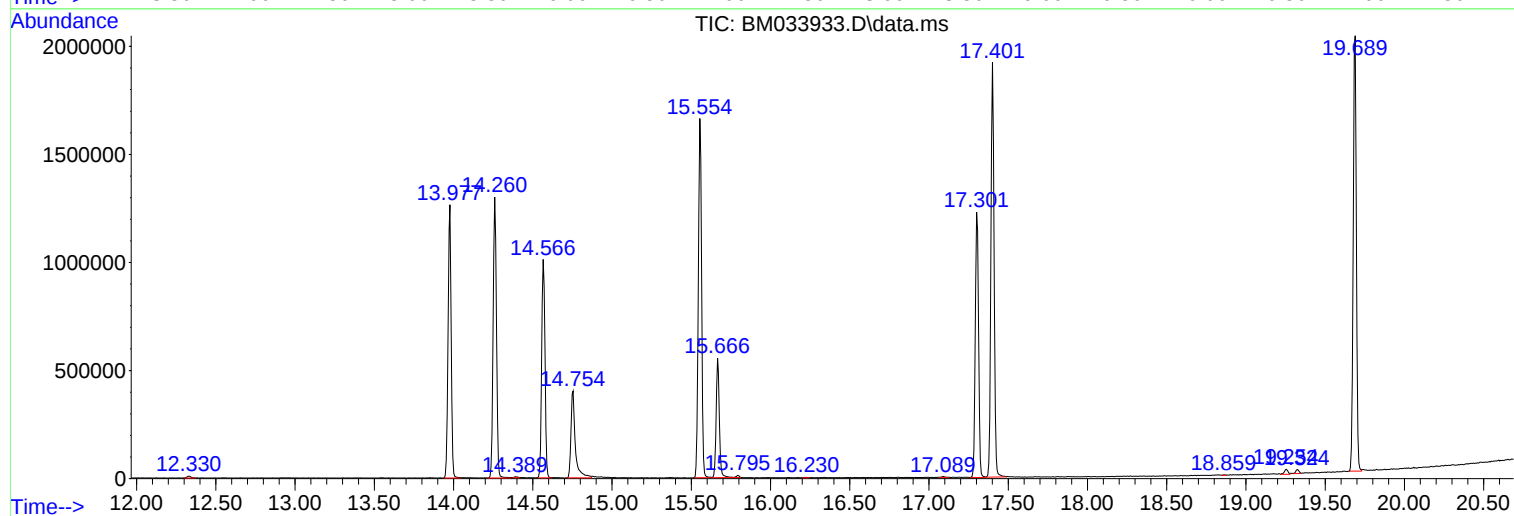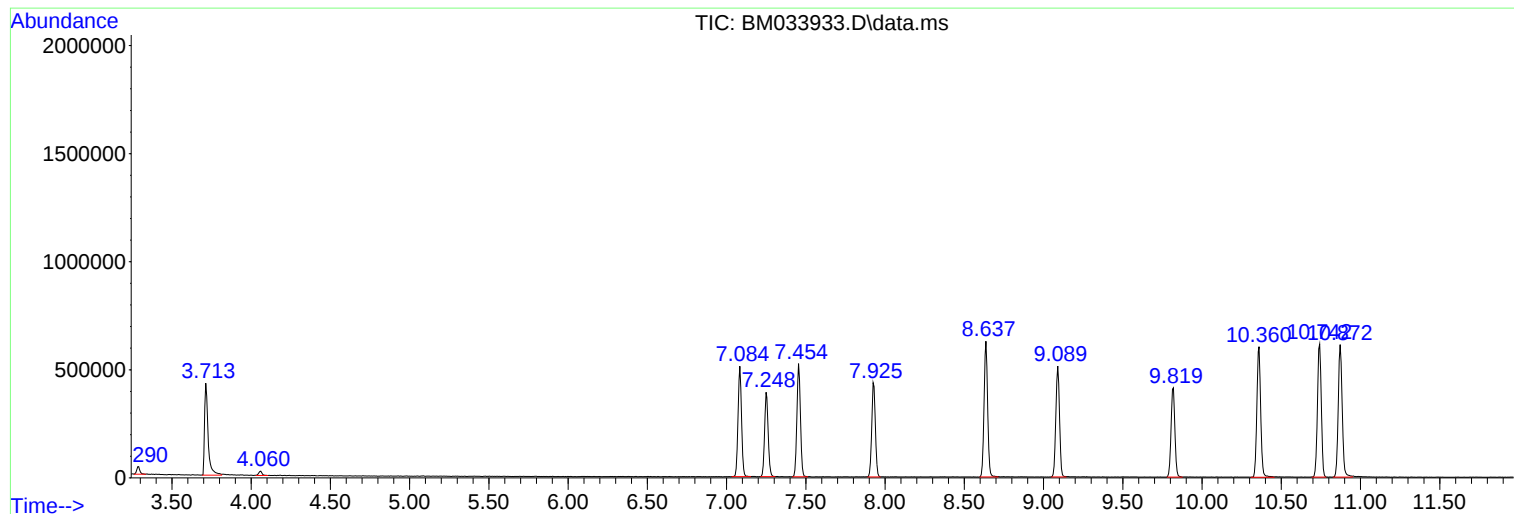

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020122\
Data File : BM033933.D
Acq On : 01 Feb 2022 10:59
Operator : CG/JU
Sample : PB142371BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK371

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020122\
Data File : BM033933.D
Acq On : 01 Feb 2022 10:59
Operator : CG/JU
Sample : PB142371BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK371

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc