

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020122\
 Data File : BM033934.D
 Acq On : 01 Feb 2022 11:59
 Operator : CG/JU
 Sample : PB142407BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK407

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
 Title : SVOA CALIBRATION

Signal : TIC: BM033934.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.284	5	8	17	rVB	35378	51213	1.67%	0.160%
2	3.713	77	81	106	rBV	431371	679258	22.14%	2.121%
3	4.060	135	140	145	rBV	19107	27848	0.91%	0.087%
4	7.084	647	654	666	rBV	523523	807610	26.33%	2.521%
5	7.248	674	682	694	rBV	399349	632008	20.60%	1.973%
6	7.454	710	717	726	rBV	534199	828331	27.00%	2.586%
7	7.925	791	797	808	rVB	455664	708152	23.09%	2.211%
8	8.637	911	918	929	rBV	637486	1024129	33.39%	3.197%
9	9.089	987	995	1005	rBV	521761	838225	27.33%	2.617%
10	9.819	1111	1119	1127	rBV	429882	718661	23.43%	2.244%
11	10.354	1204	1210	1225	rBV	592537	1043174	34.01%	3.257%
12	10.742	1268	1276	1285	rVB	637696	1067093	34.79%	3.331%
13	10.872	1290	1298	1315	rBV	638721	1103000	35.96%	3.443%
14	12.330	1540	1546	1552	rVB2	9633	16497	0.54%	0.052%
15	13.977	1818	1826	1837	rBV	1331992	1814468	59.15%	5.664%
16	14.260	1867	1874	1889	rBV	1342887	1956498	63.78%	6.108%
17	14.389	1893	1896	1902	rBV5	4923	7959	0.26%	0.025%
18	14.566	1920	1926	1935	rBV	1021575	1530517	49.89%	4.778%
19	14.748	1952	1957	1980	rBV	457415	830508	27.07%	2.593%
20	15.554	2087	2094	2106	rBV	1764771	2479116	80.82%	7.739%
21	15.665	2107	2113	2131	rVV	617660	853680	27.83%	2.665%
22	15.795	2131	2135	2140	rVB2	11380	13769	0.45%	0.043%
23	17.089	2351	2355	2359	rBV4	5276	8486	0.28%	0.026%
24	17.301	2385	2391	2400	rBV	1267285	1847220	60.22%	5.767%
25	17.401	2400	2408	2420	rBV	1956637	2789325	90.93%	8.708%
26	18.171	2535	2539	2542	rBV5	2332	4341	0.14%	0.014%
27	19.253	2719	2723	2729	rVB3	22167	29609	0.97%	0.092%
28	19.324	2731	2735	2739	rBV	22281	31730	1.03%	0.099%
29	19.689	2791	2797	2804	rBV	2289911	3067491	100.00%	9.576%
30	21.465	3094	3099	3109	rBV	1298709	1691544	55.14%	5.281%
31	23.706	3473	3480	3487	rBV	1114404	2168456	70.69%	6.769%
32	23.859	3500	3506	3515	rVB2	669252	1362937	44.43%	4.255%




Sum of corrected areas: 32032853

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020122\
Data File : BM033934.D
Acq On : 01 Feb 2022 11:59
Operator : CG/JU
Sample : PB142407BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK407

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

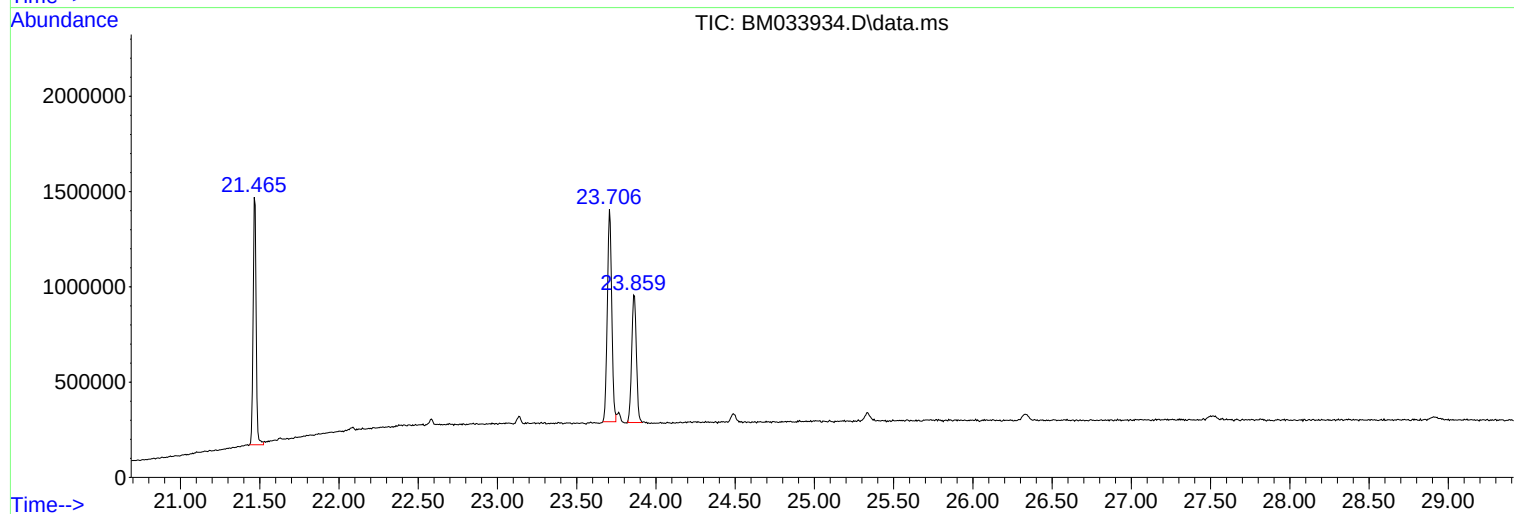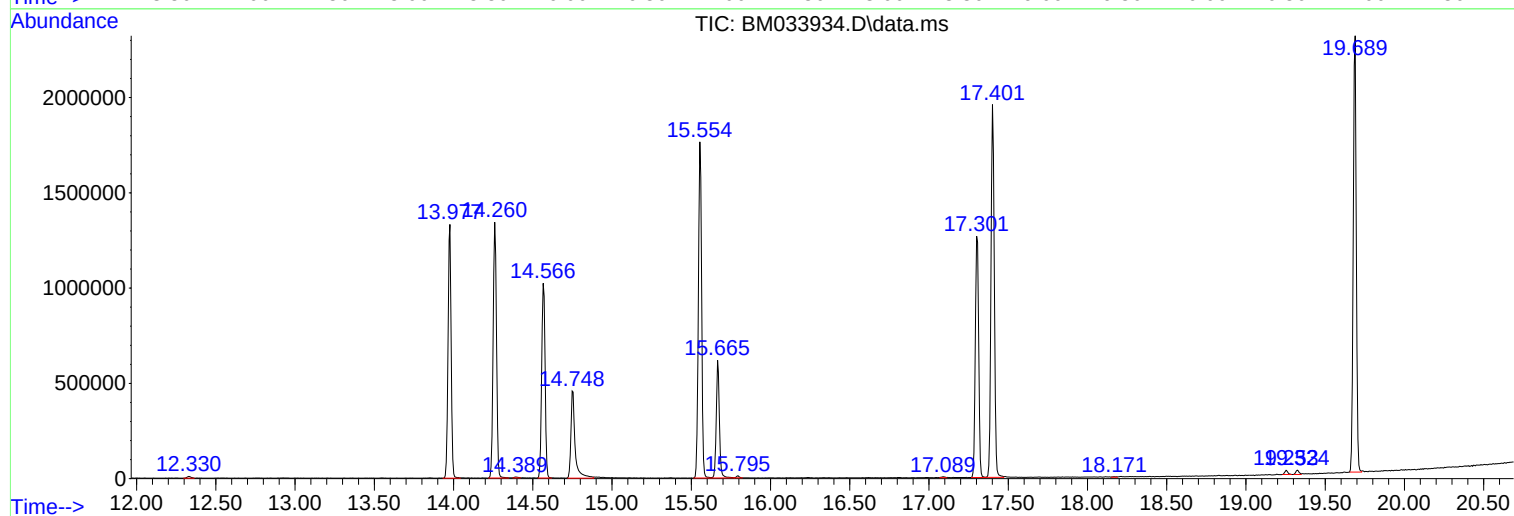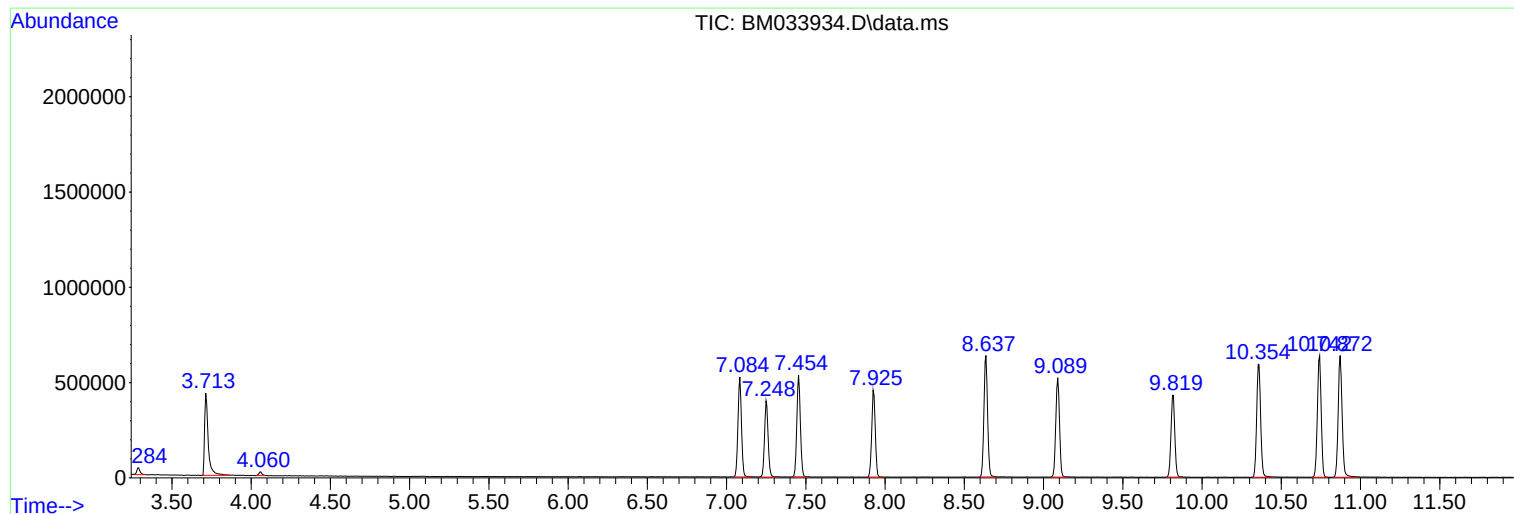

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020122\
Data File : BM033934.D
Acq On : 01 Feb 2022 11:59
Operator : CG/JU
Sample : PB142407BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK407

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020122\
Data File : BM033934.D
Acq On : 01 Feb 2022 11:59
Operator : CG/JU
Sample : PB142407BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK407

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc