

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020122\
 Data File : BM033937.D
 Acq On : 01 Feb 2022 13:46
 Operator : CG/JU
 Sample : N1273-17
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 COHL5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
 Title : SVOA CALIBRATION

Signal : TIC: BM033937.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.325	12	15	32	rVB	398823	574805	2.21%	1.070%
2	4.160	152	157	166	rBV3	24870	40411	0.16%	0.075%
3	4.607	226	233	247	rBV	16891303	25998358	100.00%	48.406%
4	7.084	647	654	667	rVB	115687	196770	0.76%	0.366%
5	7.254	676	683	694	rBV	442235	697052	2.68%	1.298%
6	7.454	710	717	728	rBV	448418	712569	2.74%	1.327%
7	7.619	739	745	750	rVB	36230	55674	0.21%	0.104%
8	7.931	791	798	806	rBV	391883	621699	2.39%	1.158%
9	8.637	912	918	928	rBV	324205	520028	2.00%	0.968%
10	9.089	988	995	1004	rBV	585987	929944	3.58%	1.731%
11	9.819	1110	1119	1132	rBV	470304	780881	3.00%	1.454%
12	10.360	1203	1211	1224	rBV	612408	1037343	3.99%	1.931%
13	10.525	1233	1239	1250	rBV2	17081	34256	0.13%	0.064%
14	10.742	1268	1276	1283	rBV	548753	916263	3.52%	1.706%
15	10.872	1293	1298	1311	rVB	91204	156525	0.60%	0.291%
16	13.977	1818	1826	1838	rBV	1304644	1818417	6.99%	3.386%
17	14.260	1868	1874	1888	rVB	1350588	1908528	7.34%	3.553%
18	14.566	1919	1926	1935	rBV	865926	1236183	4.75%	2.302%
19	14.760	1951	1959	1970	rBV2	50440	121238	0.47%	0.226%
20	15.554	2087	2094	2107	rBV	1750415	2564978	9.87%	4.776%
21	15.666	2107	2113	2126	rVV	648559	885287	3.41%	1.648%
22	15.795	2130	2135	2144	rVB3	14039	26866	0.10%	0.050%
23	17.301	2385	2391	2400	rBV	940426	1341142	5.16%	2.497%
24	17.401	2400	2408	2419	rBV	2060621	2823402	10.86%	5.257%
25	18.195	2539	2543	2549	rBV4	29932	43516	0.17%	0.081%
26	19.254	2719	2723	2726	rBV2	21083	30067	0.12%	0.056%
27	19.318	2731	2734	2740	rVB	21525	26263	0.10%	0.049%
28	19.683	2790	2796	2809	rBV	2091005	2847637	10.95%	5.302%
29	21.177	3047	3050	3055	rBV3	49955	72187	0.28%	0.134%
30	21.465	3094	3099	3107	rBV	898246	1143711	4.40%	2.129%
31	23.700	3472	3479	3487	rBV2	1251014	2444899	9.40%	4.552%
32	23.853	3499	3505	3514	rVB2	556118	1101787	4.24%	2.051%




Sum of corrected areas: 53708686

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020122\
Data File : BM033937.D
Acq On : 01 Feb 2022 13:46
Operator : CG/JU
Sample : N1273-17
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
COHL5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

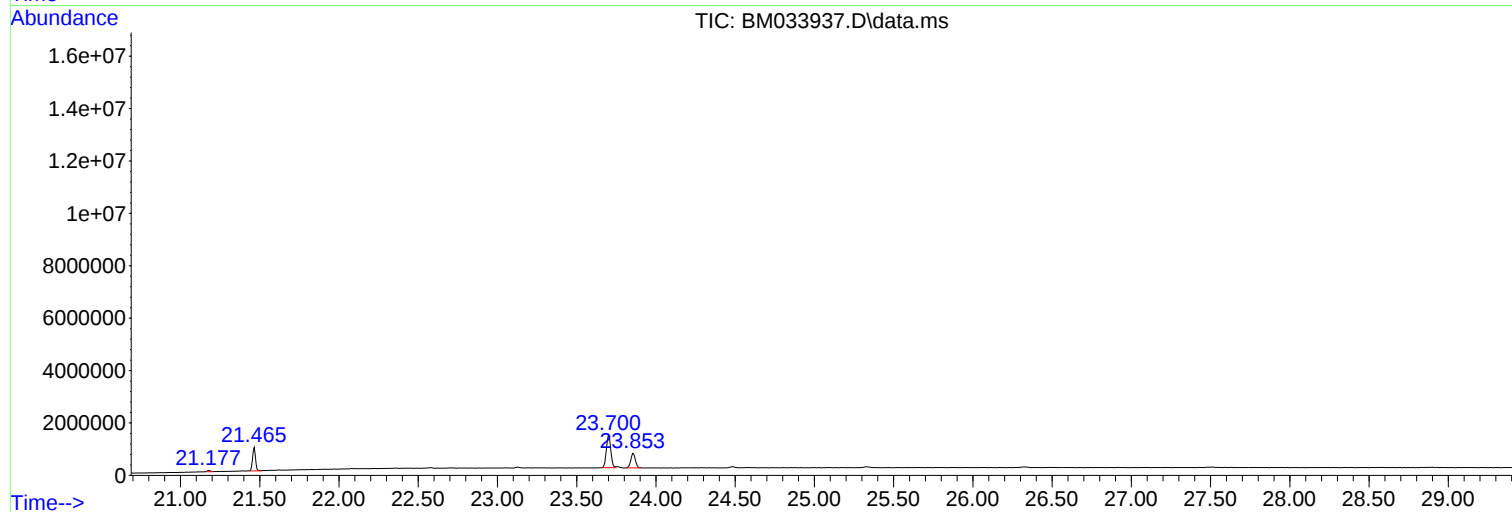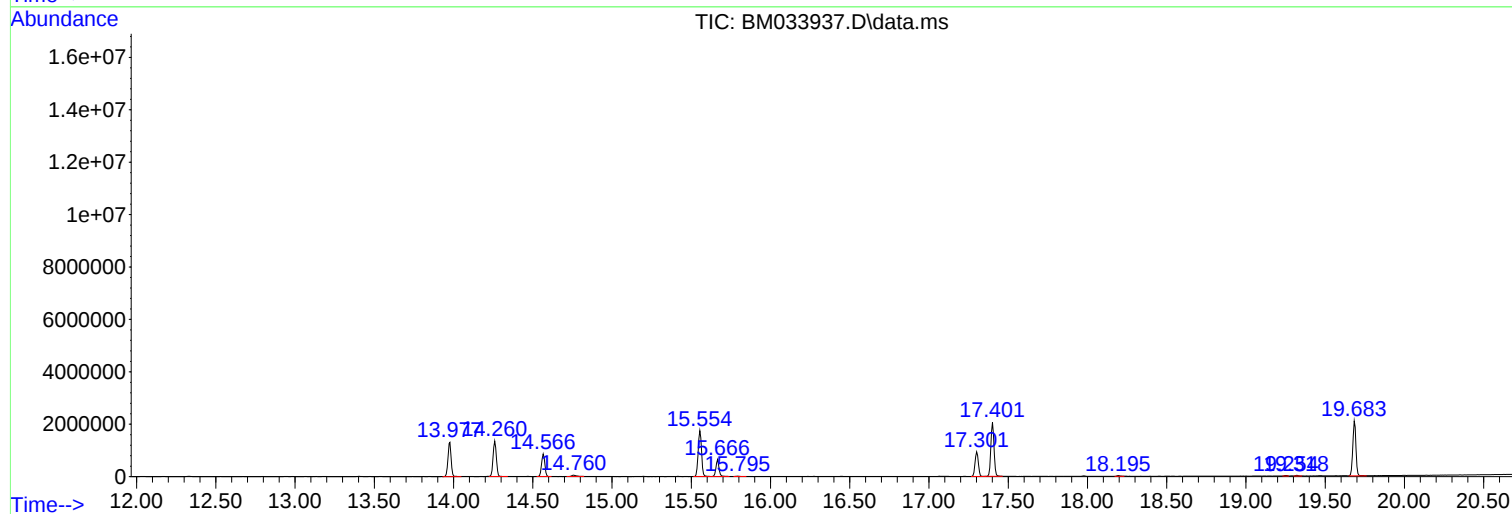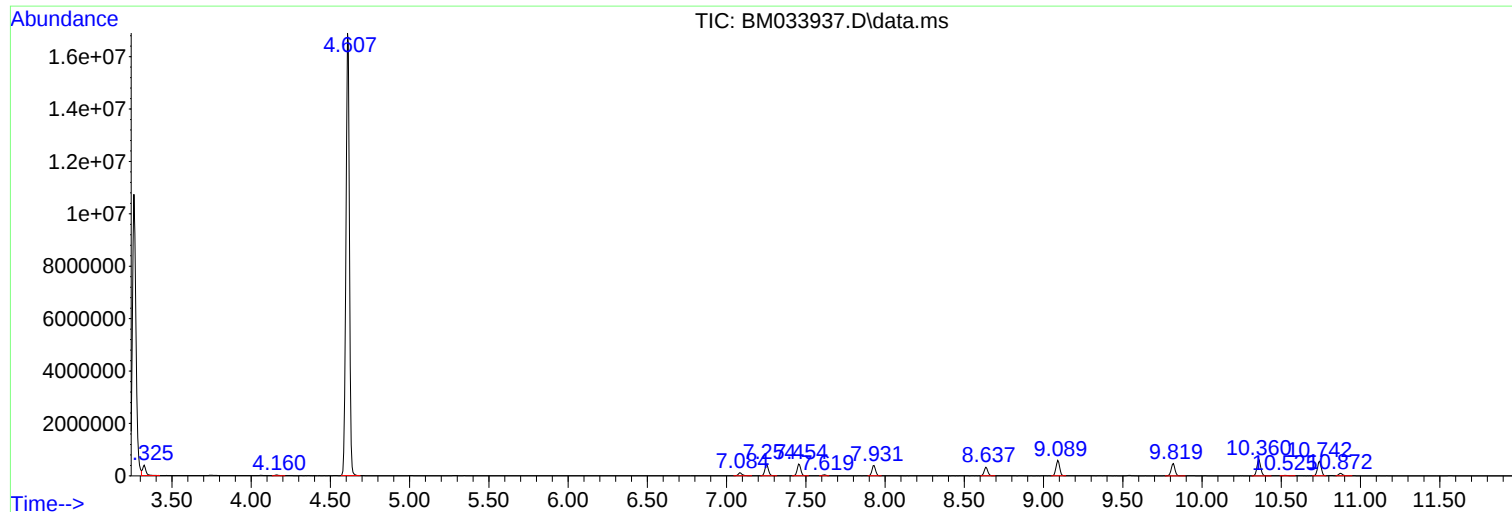

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020122\
Data File : BM033937.D
Acq On : 01 Feb 2022 13:46
Operator : CG/JU
Sample : N1273-17
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0HL5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020122\
Data File : BM033937.D
Acq On : 01 Feb 2022 13:46
Operator : CG/JU
Sample : N1273-17
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0HL5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
