

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020122\
 Data File : BM033938.D
 Acq On : 01 Feb 2022 14:22
 Operator : CG/JU
 Sample : N1273-13
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 COHL1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
 Title : SVOA CALIBRATION

Signal : TIC: BM033938.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.325	13	15	21	rVB	20198	25154	0.37%	0.073%
2	3.731	80	84	94	rBV	50278	90479	1.32%	0.262%
3	4.061	136	140	146	rVB	10218	14391	0.21%	0.042%
4	4.608	226	233	246	rBV	4609910	6831402	100.00%	19.817%
5	5.013	297	302	306	rBV5	4893	8193	0.12%	0.024%
6	5.213	331	336	343	rVB2	29026	44300	0.65%	0.129%
7	7.084	648	654	666	rVB2	122725	197854	2.90%	0.574%
8	7.254	676	683	692	rBV	425399	681625	9.98%	1.977%
9	7.454	711	717	730	rVB	439747	694725	10.17%	2.015%
10	7.931	791	798	808	rBV	383073	635881	9.31%	1.845%
11	8.637	912	918	928	rBV2	320693	515466	7.55%	1.495%
12	9.090	987	995	1004	rBV	575339	923766	13.52%	2.680%
13	9.543	1066	1072	1081	rVB	53526	80397	1.18%	0.233%
14	9.819	1111	1119	1134	rBV	461580	751862	11.01%	2.181%
15	10.360	1203	1211	1225	rBV	590559	1011811	14.81%	2.935%
16	10.742	1268	1276	1283	rVB	539971	896767	13.13%	2.601%
17	10.813	1283	1288	1292	rBV2	11293	17483	0.26%	0.051%
18	10.872	1292	1298	1316	rVB	432777	736067	10.77%	2.135%
19	12.042	1491	1497	1502	rBV	22545	34288	0.50%	0.099%
20	12.331	1541	1546	1553	rBV2	10457	17424	0.26%	0.051%
21	13.978	1819	1826	1831	rBV	1266831	1771973	25.94%	5.140%
22	14.260	1868	1874	1884	rBV	1419654	2013447	29.47%	5.841%
23	14.566	1919	1926	1936	rBV	852403	1221614	17.88%	3.544%
24	14.760	1954	1959	1982	rBV2	48088	120653	1.77%	0.350%
25	15.554	2088	2094	2107	rBV	1821122	2524441	36.95%	7.323%
26	15.666	2107	2113	2125	rVV	608477	824910	12.08%	2.393%
27	15.795	2130	2135	2140	rVB	13740	19846	0.29%	0.058%
28	16.330	2224	2226	2233	rVB7	4280	6859	0.10%	0.020%
29	16.807	2304	2307	2312	rVB2	9286	12094	0.18%	0.035%
30	17.083	2346	2354	2358	rBV5	6155	14579	0.21%	0.042%
31	17.301	2385	2391	2400	rBV	948736	1345214	19.69%	3.902%
32	17.401	2401	2408	2420	rBV2	1911074	2774590	40.62%	8.049%
33	17.883	2485	2490	2493	rBV	9375	13021	0.19%	0.038%
34	18.195	2538	2543	2547	rBV3	20440	29500	0.43%	0.086%
35	18.818	2646	2649	2653	rVB4	9768	12655	0.19%	0.037%
36	19.254	2718	2723	2727	rBV4	20972	31650	0.46%	0.092%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020122\
Data File : BM033938.D
Acq On : 01 Feb 2022 14:22
Operator : CG/JU
Sample : N1273-13
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
COHL1

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
Title : SVOA CALIBRATION

37	19.324	2730	2735	2738	rVV	19844	28021	0.41%	0.081%
38	19.471	2757	2760	2765	rBV6	10449	16508	0.24%	0.048%
39	19.612	2781	2784	2787	rVB4	12054	14096	0.21%	0.041%
40	19.683	2790	2796	2803	rBV	2157452	2815295	41.21%	8.167%
41	21.465	3094	3099	3104	rBV	878741	1129591	16.54%	3.277%
42	23.700	3472	3479	3486	rBV2	1247769	2393125	35.03%	6.942%
43	23.853	3499	3505	3516	rVB2	572171	1130195	16.54%	3.278%




Sum of corrected areas: 34473212

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020122\
Data File : BM033938.D
Acq On : 01 Feb 2022 14:22
Operator : CG/JU
Sample : N1273-13
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
COHL1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

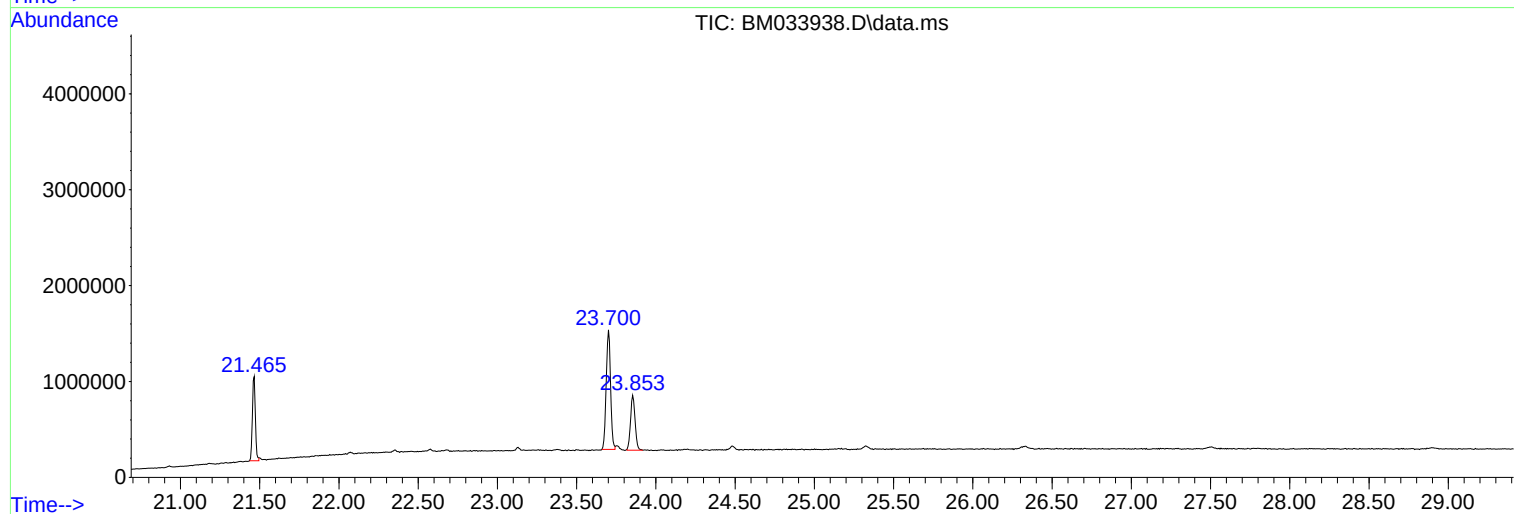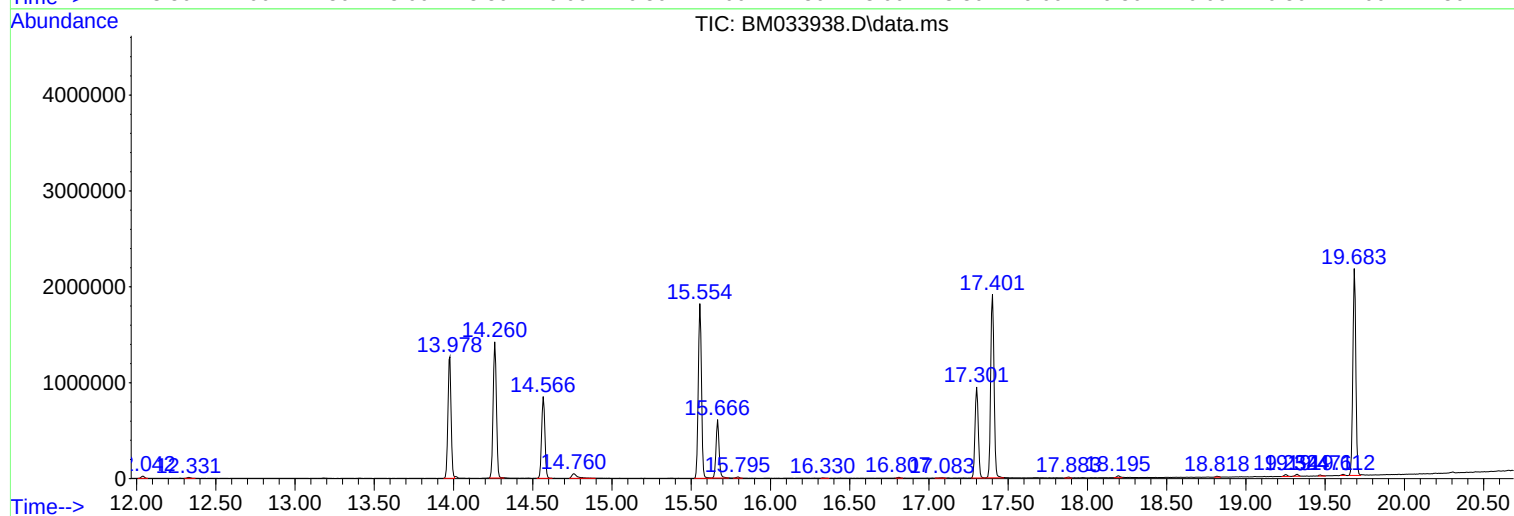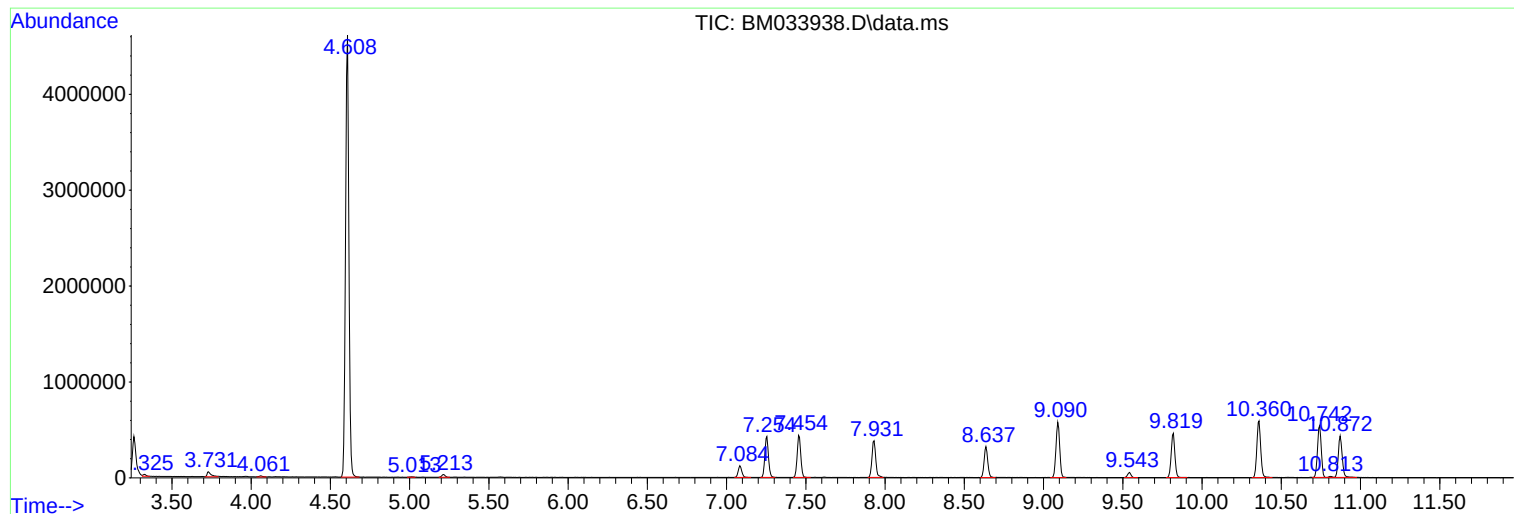

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020122\
Data File : BM033938.D
Acq On : 01 Feb 2022 14:22
Operator : CG/JU
Sample : N1273-13
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0HL1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020122\
Data File : BM033938.D
Acq On : 01 Feb 2022 14:22
Operator : CG/JU
Sample : N1273-13
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0HL1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc