

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020122\
 Data File : BM033940.D
 Acq On : 01 Feb 2022 15:34
 Operator : CG/JU
 Sample : N1273-20
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 COHL8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
 Title : SVOA CALIBRATION

Signal : TIC: BM033940.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.325	13	15	27	rVB	172417	227332	1.14%	0.475%
2	4.160	153	157	164	rVB6	16705	24013	0.12%	0.050%
3	4.607	226	233	246	rBV	13259579	19957037	100.00%	41.725%
4	7.084	649	654	664	rVB2	101397	177818	0.89%	0.372%
5	7.254	676	683	692	rBV	437625	698544	3.50%	1.460%
6	7.454	710	717	727	rVB	430163	669122	3.35%	1.399%
7	7.613	740	744	750	rVB	19454	29021	0.15%	0.061%
8	7.931	791	798	807	rBV	401792	626451	3.14%	1.310%
9	8.636	911	918	927	rBV	312106	492555	2.47%	1.030%
10	9.089	988	995	1003	rBV	595587	956367	4.79%	2.000%
11	9.819	1111	1119	1127	rBV	495478	782078	3.92%	1.635%
12	10.360	1203	1211	1224	rBV	617758	1047132	5.25%	2.189%
13	10.519	1233	1238	1254	rVB2	45764	81268	0.41%	0.170%
14	10.742	1266	1276	1284	rVB	552994	919110	4.61%	1.922%
15	10.872	1291	1298	1313	rVB	466261	799653	4.01%	1.672%
16	13.471	1735	1740	1748	rVB2	17289	28379	0.14%	0.059%
17	13.977	1819	1826	1836	rBV	1301985	1843486	9.24%	3.854%
18	14.260	1867	1874	1890	rVB	1456207	2131593	10.68%	4.457%
19	14.566	1920	1926	1936	rVB	869441	1231742	6.17%	2.575%
20	14.754	1954	1958	1975	rBV3	35364	96280	0.48%	0.201%
21	15.554	2087	2094	2107	rBV	1871492	2620629	13.13%	5.479%
22	15.665	2107	2113	2126	rVV	583883	815835	4.09%	1.706%
23	17.301	2385	2391	2401	rBV	969317	1359290	6.81%	2.842%
24	17.401	2401	2408	2423	rBV2	1944747	2760164	13.83%	5.771%
25	17.977	2501	2506	2513	rVB	60605	78225	0.39%	0.164%
26	18.195	2539	2543	2546	rBV4	20923	30256	0.15%	0.063%
27	19.142	2700	2704	2712	rVB	89672	108104	0.54%	0.226%
28	19.253	2719	2723	2725	rBV2	19985	26887	0.13%	0.056%
29	19.324	2731	2735	2739	rVB	18617	24004	0.12%	0.050%
30	19.683	2790	2796	2809	rBV	2095143	2735047	13.70%	5.718%
31	21.465	3094	3099	3108	rBV	901033	1149645	5.76%	2.404%
32	23.700	3473	3479	3487	rBV2	1118512	2219264	11.12%	4.640%
33	23.859	3500	3506	3515	rVB2	539596	1083476	5.43%	2.265%




Sum of corrected areas: 47829807

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020122\
Data File : BM033940.D
Acq On : 01 Feb 2022 15:34
Operator : CG/JU
Sample : N1273-20
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
COHL8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

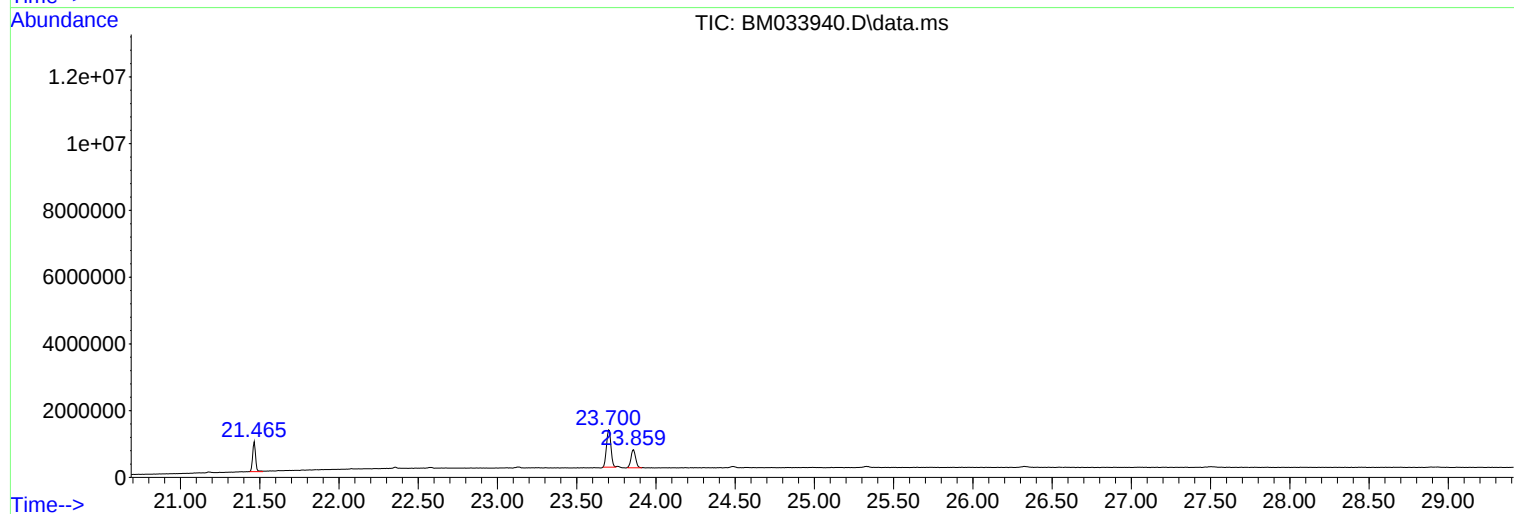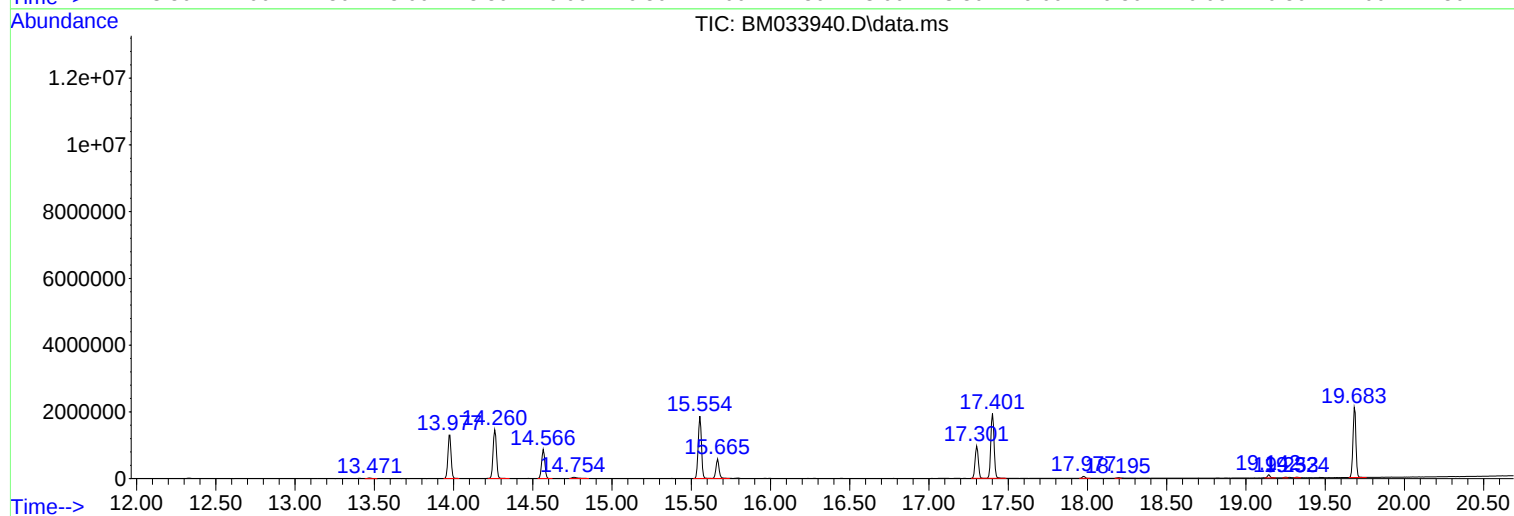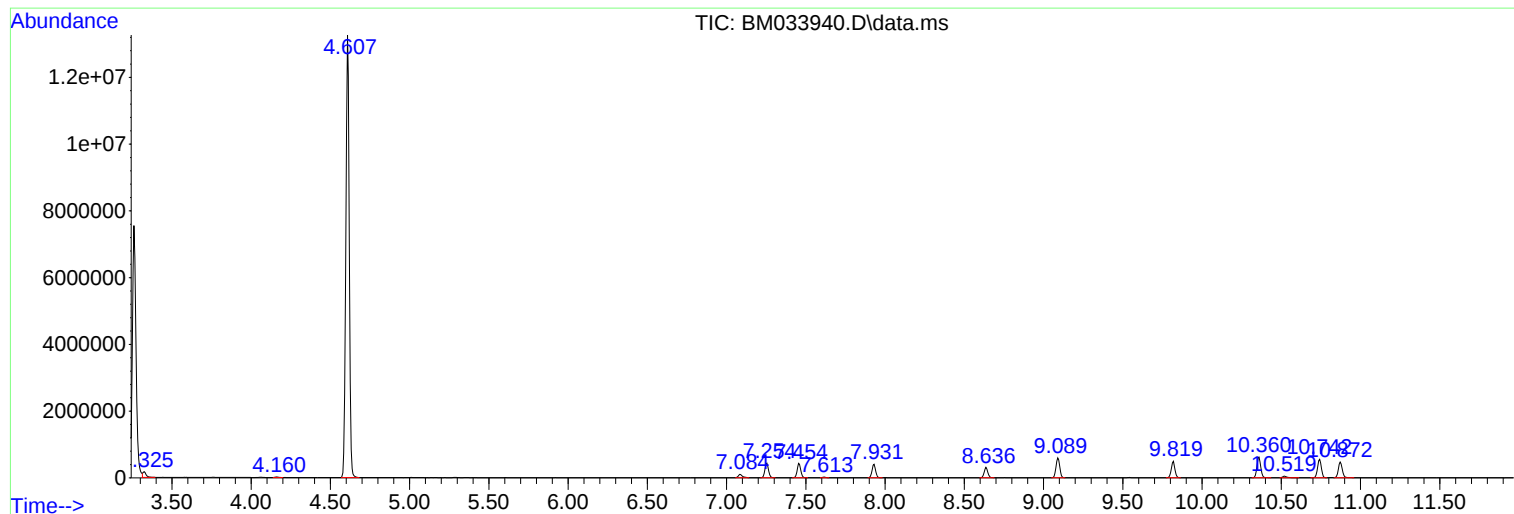

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020122\
Data File : BM033940.D
Acq On : 01 Feb 2022 15:34
Operator : CG/JU
Sample : N1273-20
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0HL8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020122\
Data File : BM033940.D
Acq On : 01 Feb 2022 15:34
Operator : CG/JU
Sample : N1273-20
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0HL8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------