

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020122\
 Data File : BM033942.D
 Acq On : 01 Feb 2022 16:45
 Operator : CG/JU
 Sample : N1273-15
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 COHL3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
 Title : SVOA CALIBRATION

Signal : TIC: BM033942.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.325	13	15	21	rVB	20507	29879	0.99%	0.095%
2	3.725	81	83	98	rBV	57744	99488	3.31%	0.317%
3	4.060	136	140	146	rBV2	12046	17850	0.59%	0.057%
4	4.607	226	233	247	rVB	1983982	3004369	100.00%	9.572%
5	5.013	298	302	305	rVB4	3603	5090	0.17%	0.016%
6	7.084	648	654	663	rVB	110994	171853	5.72%	0.548%
7	7.254	676	683	692	rBV	451947	720843	23.99%	2.297%
8	7.454	711	717	726	rVB	455764	705582	23.49%	2.248%
9	7.931	791	798	806	rVB	444093	698740	23.26%	2.226%
10	8.637	911	918	928	rBV	315224	499454	16.62%	1.591%
11	9.089	987	995	1007	rBV	599031	971170	32.33%	3.094%
12	9.542	1066	1072	1077	rVB	55078	84038	2.80%	0.268%
13	9.819	1111	1119	1135	rVB	475308	787501	26.21%	2.509%
14	10.354	1204	1210	1225	rBV	608543	1046499	34.83%	3.334%
15	10.554	1237	1244	1246	rBV5	1757	3200	0.11%	0.010%
16	10.689	1262	1267	1269	rBV3	3549	5139	0.17%	0.016%
17	10.742	1269	1276	1283	rVB	592585	997227	33.19%	3.177%
18	10.813	1283	1288	1291	rBV4	4634	7481	0.25%	0.024%
19	10.872	1291	1298	1315	rVV	492166	868928	28.92%	2.769%
20	12.036	1490	1496	1503	rBV	42476	63700	2.12%	0.203%
21	12.330	1541	1546	1551	rBV2	11935	18249	0.61%	0.058%
22	13.195	1686	1693	1696	rBV6	2660	4485	0.15%	0.014%
23	13.401	1725	1728	1733	rBV4	2295	3053	0.10%	0.010%
24	13.542	1748	1752	1757	rBV6	2643	3303	0.11%	0.011%
25	13.842	1801	1803	1809	rBV4	2266	3453	0.11%	0.011%
26	13.971	1819	1825	1831	rBV	1255785	1735693	57.77%	5.530%
27	14.207	1859	1865	1867	rBV5	3874	6990	0.23%	0.022%
28	14.260	1867	1874	1884	rVV	1451661	2048617	68.19%	6.527%
29	14.566	1919	1926	1934	rBV	897678	1288443	42.89%	4.105%
30	14.760	1954	1959	1968	rBV2	37063	89603	2.98%	0.285%
31	15.554	2087	2094	2107	rBV	1813420	2478604	82.50%	7.897%
32	15.665	2107	2113	2125	rVV	568422	772495	25.71%	2.461%
33	15.795	2131	2135	2142	rVB3	12844	18664	0.62%	0.059%
34	16.807	2304	2307	2312	rVB4	3403	4672	0.16%	0.015%
35	17.089	2352	2355	2360	rVB	3929	4575	0.15%	0.015%
36	17.301	2384	2391	2401	rBV	999760	1379973	45.93%	4.397%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020122\
 Data File : BM033942.D
 Acq On : 01 Feb 2022 16:45
 Operator : CG/JU
 Sample : N1273-15
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 COHL3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
 Title : SVOA CALIBRATION

37	17.401	2401	2408	2423	rVV	1886095	2660902	88.57%	8.478%
38	17.677	2451	2455	2457	rBV5	2416	4112	0.14%	0.013%
39	17.877	2485	2489	2492	rBV5	4465	4912	0.16%	0.016%
40	17.977	2501	2506	2511	rBV	13846	16671	0.55%	0.053%
41	18.195	2539	2543	2550	rBV3	22656	37149	1.24%	0.118%
42	18.489	2591	2593	2597	rBV4	2920	4022	0.13%	0.013%
43	18.812	2646	2648	2654	rVB7	4919	8155	0.27%	0.026%
44	18.865	2654	2657	2658	rBV2	3290	3314	0.11%	0.011%
45	19.142	2702	2704	2707	rVB3	9083	9668	0.32%	0.031%
46	19.248	2719	2722	2728	rVB4	17638	23897	0.80%	0.076%
47	19.318	2731	2734	2740	rBV	17569	25208	0.84%	0.080%
48	19.465	2756	2759	2765	rBV5	17414	27150	0.90%	0.087%
49	19.612	2782	2784	2788	rVB5	9097	9690	0.32%	0.031%
50	19.683	2790	2796	2802	rBV	2057313	2724936	90.70%	8.682%
51	21.465	3094	3099	3104	rBV	1005085	1259834	41.93%	4.014%
52	23.700	3472	3479	3486	rBV2	1284431	2597950	86.47%	8.277%
53	23.859	3499	3506	3516	rVB	642361	1319718	43.93%	4.205%




Sum of corrected areas: 31386191

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020122\
Data File : BM033942.D
Acq On : 01 Feb 2022 16:45
Operator : CG/JU
Sample : N1273-15
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
COHL3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

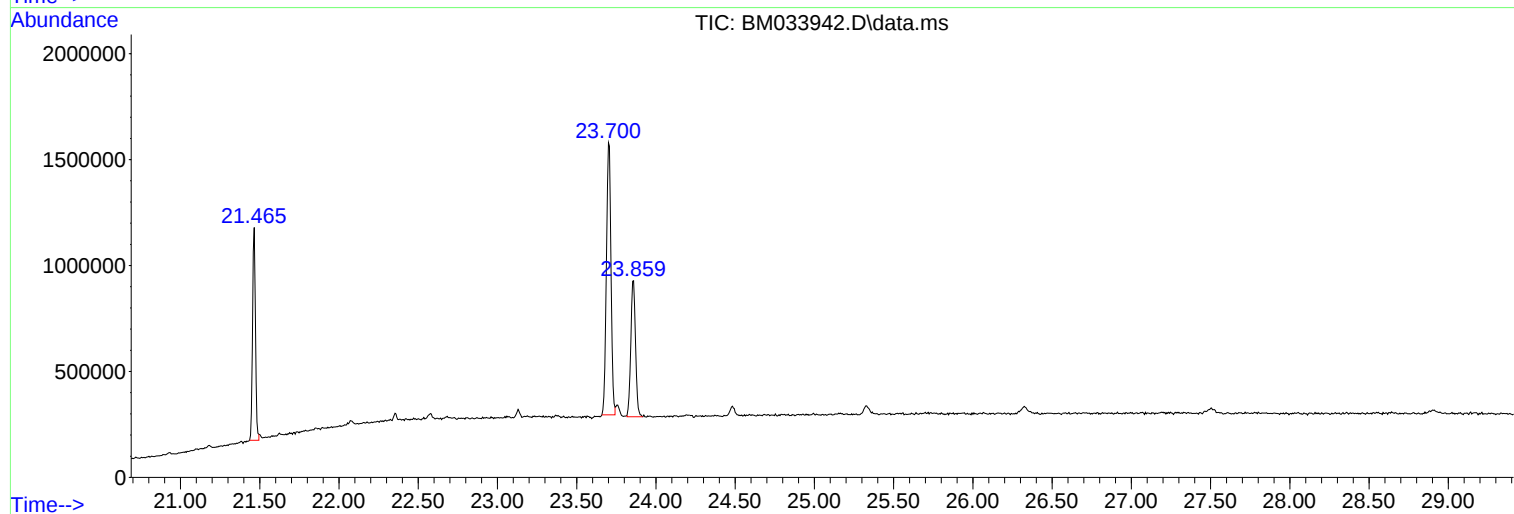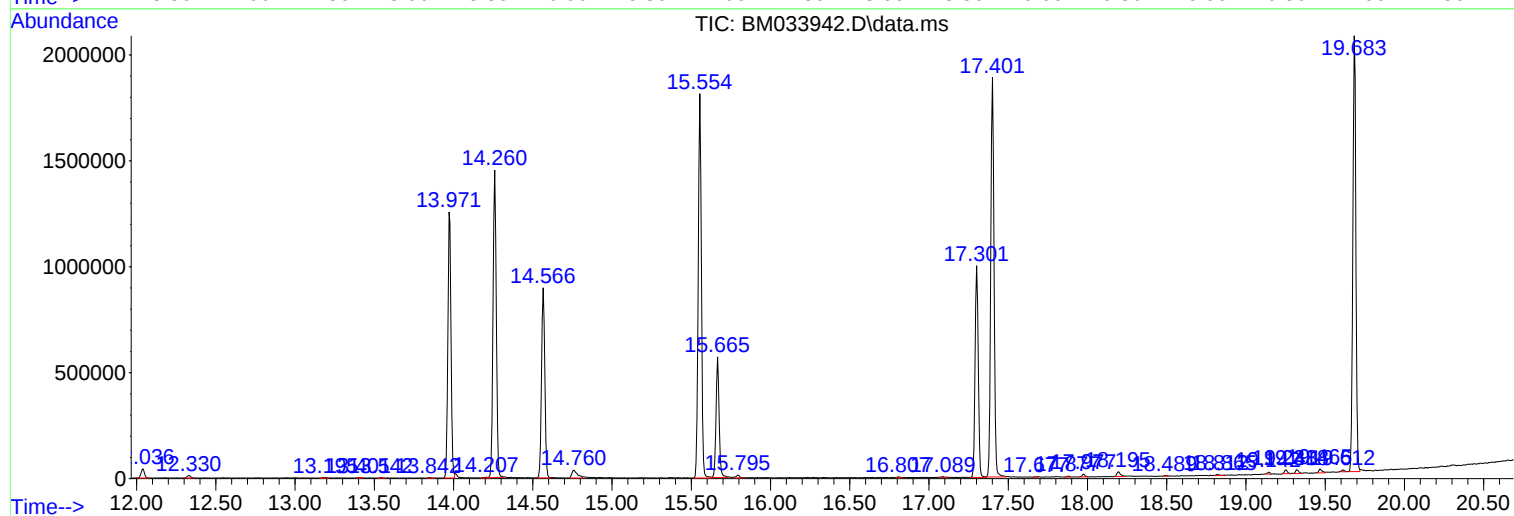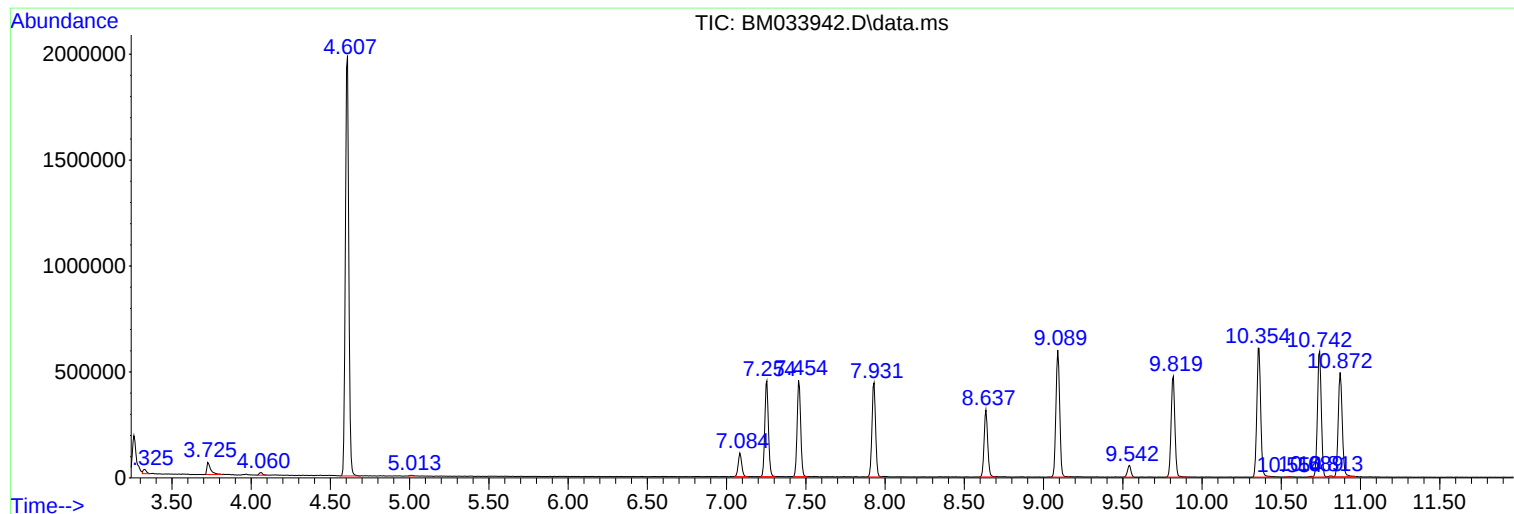

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020122\
Data File : BM033942.D
Acq On : 01 Feb 2022 16:45
Operator : CG/JU
Sample : N1273-15
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0HL3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020122\
Data File : BM033942.D
Acq On : 01 Feb 2022 16:45
Operator : CG/JU
Sample : N1273-15
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0HL3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc