

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020122\
 Data File : BM033943.D
 Acq On : 01 Feb 2022 17:21
 Operator : CG/JU
 Sample : N1273-14
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 COHL2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
 Title : SVOA CALIBRATION

Signal : TIC: BM033943.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.325	13	15	22	rVB	22899	28071	0.37%	0.076%
2	3.725	80	83	96	rBV	95741	162109	2.13%	0.440%
3	3.960	121	123	129	rVB5	4933	7895	0.10%	0.021%
4	4.060	135	140	145	rVB2	11687	16881	0.22%	0.046%
5	4.607	226	233	245	rVB	5123153	7604505	100.00%	20.621%
6	5.213	331	336	343	rVB	32793	47438	0.62%	0.129%
7	6.919	621	626	634	rBV5	6062	13997	0.18%	0.038%
8	7.084	648	654	667	rVB2	117723	189104	2.49%	0.513%
9	7.254	676	683	693	rBV	445136	721614	9.49%	1.957%
10	7.454	711	717	728	rBV	465656	721508	9.49%	1.957%
11	7.619	740	745	752	rVB4	4485	8175	0.11%	0.022%
12	7.931	790	798	809	rBV	451330	759534	9.99%	2.060%
13	8.637	911	918	929	rBV	327356	517997	6.81%	1.405%
14	9.090	988	995	1004	rBV	605665	960677	12.63%	2.605%
15	9.542	1066	1072	1078	rVB	37749	57300	0.75%	0.155%
16	9.819	1111	1119	1128	rBV	473501	778717	10.24%	2.112%
17	10.360	1204	1211	1221	rBV	613869	1044080	13.73%	2.831%
18	10.742	1268	1276	1283	rBV	637304	1045802	13.75%	2.836%
19	10.813	1283	1288	1292	rBV	11575	15778	0.21%	0.043%
20	10.872	1292	1298	1309	rBV	562763	945776	12.44%	2.565%
21	12.036	1490	1496	1504	rVB3	17168	26740	0.35%	0.073%
22	12.325	1540	1545	1551	rBV	11443	20114	0.26%	0.055%
23	13.977	1819	1826	1831	rBV	1317031	1778256	23.38%	4.822%
24	14.260	1867	1874	1889	rVV	1442142	2034899	26.76%	5.518%
25	14.566	1919	1926	1936	rBV	968552	1367091	17.98%	3.707%
26	14.760	1950	1959	1972	rBV2	51626	119530	1.57%	0.324%
27	15.554	2085	2094	2102	rBV	1772495	2554396	33.59%	6.927%
28	15.666	2107	2113	2128	rVV	609122	849305	11.17%	2.303%
29	15.789	2131	2134	2143	rVB4	11670	19533	0.26%	0.053%
30	16.348	2223	2229	2240	rBV2	33668	66356	0.87%	0.180%
31	16.560	2260	2265	2269	rBV	7494	10764	0.14%	0.029%
32	16.666	2276	2283	2288	rBV7	7757	12320	0.16%	0.033%
33	17.301	2385	2391	2401	rBV	1053494	1476164	19.41%	4.003%
34	17.401	2401	2408	2425	rVV	1984146	2792866	36.73%	7.573%
35	18.195	2539	2543	2549	rBV6	14789	22581	0.30%	0.061%
36	18.818	2646	2649	2655	rBV6	6266	8399	0.11%	0.023%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020122\
Data File : BM033943.D
Acq On : 01 Feb 2022 17:21
Operator : CG/JU
Sample : N1273-14
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
COHL2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
Title : SVOA CALIBRATION

37	19.254	2719	2723	2727	rBV3	25656	36240	0.48%	0.098%
38	19.324	2731	2735	2739	rVV	21188	29169	0.38%	0.079%
39	19.471	2757	2760	2766	rBV7	9601	15409	0.20%	0.042%
40	19.612	2782	2784	2788	rVB4	10367	11789	0.16%	0.032%
41	19.683	2790	2796	2804	rBV	2117223	2864625	37.67%	7.768%
42	21.465	3094	3099	3104	rBV	1005426	1288606	16.95%	3.494%
43	23.706	3473	3480	3487	rBV2	1313445	2525548	33.21%	6.849%
44	23.859	3500	3506	3514	rVB2	661881	1299553	17.09%	3.524%




Sum of corrected areas: 36877211

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020122\
Data File : BM033943.D
Acq On : 01 Feb 2022 17:21
Operator : CG/JU
Sample : N1273-14
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
COHL2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

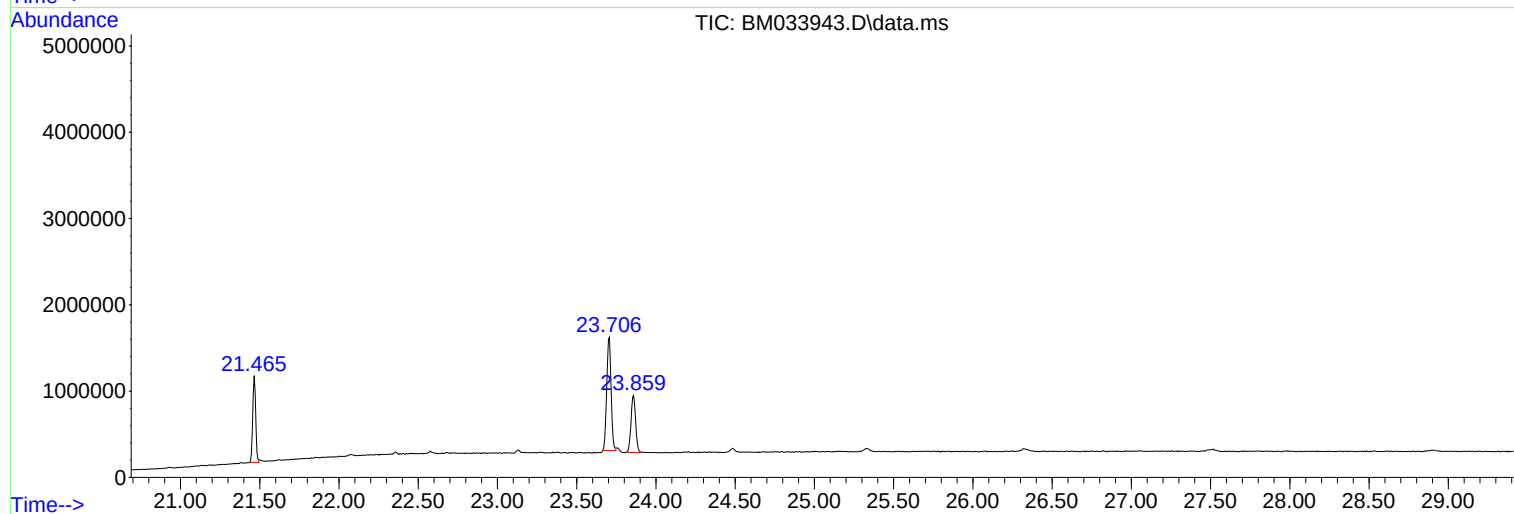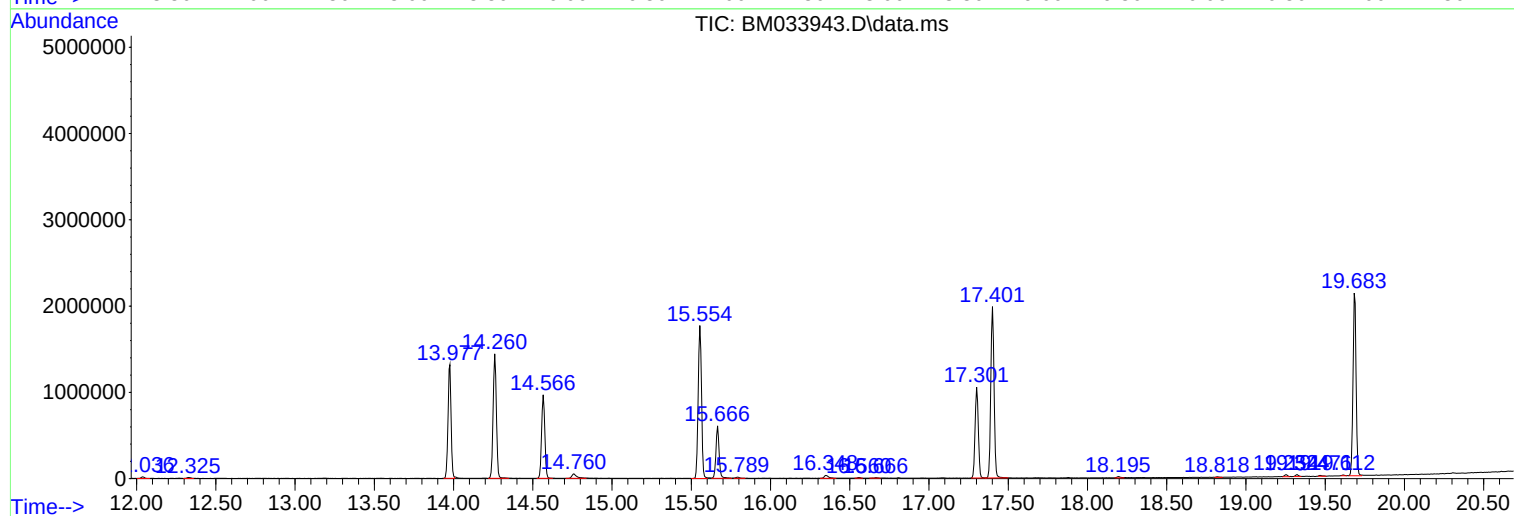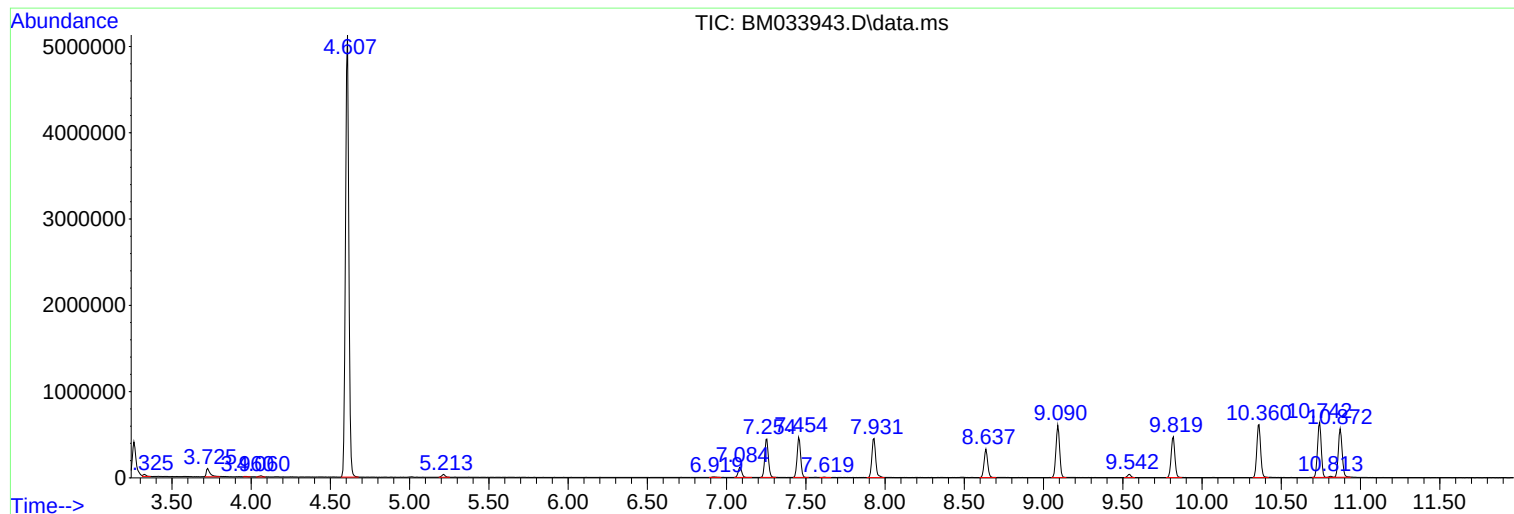

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020122\
Data File : BM033943.D
Acq On : 01 Feb 2022 17:21
Operator : CG/JU
Sample : N1273-14
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0HL2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020122\
Data File : BM033943.D
Acq On : 01 Feb 2022 17:21
Operator : CG/JU
Sample : N1273-14
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0HL2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc