

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020122\
 Data File : BM033949.D
 Acq On : 01 Feb 2022 21:30
 Operator : CG/JU
 Sample : PB142346BL
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK346

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
 Title : SVOA CALIBRATION

Signal : TIC: BM033949.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.290	5	9	18	rVB	39737	53268	2.00%	0.176%
2	3.713	77	81	98	rBV	436773	681559	25.65%	2.253%
3	4.060	137	140	144	rVB2	9483	12864	0.48%	0.043%
4	7.084	647	654	664	rBV	568204	871817	32.81%	2.882%
5	7.248	674	682	692	rBV	429463	682989	25.71%	2.258%
6	7.454	710	717	729	rVB	583615	916305	34.49%	3.029%
7	7.925	790	797	807	rVB	481680	749700	28.22%	2.478%
8	8.637	911	918	927	rBV	652569	1062819	40.00%	3.514%
9	9.089	987	995	1006	rBV	541220	887718	33.41%	2.935%
10	9.813	1111	1118	1129	rBV	460063	744154	28.01%	2.460%
11	10.354	1202	1210	1220	rBV	648200	1070361	40.29%	3.538%
12	10.419	1220	1221	1227	rVB4	4952	4395	0.17%	0.015%
13	10.736	1268	1275	1284	rBV	650335	1063887	40.04%	3.517%
14	10.872	1290	1298	1311	rBV	615728	1100457	41.42%	3.638%
15	10.960	1311	1313	1319	rVB6	3143	4738	0.18%	0.016%
16	12.330	1541	1546	1555	rBV	9464	17969	0.68%	0.059%
17	13.971	1819	1825	1838	rBV	1187069	1654622	62.28%	5.470%
18	14.260	1867	1874	1891	rBV	1241027	1847583	69.54%	6.108%
19	14.566	1918	1926	1934	rBV	957765	1372571	51.66%	4.538%
20	14.748	1951	1957	1976	rBV	373907	703146	26.46%	2.325%
21	15.554	2086	2094	2106	rBV	1598023	2282101	85.89%	7.544%
22	15.666	2107	2113	2130	rVV	528076	756294	28.46%	2.500%
23	15.789	2130	2134	2140	rVB2	10681	16165	0.61%	0.053%
24	17.083	2349	2354	2359	rBV3	3549	6635	0.25%	0.022%
25	17.301	2382	2391	2398	rBV	1066628	1517253	57.10%	5.016%
26	17.401	2401	2408	2426	rVB	1778614	2495837	93.94%	8.251%
27	19.248	2718	2722	2726	rBV2	20074	24414	0.92%	0.081%
28	19.318	2731	2734	2738	rVV2	16910	21100	0.79%	0.070%
29	19.683	2790	2796	2804	rBV	2045415	2656957	100.00%	8.784%
30	21.459	3094	3098	3108	rBV	1061493	1371559	51.62%	4.534%
31	23.694	3472	3478	3486	rBV	1164004	2300726	86.59%	7.606%
32	23.853	3499	3505	3514	rVB2	644844	1297285	48.83%	4.289%




Sum of corrected areas: 30249248

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020122\
Data File : BM033949.D
Acq On : 01 Feb 2022 21:30
Operator : CG/JU
Sample : PB142346BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK346

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

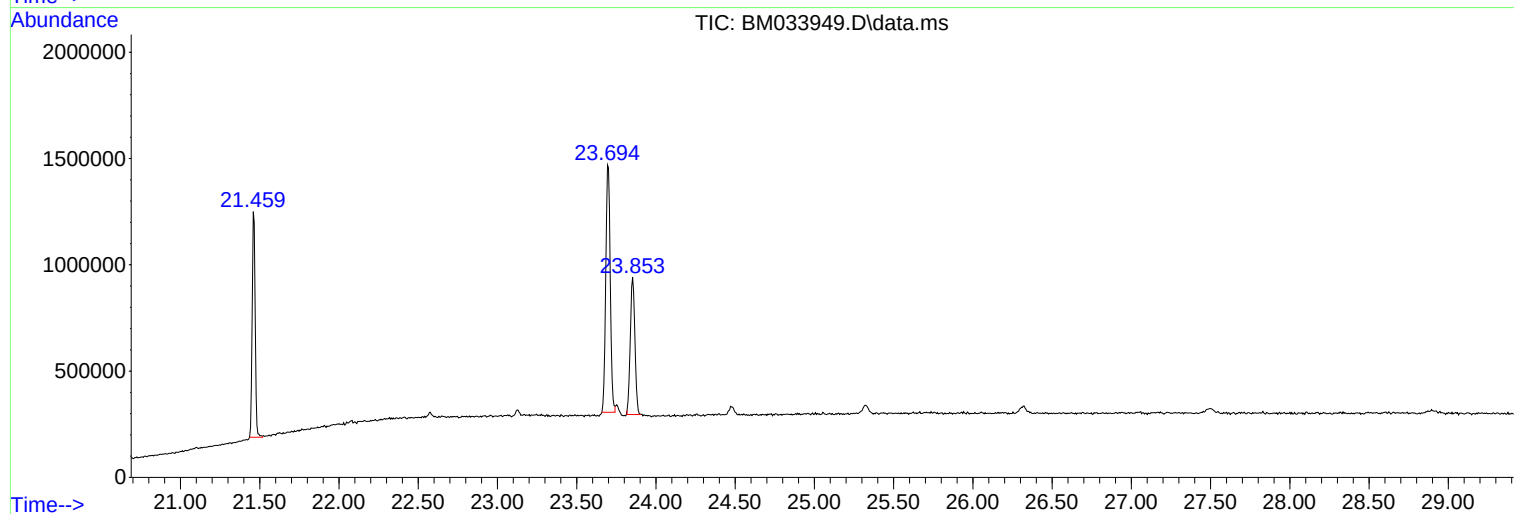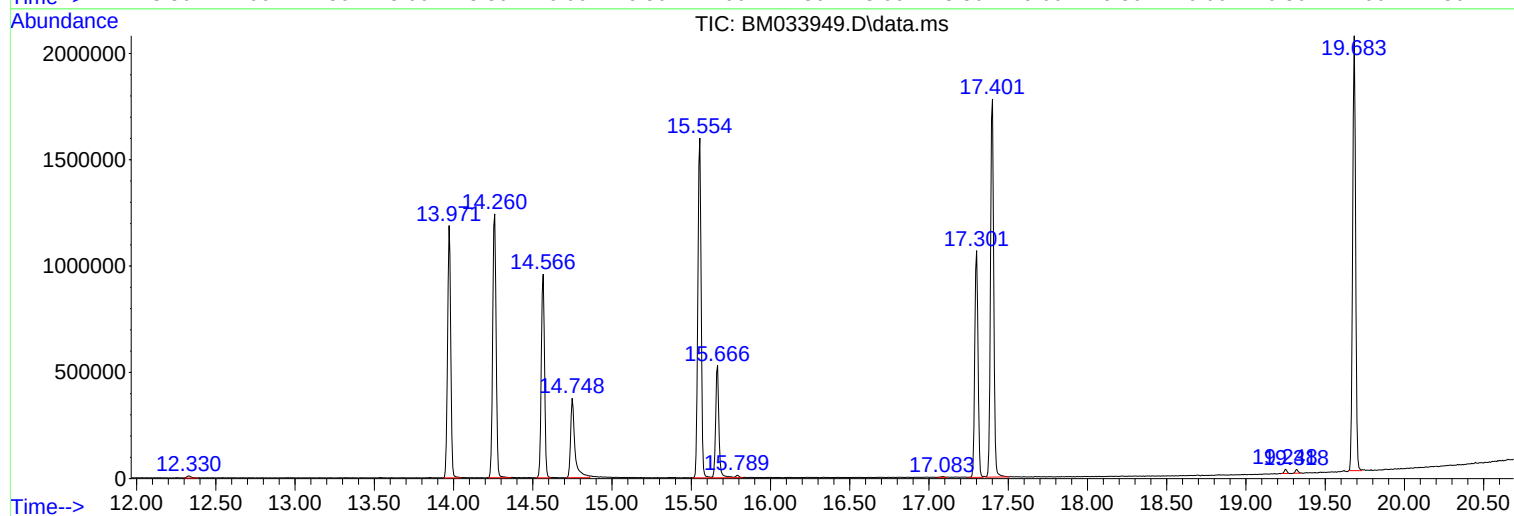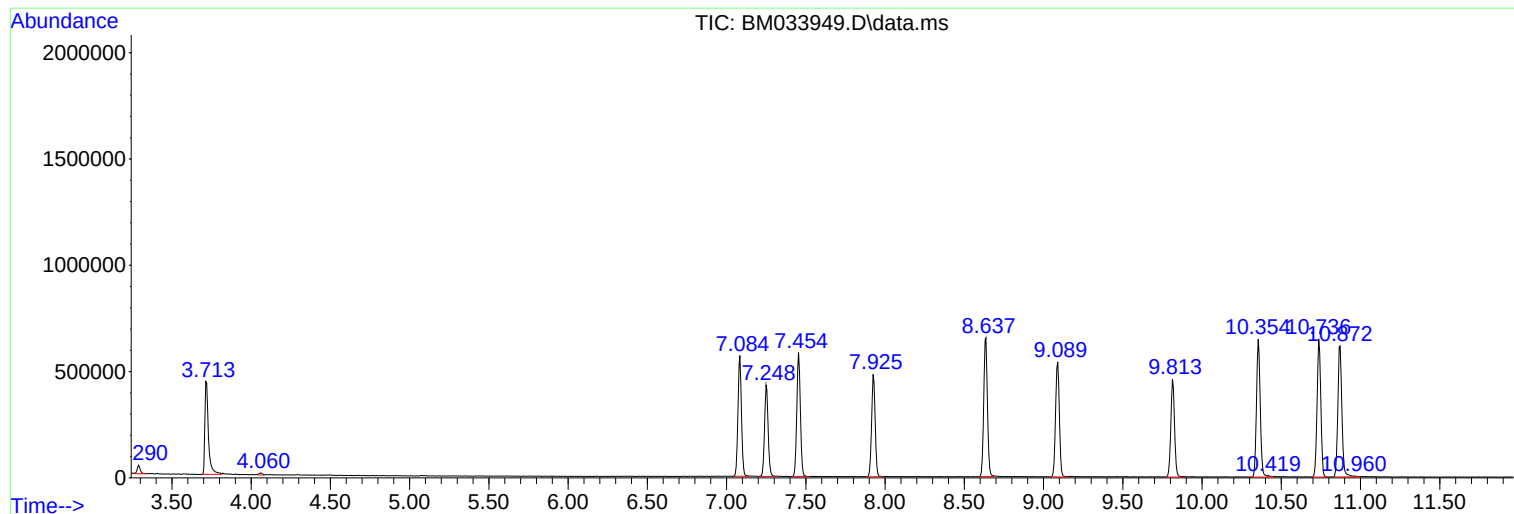

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020122\
Data File : BM033949.D
Acq On : 01 Feb 2022 21:30
Operator : CG/JU
Sample : PB142346BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK346

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020122\
Data File : BM033949.D
Acq On : 01 Feb 2022 21:30
Operator : CG/JU
Sample : PB142346BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK346

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
