

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020122\
 Data File : BM033950.D
 Acq On : 01 Feb 2022 22:05
 Operator : CG/JU
 Sample : PB142348BL
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK348

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
 Title : SVOA CALIBRATION

Signal : TIC: BM033950.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.290	5	9	18	rVB	43382	57001	1.83%	0.172%
2	3.713	77	81	104	rBV	514576	788004	25.32%	2.380%
3	4.060	136	140	145	rVB4	7787	12112	0.39%	0.037%
4	7.084	647	654	663	rBV	630991	975864	31.36%	2.948%
5	7.248	676	682	693	rVB	485195	755521	24.28%	2.282%
6	7.454	710	717	730	rVB	650974	1019186	32.75%	3.079%
7	7.925	790	797	806	rBV	420642	663247	21.31%	2.003%
8	8.631	909	917	929	rBV	754828	1218163	39.14%	3.680%
9	9.089	987	995	1005	rBV	616510	1007904	32.39%	3.045%
10	9.813	1111	1118	1129	rBV	515190	847704	27.24%	2.561%
11	10.354	1203	1210	1225	rBV	747120	1225951	39.39%	3.703%
12	10.736	1268	1275	1285	rVB	581786	956276	30.73%	2.889%
13	10.872	1290	1298	1315	rBV	732372	1271075	40.84%	3.840%
14	12.330	1540	1546	1553	rBV3	10154	17331	0.56%	0.052%
15	13.971	1819	1825	1837	rBV	1428308	1930241	62.02%	5.831%
16	14.260	1867	1874	1883	rBV	1500404	2129133	68.41%	6.431%
17	14.565	1919	1926	1933	rBV	865371	1250950	40.19%	3.779%
18	14.748	1951	1957	1975	rBV	476412	839061	26.96%	2.535%
19	14.924	1985	1987	1990	rVB4	2862	3377	0.11%	0.010%
20	14.977	1990	1996	1998	rVV6	2340	4070	0.13%	0.012%
21	15.554	2087	2094	2105	rBV	1870780	2630371	84.52%	7.945%
22	15.665	2107	2113	2128	rVV	621478	888916	28.56%	2.685%
23	15.789	2130	2134	2139	rVB	11318	17986	0.58%	0.054%
24	17.089	2351	2355	2359	rBV3	4038	5491	0.18%	0.017%
25	17.301	2384	2391	2401	rBV	1017830	1399861	44.98%	4.229%
26	17.401	2401	2408	2421	rVV	2039670	2896190	93.06%	8.748%
27	19.253	2718	2723	2727	rBV3	22103	30891	0.99%	0.093%
28	19.318	2731	2734	2740	rVB	19247	28370	0.91%	0.086%
29	19.683	2790	2796	2805	rBV	2427174	3112244	100.00%	9.401%
30	21.459	3094	3098	3106	rBV	975640	1267076	40.71%	3.827%
31	23.700	3472	3479	3487	rBV2	1309909	2624965	84.34%	7.929%
32	23.853	3499	3505	3516	rVB2	591749	1230641	39.54%	3.717%




Sum of corrected areas: 33105173

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020122\
Data File : BM033950.D
Acq On : 01 Feb 2022 22:05
Operator : CG/JU
Sample : PB142348BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK348

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

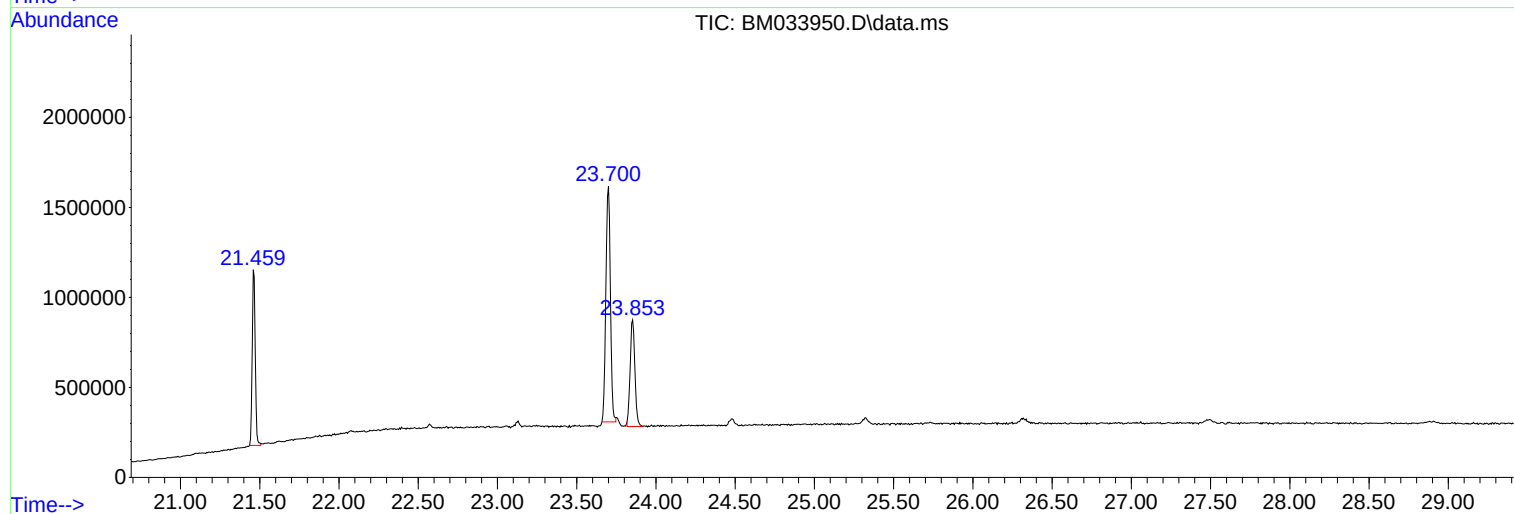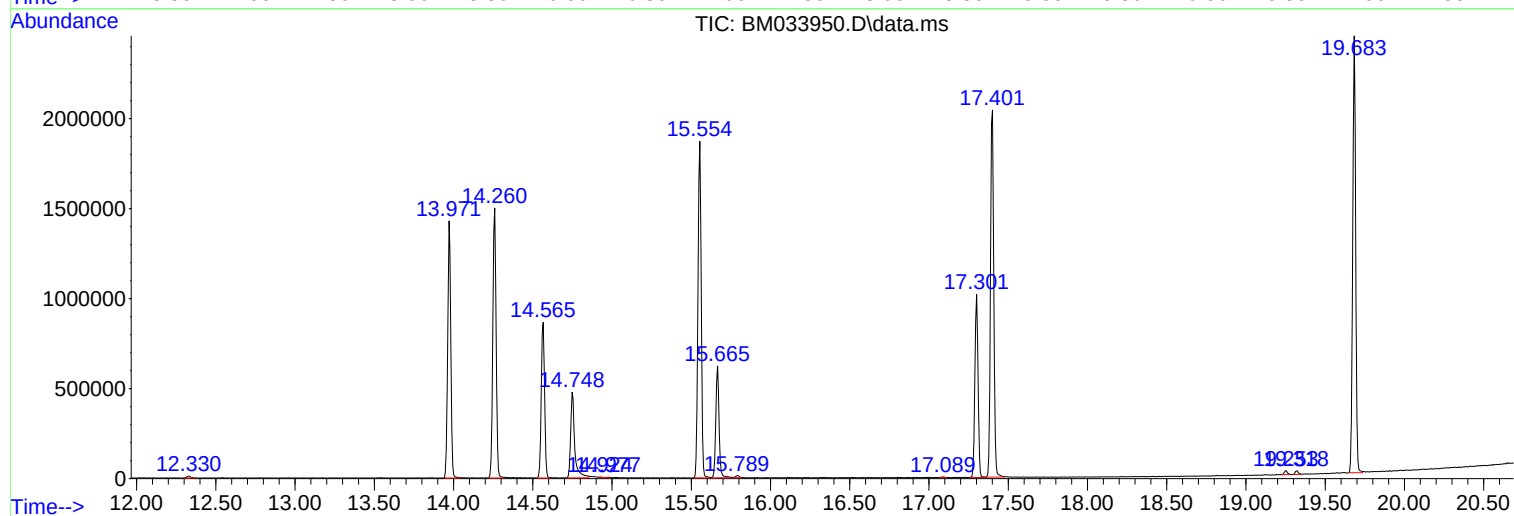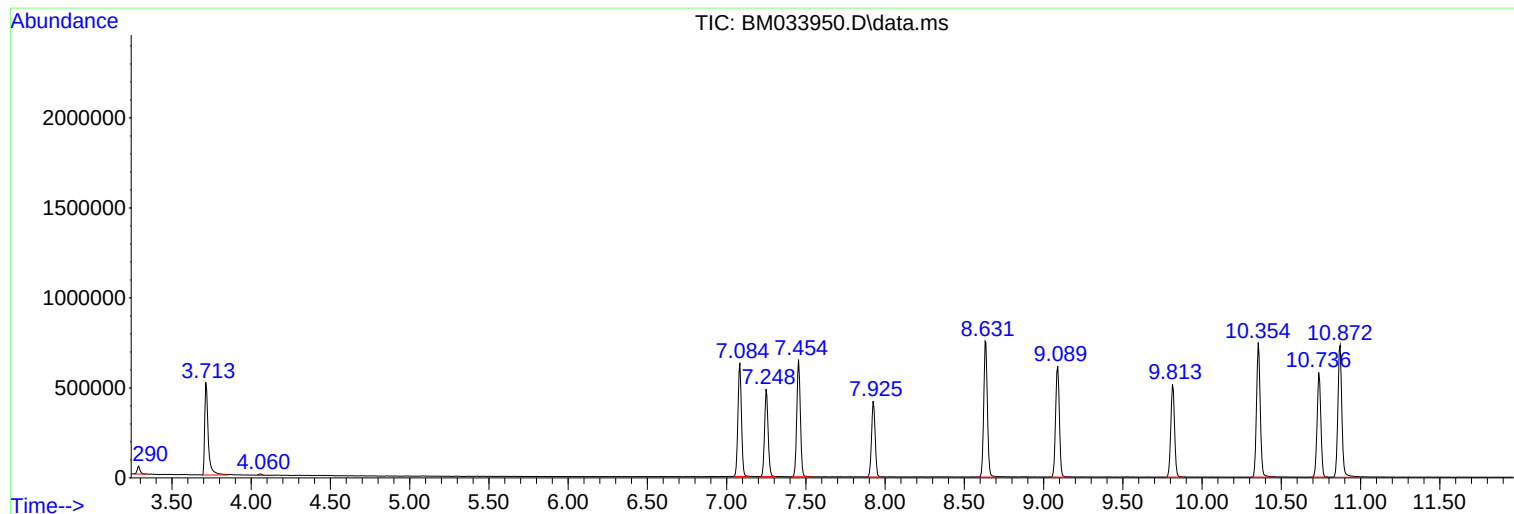

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020122\
Data File : BM033950.D
Acq On : 01 Feb 2022 22:05
Operator : CG/JU
Sample : PB142348BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK348

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020122\
Data File : BM033950.D
Acq On : 01 Feb 2022 22:05
Operator : CG/JU
Sample : PB142348BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK348

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------