

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020122\
 Data File : BM033952.D
 Acq On : 01 Feb 2022 23:16
 Operator : CG/JU
 Sample : N1307-04
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0Q33

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
 Title : SVOA CALIBRATION

Signal : TIC: BM033952.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.290	5	9	14	rBV	27474	34894	1.37%	0.127%
2	3.720	79	82	95	rBV	134652	211670	8.34%	0.770%
3	3.961	121	123	129	rVB6	5867	9630	0.38%	0.035%
4	4.061	137	140	146	rVB3	7697	10253	0.40%	0.037%
5	4.290	175	179	184	rVB8	5035	8379	0.33%	0.030%
6	4.714	247	251	254	rBV5	2534	3213	0.13%	0.012%
7	5.014	298	302	307	rVB5	4713	7559	0.30%	0.027%
8	6.825	609	610	614	rBV3	2170	2580	0.10%	0.009%
9	7.084	648	654	667	rVB	117850	208205	8.20%	0.757%
10	7.249	676	682	691	rBV	431854	671113	26.44%	2.441%
11	7.455	710	717	727	rBV	444360	700037	27.58%	2.546%
12	7.555	731	734	739	rVB6	2760	3758	0.15%	0.014%
13	7.925	789	797	805	rBV	456643	709361	27.95%	2.580%
14	7.996	805	809	812	rVB3	5507	7558	0.30%	0.027%
15	8.631	911	917	929	rBV	331386	540035	21.28%	1.964%
16	9.090	986	995	1006	rBV	524649	881880	34.75%	3.207%
17	9.266	1020	1025	1026	rBV4	3139	3464	0.14%	0.013%
18	9.537	1066	1071	1077	rVB	15166	23437	0.92%	0.085%
19	9.813	1111	1118	1127	rBV	435841	702760	27.69%	2.556%
20	10.354	1203	1210	1225	rBV	596152	986083	38.85%	3.586%
21	10.525	1235	1239	1244	rBV5	8521	15131	0.60%	0.055%
22	10.737	1268	1275	1283	rBV	610537	1011891	39.87%	3.680%
23	10.872	1290	1298	1313	rBV	507379	912605	35.96%	3.319%
24	11.395	1382	1387	1391	rVB7	2391	4807	0.19%	0.017%
25	12.037	1491	1496	1502	rBV6	2104	3823	0.15%	0.014%
26	12.166	1514	1518	1523	rBV7	2675	4146	0.16%	0.015%
27	12.325	1540	1545	1551	rVB2	9383	15891	0.63%	0.058%
28	12.978	1653	1656	1660	rVB6	2672	3491	0.14%	0.013%
29	13.184	1685	1691	1695	rBV4	3679	5583	0.22%	0.020%
30	13.401	1724	1728	1734	rVB	8728	13110	0.52%	0.048%
31	13.472	1737	1740	1744	rVB3	2099	2744	0.11%	0.010%
32	13.542	1749	1752	1756	rVB3	2992	3531	0.14%	0.013%
33	13.972	1819	1825	1831	rBV	1227737	1632564	64.32%	5.937%
34	14.107	1842	1848	1854	rVB4	9968	16057	0.63%	0.058%
35	14.213	1861	1866	1867	rBV5	9414	10899	0.43%	0.040%
36	14.260	1867	1874	1888	rVB	1235847	1858700	73.23%	6.759%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020122\
 Data File : BM033952.D
 Acq On : 01 Feb 2022 23:16
 Operator : CG/JU
 Sample : N1307-04
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0Q33

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
 Title : SVOA CALIBRATION

37	14.472	1905	1910	1914	rVB	6818	10015	0.39%	0.036%
38	14.566	1919	1926	1936	rBV	885491	1287253	50.72%	4.681%
39	14.754	1953	1958	1977	rBV2	39995	102030	4.02%	0.371%
40	14.972	1990	1995	2002	rVB8	5173	10332	0.41%	0.038%
41	15.148	2022	2025	2029	rVV7	2770	3893	0.15%	0.014%
42	15.195	2029	2033	2038	rVB	7337	9210	0.36%	0.033%
43	15.301	2046	2051	2056	rVB5	2681	3622	0.14%	0.013%
44	15.378	2056	2064	2068	rBV	99969	138676	5.46%	0.504%
45	15.413	2068	2070	2075	rVB2	8300	10586	0.42%	0.038%
46	15.554	2087	2094	2103	rBV	1568720	2279665	89.82%	8.290%
47	15.666	2107	2113	2123	rVV	459681	660041	26.01%	2.400%
48	15.795	2129	2135	2143	rBV5	9982	17003	0.67%	0.062%
49	15.913	2152	2155	2161	rVB6	3198	4805	0.19%	0.017%
50	15.966	2161	2164	2167	rBV3	5369	5780	0.23%	0.021%
51	16.025	2172	2174	2179	rVB5	1895	3767	0.15%	0.014%
52	16.189	2199	2202	2204	rBV3	2379	2593	0.10%	0.009%
53	16.230	2205	2209	2212	rBV6	5371	6588	0.26%	0.024%
54	16.272	2212	2216	2219	rBV4	7790	8217	0.32%	0.030%
55	16.336	2225	2227	2232	rVB6	4389	5616	0.22%	0.020%
56	16.448	2242	2246	2249	rBV3	6384	7098	0.28%	0.026%
57	16.619	2271	2275	2277	rBV4	2200	2929	0.12%	0.011%
58	16.677	2282	2285	2287	rBV3	2588	2815	0.11%	0.010%
59	16.777	2298	2302	2309	rBV9	2998	5897	0.23%	0.021%
60	16.954	2328	2332	2340	rVB4	24434	36890	1.45%	0.134%
61	17.019	2340	2343	2345	rBV4	2587	3130	0.12%	0.011%
62	17.066	2348	2351	2353	rBV3	7563	8385	0.33%	0.030%
63	17.219	2372	2377	2384	rVB7	6677	11287	0.44%	0.041%
64	17.301	2384	2391	2401	rBV	946009	1388319	54.70%	5.049%
65	17.395	2401	2407	2422	rVV	1672711	2378884	93.73%	8.651%
66	17.601	2440	2442	2446	rVB5	3048	3214	0.13%	0.012%
67	17.801	2473	2476	2479	rBV4	3160	4144	0.16%	0.015%
68	17.972	2502	2505	2508	rBV4	8814	9268	0.37%	0.034%
69	18.101	2522	2527	2533	rVB9	3000	7307	0.29%	0.027%
70	18.195	2538	2543	2551	rBV	75017	123099	4.85%	0.448%
71	18.448	2584	2586	2589	rBV3	3174	4118	0.16%	0.015%
72	18.560	2603	2605	2609	rBV4	2694	3641	0.14%	0.013%
73	19.248	2718	2722	2726	rBV2	20219	31144	1.23%	0.113%
74	19.318	2731	2734	2738	rVV2	21505	27741	1.09%	0.101%
75	19.466	2755	2759	2765	rBV3	61886	92639	3.65%	0.337%
76	19.683	2790	2796	2804	rBV	1946397	2538039	100.00%	9.230%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020122\
Data File : BM033952.D
Acq On : 01 Feb 2022 23:16
Operator : CG/JU
Sample : N1307-04
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0Q33

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
Title : SVOA CALIBRATION

77	21.177	3046	3050	3056	rBV3	75062	112768	4.44%	0.410%
78	21.460	3093	3098	3103	rBV	1026626	1297627	51.13%	4.719%
79	23.695	3472	3478	3485	rBV	1228236	2266335	89.29%	8.242%
80	23.853	3498	3505	3515	rVB2	632751	1320724	52.04%	4.803%


Sum of corrected areas: 27497976

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020122\
Data File : BM033952.D
Acq On : 01 Feb 2022 23:16
Operator : CG/JU
Sample : N1307-04
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0Q33

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

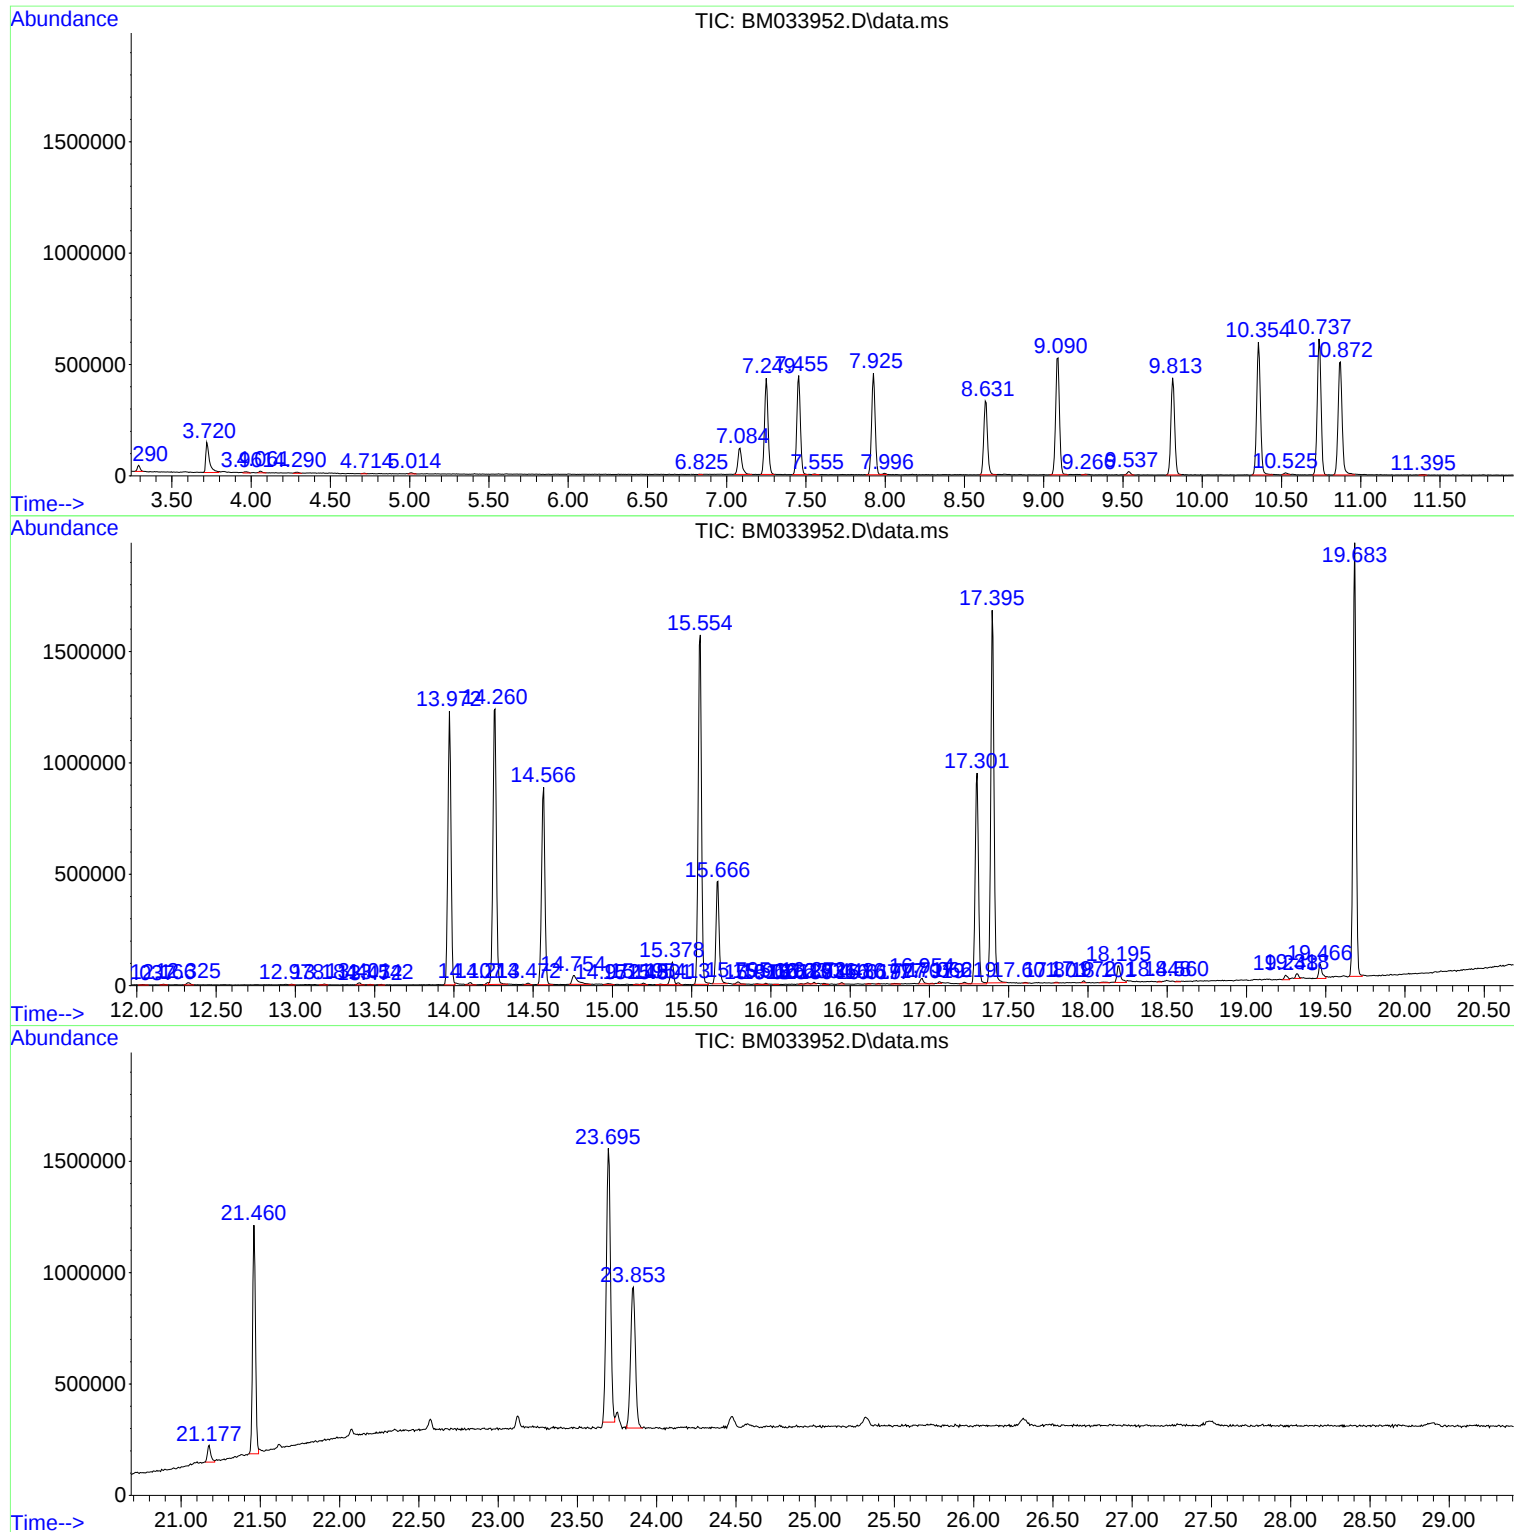

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020122\
Data File : BM033952.D
Acq On : 01 Feb 2022 23:16
Operator : CG/JU
Sample : N1307-04
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0Q33

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020122\
Data File : BM033952.D
Acq On : 01 Feb 2022 23:16
Operator : CG/JU
Sample : N1307-04
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0Q33

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc