

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020122\
 Data File : BM033953.D
 Acq On : 01 Feb 2022 23:51
 Operator : CG/JU
 Sample : N1273-16
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 COHL4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
 Title : SVOA CALIBRATION

Signal : TIC: BM033953.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.325	12	15	32	rVB	383514	557302	2.01%	0.907%
2	3.725	80	83	91	rBV	84445	135816	0.49%	0.221%
3	4.160	152	157	163	rVB	25158	36892	0.13%	0.060%
4	4.607	225	233	247	rBV	18247689	27681447	100.00%	45.073%
5	7.084	648	654	664	rVB	116414	195592	0.71%	0.318%
6	7.248	675	682	695	rBV	516891	804391	2.91%	1.310%
7	7.454	710	717	728	rBV	506321	783646	2.83%	1.276%
8	7.613	739	744	750	rVB2	41083	63943	0.23%	0.104%
9	7.925	790	797	805	rBV	476118	753671	2.72%	1.227%
10	8.631	908	917	928	rBV	358674	581012	2.10%	0.946%
11	9.090	987	995	1006	rBV	660277	1082650	3.91%	1.763%
12	9.813	1110	1118	1127	rBV	542665	878021	3.17%	1.430%
13	10.354	1203	1210	1222	rBV	703699	1166104	4.21%	1.899%
14	10.525	1234	1239	1250	rBV2	11904	27785	0.10%	0.045%
15	10.737	1268	1275	1283	rVB	666393	1097358	3.96%	1.787%
16	10.872	1291	1298	1313	rVB	617212	1071216	3.87%	1.744%
17	13.972	1818	1825	1831	rBV	1560712	2070289	7.48%	3.371%
18	14.260	1862	1874	1890	rBV	1635129	2416156	8.73%	3.934%
19	14.566	1918	1926	1935	rBV	995009	1484948	5.36%	2.418%
20	14.754	1950	1958	1972	rBV2	48604	122429	0.44%	0.199%
21	15.554	2087	2094	2106	rBV	2121352	3001661	10.84%	4.888%
22	15.666	2106	2113	2124	rBV	662638	942701	3.41%	1.535%
23	17.301	2384	2391	2401	rBV	1176783	1672423	6.04%	2.723%
24	17.401	2401	2408	2420	rBV	2322780	3301230	11.93%	5.375%
25	17.971	2500	2505	2509	rBV	41515	52003	0.19%	0.085%
26	19.254	2718	2723	2727	rBV2	27270	42657	0.15%	0.069%
27	19.318	2730	2734	2741	rVB	25709	38507	0.14%	0.063%
28	19.683	2790	2796	2802	rBV	2711422	3473570	12.55%	5.656%
29	21.171	3047	3049	3055	rVB6	33484	43047	0.16%	0.070%
30	21.459	3093	3098	3108	rBV	1237943	1538363	5.56%	2.505%
31	23.694	3471	3478	3485	rBV2	1443209	2891794	10.45%	4.709%
32	23.847	3498	3504	3515	rVB2	694109	1405727	5.08%	2.289%




Sum of corrected areas: 61414351

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020122\
Data File : BM033953.D
Acq On : 01 Feb 2022 23:51
Operator : CG/JU
Sample : N1273-16
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
COHL4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

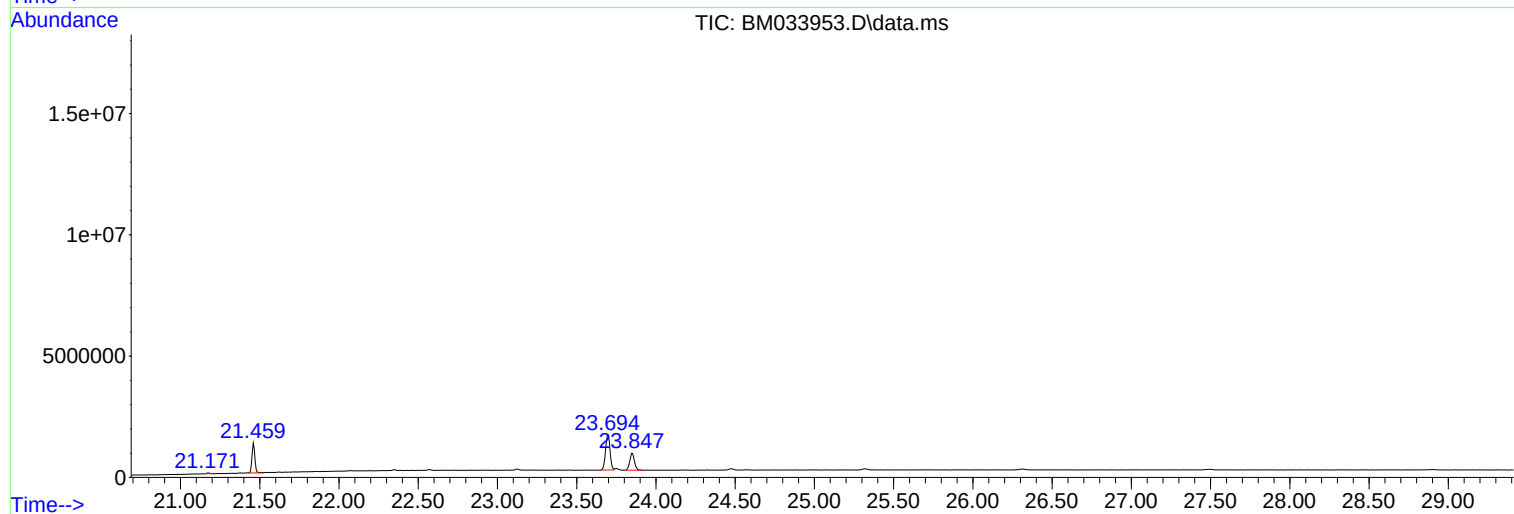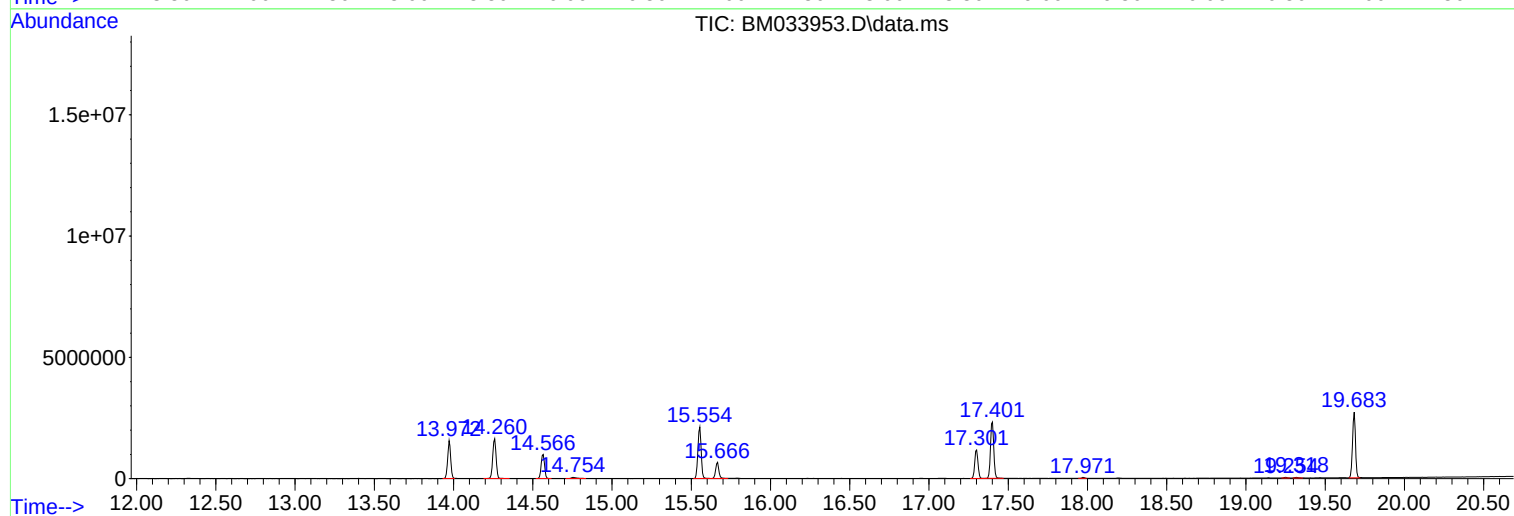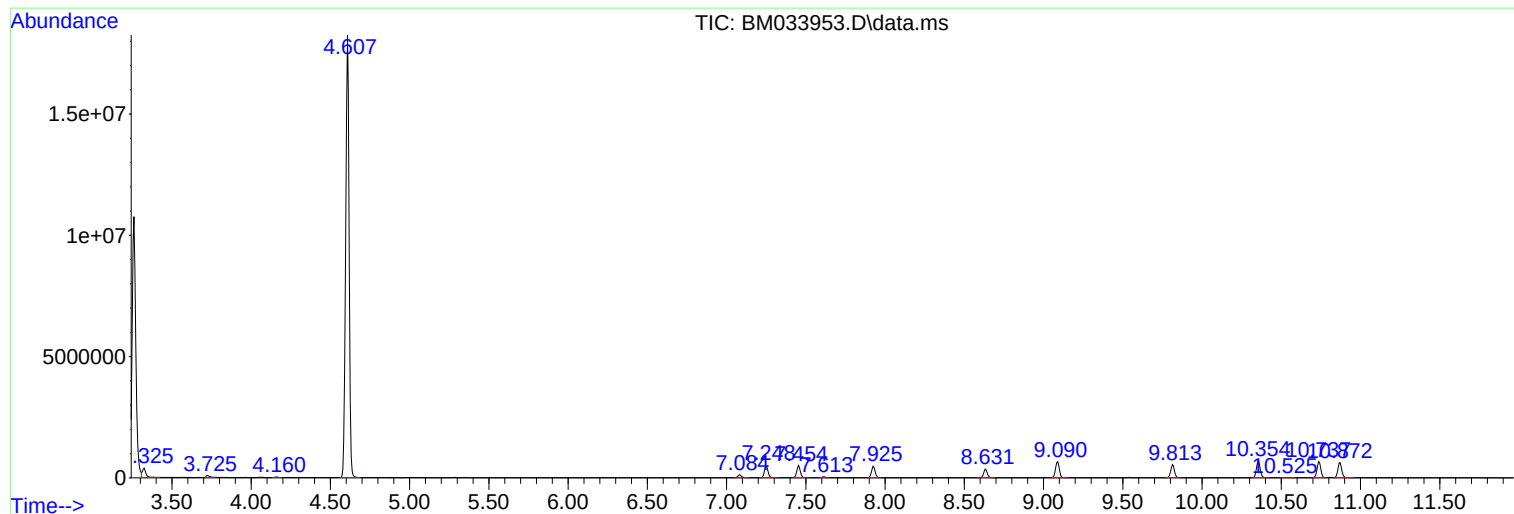

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020122\
Data File : BM033953.D
Acq On : 01 Feb 2022 23:51
Operator : CG/JU
Sample : N1273-16
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0HL4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020122\
Data File : BM033953.D
Acq On : 01 Feb 2022 23:51
Operator : CG/JU
Sample : N1273-16
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0HL4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc