

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020122\
 Data File : BM033955.D
 Acq On : 02 Feb 2022 01:02
 Operator : CG/JU
 Sample : N1307-06
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0Q04

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
 Title : SVOA CALIBRATION

Signal : TIC: BM033955.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.290	5	9	15	rVB	26075	32663	1.07%	0.105%
2	3.731	81	84	98	rBV	37206	63677	2.08%	0.204%
3	4.054	136	139	144	rVB2	9723	15052	0.49%	0.048%
4	5.013	297	302	306	rVB3	4253	6095	0.20%	0.020%
5	6.472	545	550	554	rBV6	2208	3321	0.11%	0.011%
6	7.084	647	654	668	rVB	125530	222894	7.28%	0.713%
7	7.248	676	682	691	rBV	453341	702851	22.96%	2.250%
8	7.454	710	717	725	rBV	473087	734112	23.98%	2.350%
9	7.554	730	734	737	rBV5	2907	4666	0.15%	0.015%
10	7.925	791	797	805	rBV	483714	755638	24.68%	2.419%
11	7.990	805	808	814	rBV6	4730	7296	0.24%	0.023%
12	8.631	911	917	926	rBV	341978	552866	18.06%	1.770%
13	8.766	935	940	946	rVB9	3708	8404	0.27%	0.027%
14	9.089	987	995	1005	rBV	554432	923676	30.17%	2.956%
15	9.201	1010	1014	1019	rVB6	3799	6781	0.22%	0.022%
16	9.266	1022	1025	1033	rVB6	3523	6015	0.20%	0.019%
17	9.536	1065	1071	1076	rBV	14716	20783	0.68%	0.067%
18	9.813	1111	1118	1128	rBV	465282	757096	24.73%	2.423%
19	10.354	1203	1210	1222	rBV	626443	1034678	33.80%	3.312%
20	10.519	1233	1238	1247	rBV4	14155	28805	0.94%	0.092%
21	10.736	1267	1275	1283	rVB	674307	1095679	35.79%	3.507%
22	10.872	1290	1298	1311	rBV	299267	553122	18.07%	1.770%
23	11.530	1405	1410	1411	rBV4	3172	4562	0.15%	0.015%
24	12.166	1514	1518	1522	rBV5	2604	4328	0.14%	0.014%
25	12.325	1541	1545	1552	rVB2	11299	18566	0.61%	0.059%
26	12.942	1644	1650	1653	rBV6	2649	4433	0.14%	0.014%
27	13.183	1685	1691	1696	rVB5	4692	8982	0.29%	0.029%
28	13.401	1725	1728	1734	rVB2	12106	14514	0.47%	0.046%
29	13.477	1736	1741	1747	rVB7	2193	3849	0.13%	0.012%
30	13.542	1747	1752	1755	rBV6	2618	4741	0.15%	0.015%
31	13.848	1798	1804	1807	rBV7	3952	6367	0.21%	0.020%
32	13.971	1818	1825	1837	rBV	1379176	1866625	60.98%	5.974%
33	14.048	1837	1838	1844	rVB5	3454	4467	0.15%	0.014%
34	14.213	1861	1866	1867	rVV3	12597	15154	0.50%	0.049%
35	14.254	1867	1873	1886	rVV	1345958	2022208	66.06%	6.472%
36	14.348	1888	1889	1894	rVB5	2303	3402	0.11%	0.011%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020122\
 Data File : BM033955.D
 Acq On : 02 Feb 2022 01:02
 Operator : CG/JU
 Sample : N1307-06
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0Q04

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
 Title : SVOA CALIBRATION

37	14.466	1904	1909	1914	rVB4	7620	12491	0.41%	0.040%
38	14.566	1919	1926	1934	rBV	949327	1394564	45.56%	4.463%
39	14.754	1953	1958	1966	rBV	62681	123415	4.03%	0.395%
40	14.924	1981	1987	1990	rVB8	3005	6443	0.21%	0.021%
41	14.971	1990	1995	1999	rBV5	6307	9972	0.33%	0.032%
42	15.101	2009	2017	2020	rBV10	5644	12351	0.40%	0.040%
43	15.148	2020	2025	2028	rVV6	11444	18888	0.62%	0.060%
44	15.189	2028	2032	2038	rVB3	13586	23853	0.78%	0.076%
45	15.371	2057	2063	2067	rBV3	9850	17413	0.57%	0.056%
46	15.413	2067	2070	2073	rVB3	6790	6835	0.22%	0.022%
47	15.554	2087	2094	2102	rBV	1786149	2602643	85.02%	8.330%
48	15.665	2106	2113	2126	rVB	599119	874180	28.56%	2.798%
49	15.795	2131	2135	2142	rVB2	14047	28475	0.93%	0.091%
50	15.913	2152	2155	2158	rVB5	4121	5781	0.19%	0.019%
51	15.965	2158	2164	2168	rBV7	5571	9868	0.32%	0.032%
52	16.189	2199	2202	2206	rBV6	4799	7883	0.26%	0.025%
53	16.230	2206	2209	2213	rVV4	7071	11079	0.36%	0.035%
54	16.271	2213	2216	2219	rVV5	10278	14785	0.48%	0.047%
55	16.295	2219	2220	2224	rVV4	10980	11520	0.38%	0.037%
56	16.330	2224	2226	2231	rVB6	5580	7373	0.24%	0.024%
57	16.442	2242	2245	2249	rVB3	7530	7389	0.24%	0.024%
58	16.536	2260	2261	2266	rBV5	2846	4443	0.15%	0.014%
59	16.612	2270	2274	2275	rBV4	3816	4852	0.16%	0.016%
60	16.777	2298	2302	2305	rBV5	7134	8884	0.29%	0.028%
61	16.948	2326	2331	2340	rBV	542859	766409	25.04%	2.453%
62	17.065	2348	2351	2353	rBV3	8912	10911	0.36%	0.035%
63	17.112	2357	2359	2364	rVB5	9115	12367	0.40%	0.040%
64	17.224	2375	2378	2381	rBV5	5816	6088	0.20%	0.019%
65	17.301	2384	2391	2397	rBV	1073511	1516123	49.53%	4.853%
66	17.395	2401	2407	2418	rBV	1965063	2854944	93.26%	9.138%
67	17.859	2483	2486	2487	rBV3	3667	3464	0.11%	0.011%
68	17.918	2493	2496	2500	rVB6	9252	11622	0.38%	0.037%
69	17.971	2500	2505	2511	rVB7	9602	15798	0.52%	0.051%
70	18.083	2522	2524	2528	rVB5	4037	5139	0.17%	0.016%
71	18.195	2538	2543	2550	rBV	92739	142666	4.66%	0.457%
72	19.248	2718	2722	2725	rBV2	25226	36085	1.18%	0.115%
73	19.318	2730	2734	2737	rBV	27644	35000	1.14%	0.112%
74	19.465	2755	2759	2768	rBV2	70229	109228	3.57%	0.350%
75	19.683	2790	2796	2806	rVB	2338286	3061254	100.00%	9.798%
76	21.177	3046	3050	3058	rBV6	73292	122292	3.99%	0.391%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020122\
Data File : BM033955.D
Acq On : 02 Feb 2022 01:02
Operator : CG/JU
Sample : N1307-06
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0Q04

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
Title : SVOA CALIBRATION

77	21.459	3093	3098	3104	rBV	1190829	1468065	47.96%	4.699%
78	23.694	3471	3478	3485	rBV2	1447509	2861029	93.46%	9.157%
79	23.847	3498	3504	3513	rVB2	745545	1461753	47.75%	4.679%


Sum of corrected areas: 31243985

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020122\
Data File : BM033955.D
Acq On : 02 Feb 2022 01:02
Operator : CG/JU
Sample : N1307-06
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0Q04

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

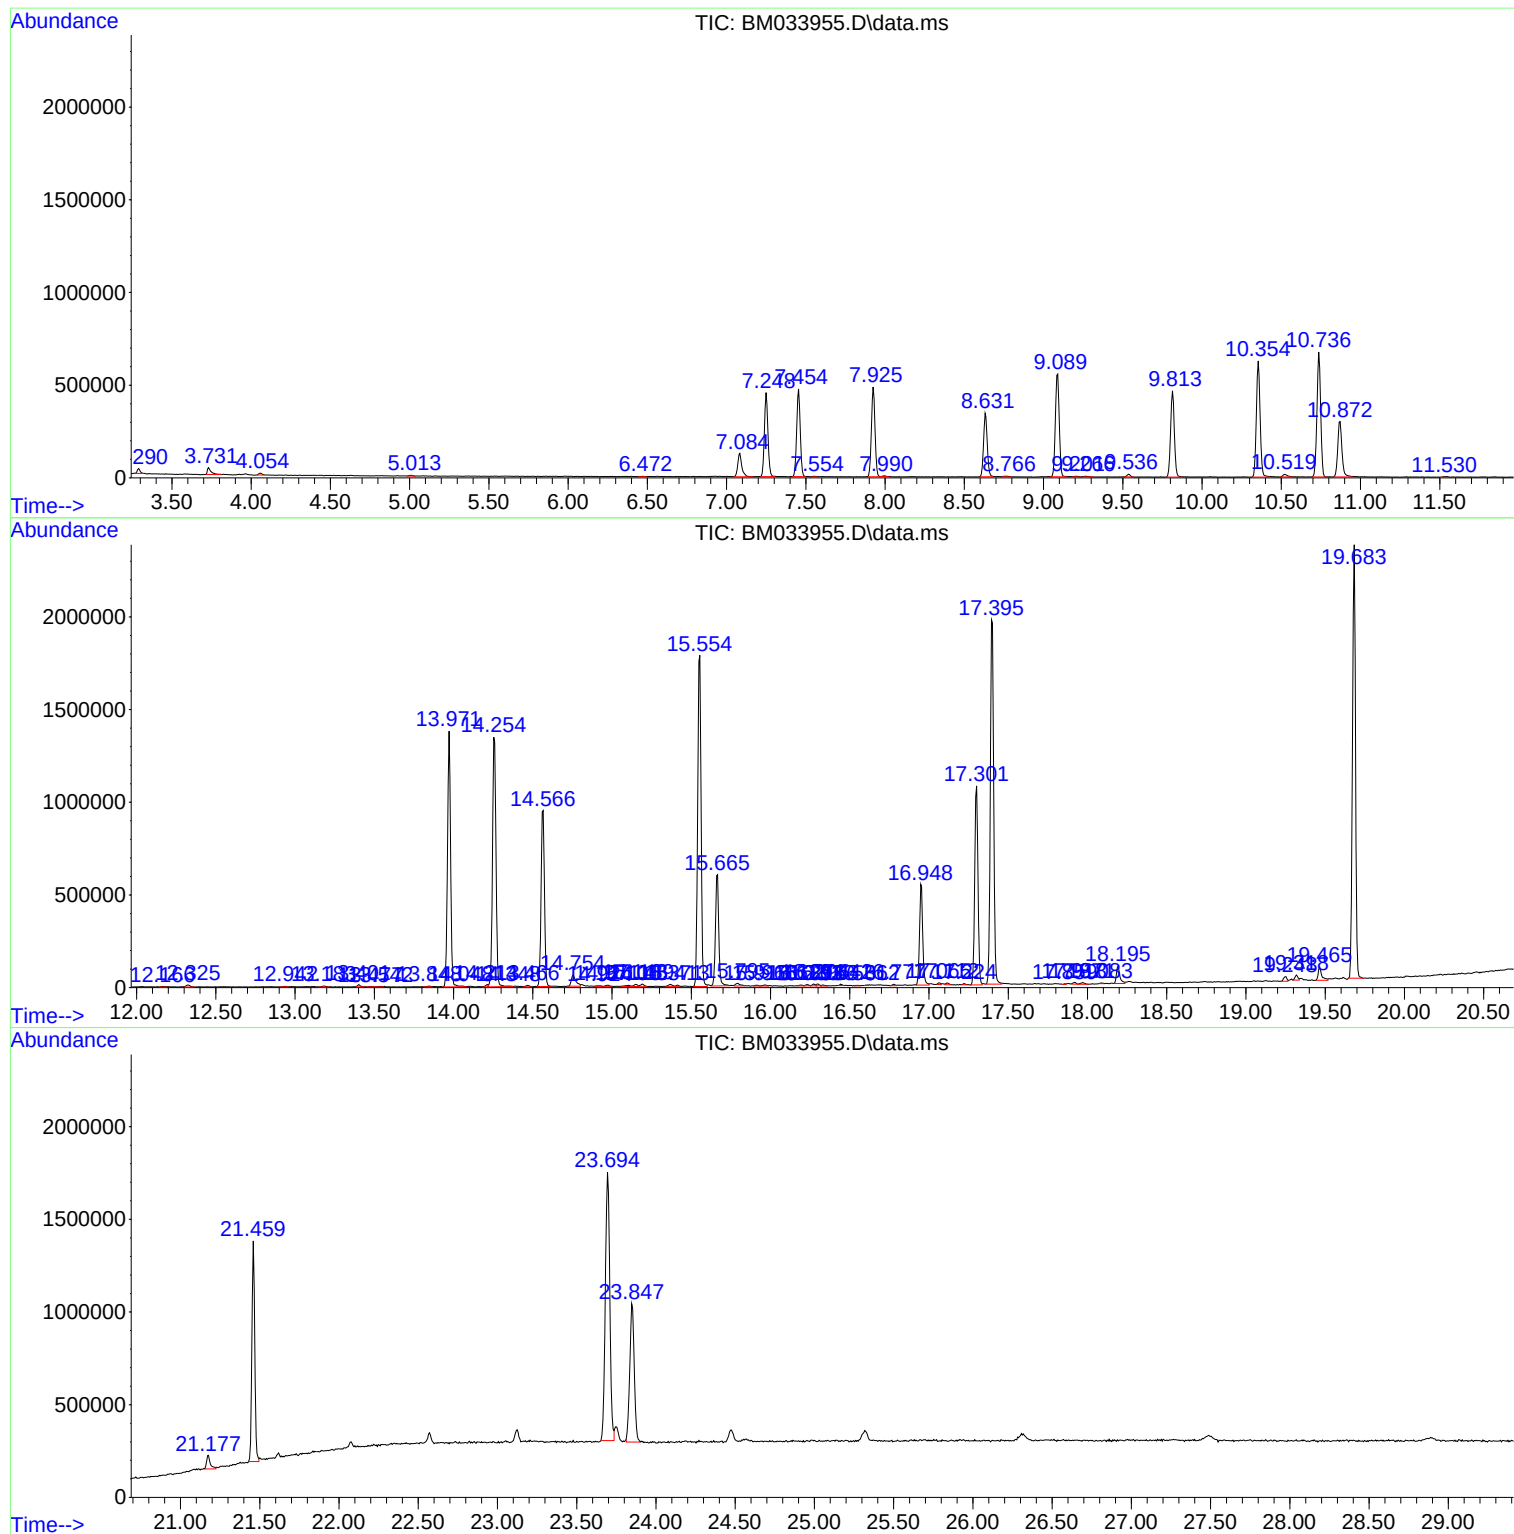

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020122\
Data File : BM033955.D
Acq On : 02 Feb 2022 01:02
Operator : CG/JU
Sample : N1307-06
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0Q04

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020122\
Data File : BM033955.D
Acq On : 02 Feb 2022 01:02
Operator : CG/JU
Sample : N1307-06
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0Q04

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------