

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020122\
 Data File : BM033958.D
 Acq On : 02 Feb 2022 02:49
 Operator : CG/JU
 Sample : N1307-02
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0Q11

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
 Title : SVOA CALIBRATION

Signal : TIC: BM033958.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.290	5	9	14	rBV	29025	36990	1.10%	0.112%
2	3.578	55	58	62	rBV5	2686	4522	0.13%	0.014%
3	3.725	80	83	94	rBV	47047	84115	2.50%	0.254%
4	4.055	137	139	144	rVB2	7909	9741	0.29%	0.029%
5	5.007	298	301	306	rVB5	4805	6027	0.18%	0.018%
6	7.084	648	654	666	rVB	137036	222942	6.63%	0.673%
7	7.248	675	682	693	rVB	495531	784533	23.33%	2.367%
8	7.454	709	717	728	rBV	509620	807118	24.00%	2.435%
9	7.925	790	797	805	rBV	515938	803350	23.89%	2.424%
10	7.995	805	809	816	rVB5	4280	6316	0.19%	0.019%
11	8.631	910	917	928	rBV	379449	616723	18.34%	1.861%
12	8.760	933	939	942	rVB7	2225	4445	0.13%	0.013%
13	9.090	987	995	1003	rBV	639829	1054699	31.36%	3.182%
14	9.537	1066	1071	1076	rVB	21200	31123	0.93%	0.094%
15	9.813	1111	1118	1132	rBV	531008	879900	26.16%	2.655%
16	10.354	1203	1210	1222	rBV	716039	1191357	35.43%	3.595%
17	10.537	1237	1241	1245	rVB6	2612	3786	0.11%	0.011%
18	10.736	1268	1275	1283	rBV	711847	1189459	35.37%	3.589%
19	10.872	1289	1298	1309	rBV	470695	845311	25.14%	2.551%
20	12.036	1489	1496	1501	rBV3	8586	13273	0.39%	0.040%
21	12.325	1540	1545	1550	rBV	12535	19821	0.59%	0.060%
22	13.401	1724	1728	1734	rVB6	5429	7862	0.23%	0.024%
23	13.972	1819	1825	1837	rBV	1524335	2064348	61.38%	6.229%
24	14.260	1862	1874	1885	rBV	1578860	2325662	69.15%	7.017%
25	14.472	1904	1910	1914	rVB4	4425	7137	0.21%	0.022%
26	14.566	1919	1926	1935	rVV	1069354	1600820	47.60%	4.830%
27	14.624	1935	1936	1943	rVB6	2270	3800	0.11%	0.011%
28	14.754	1952	1958	1976	rBV2	62613	146260	4.35%	0.441%
29	14.919	1985	1986	1992	rVB6	3690	4228	0.13%	0.013%
30	15.195	2028	2033	2036	rBV4	3823	6975	0.21%	0.021%
31	15.371	2057	2063	2066	rBV6	4257	7623	0.23%	0.023%
32	15.419	2066	2071	2074	rVB5	4315	5725	0.17%	0.017%
33	15.554	2087	2094	2107	rBV	2006669	2911693	86.58%	8.786%
34	15.666	2107	2113	2127	rVV	669307	988096	29.38%	2.981%
35	15.789	2131	2134	2139	rVB2	13727	18587	0.55%	0.056%
36	15.966	2161	2164	2168	rVB5	2760	4378	0.13%	0.013%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020122\
 Data File : BM033958.D
 Acq On : 02 Feb 2022 02:49
 Operator : CG/JU
 Sample : N1307-02
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0Q11

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
 Title : SVOA CALIBRATION

37	16.113	2187	2189	2194	rVB5	2800	3831	0.11%	0.012%
38	16.230	2205	2209	2213	rBV7	4259	8200	0.24%	0.025%
39	16.271	2213	2216	2218	rBV3	3651	3940	0.12%	0.012%
40	16.330	2223	2226	2229	rVB4	3571	4281	0.13%	0.013%
41	16.448	2241	2246	2249	rBV4	5321	8610	0.26%	0.026%
42	16.807	2304	2307	2311	rVB5	5093	6491	0.19%	0.020%
43	16.954	2329	2332	2336	rBV5	5291	8356	0.25%	0.025%
44	17.065	2347	2351	2352	rBV3	6630	7507	0.22%	0.023%
45	17.083	2352	2354	2357	rVB	4160	4546	0.14%	0.014%
46	17.218	2375	2377	2383	rVB6	2400	3826	0.11%	0.012%
47	17.301	2384	2391	2400	rBV	1218046	1740129	51.74%	5.251%
48	17.401	2401	2408	2421	rVV	2253309	3226978	95.95%	9.737%
49	17.665	2450	2453	2455	rBV4	3527	4140	0.12%	0.012%
50	17.877	2486	2489	2494	rVB7	5772	8136	0.24%	0.025%
51	18.189	2538	2542	2550	rBV2	38582	59306	1.76%	0.179%
52	18.818	2647	2649	2658	rVB6	6936	9297	0.28%	0.028%
53	19.248	2718	2722	2727	rBV2	32168	46591	1.39%	0.141%
54	19.318	2730	2734	2740	rVB	30196	40845	1.21%	0.123%
55	19.465	2755	2759	2765	rBV5	29364	44858	1.33%	0.135%
56	19.612	2782	2784	2787	rVB3	12644	11456	0.34%	0.035%
57	19.683	2790	2796	2804	rBV	2594471	3363040	100.00%	10.147%
58	21.459	3093	3098	3109	rBV	1223949	1527639	45.42%	4.609%
59	23.694	3471	3478	3485	rBV2	1445652	2835388	84.31%	8.555%
60	23.847	3498	3504	3513	rVB2	736840	1445818	42.99%	4.363%




Sum of corrected areas: 33141954

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020122\
Data File : BM033958.D
Acq On : 02 Feb 2022 02:49
Operator : CG/JU
Sample : N1307-02
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0Q11

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

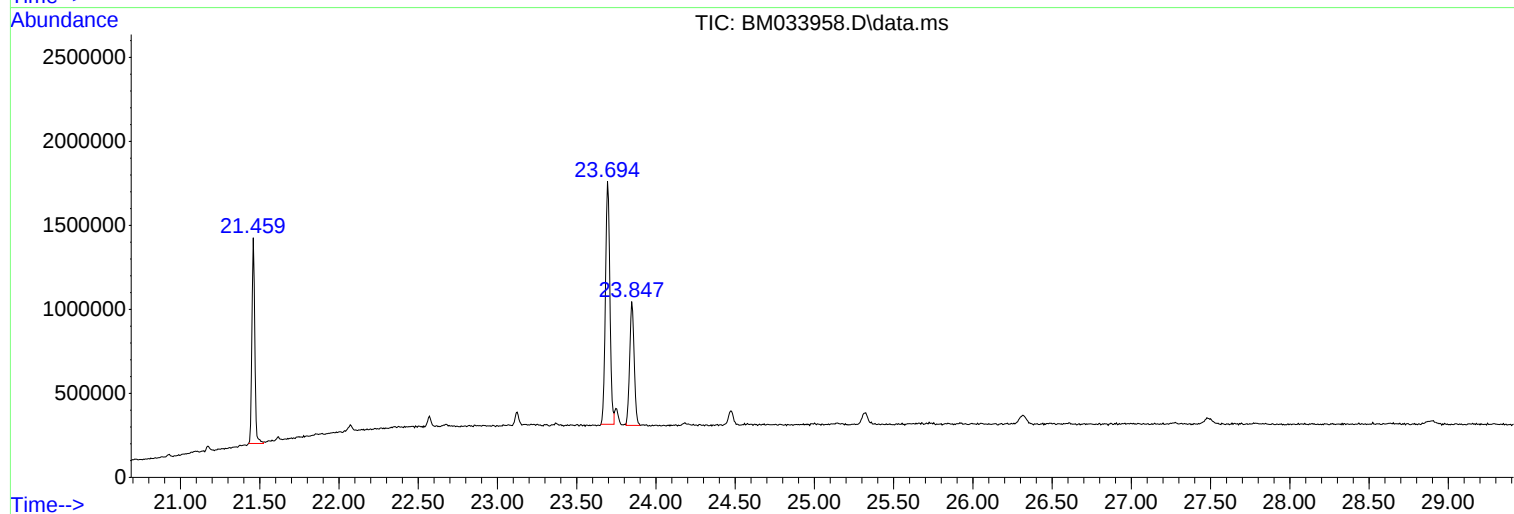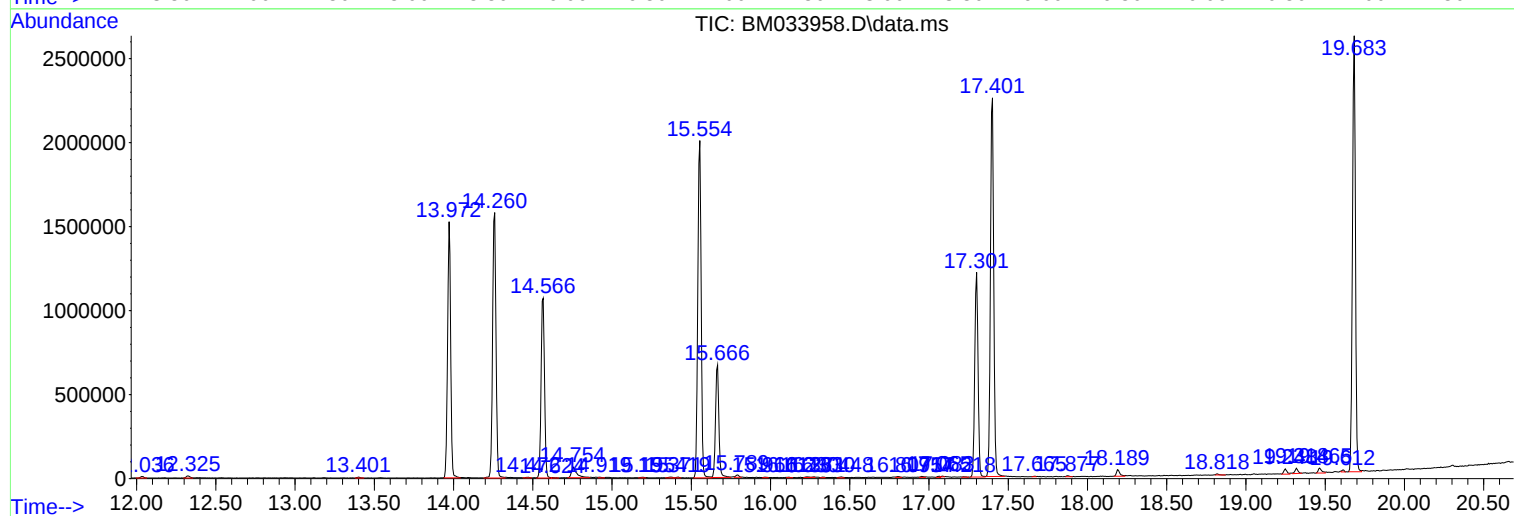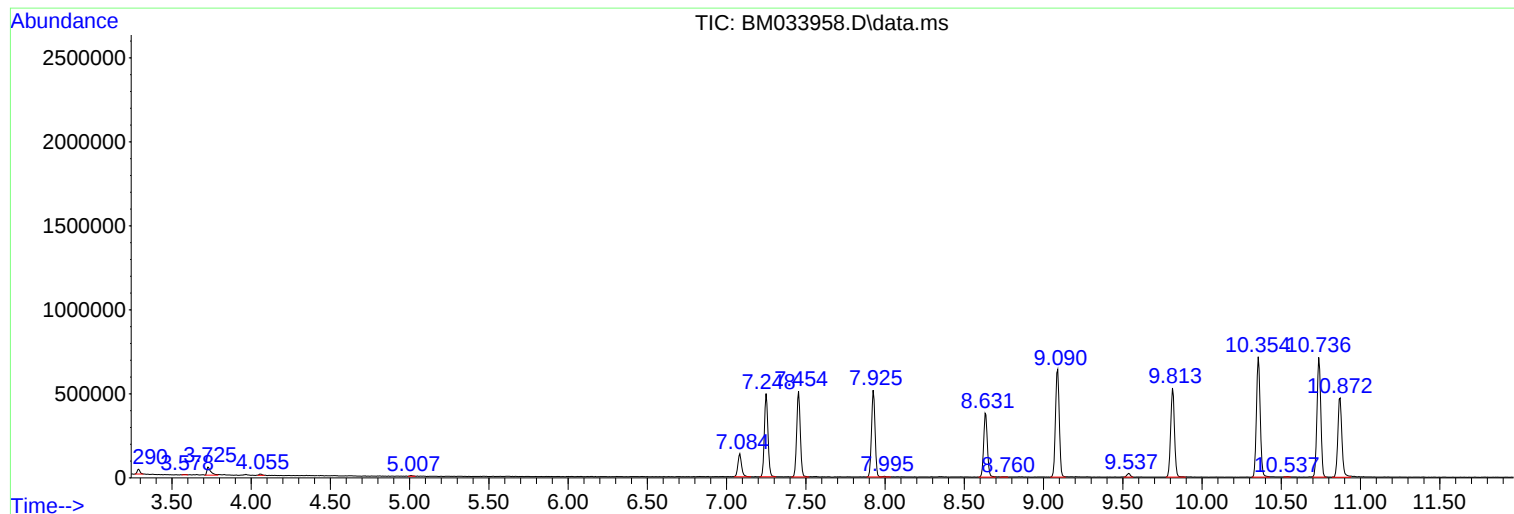

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020122\
Data File : BM033958.D
Acq On : 02 Feb 2022 02:49
Operator : CG/JU
Sample : N1307-02
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0Q11

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020122\
Data File : BM033958.D
Acq On : 02 Feb 2022 02:49
Operator : CG/JU
Sample : N1307-02
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0Q11

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc