

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020122\
 Data File : BM033968.D
 Acq On : 02 Feb 2022 10:55
 Operator : CG/JU
 Sample : N1273-17DL 5X
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 COHL5DL

Integration Parameters: LSCINT.P
 Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
 Title : SVOA CALIBRATION

Signal : TIC: BM033968.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.319	12	14	23	rVB	106579	148133	2.07%	0.662%
2	4.054	136	139	143	rBV2	8740	10261	0.14%	0.046%
3	4.154	153	156	164	rVB8	6202	10785	0.15%	0.048%
4	4.601	225	232	247	rBV	4943458	7151731	100.00%	31.967%
5	7.084	648	654	663	rVB	28060	47939	0.67%	0.214%
6	7.248	675	682	693	rVB	126184	199460	2.79%	0.892%
7	7.454	710	717	725	rVB	120284	191834	2.68%	0.857%
8	7.613	740	744	749	rVB3	10011	14108	0.20%	0.063%
9	7.925	787	797	806	rBV	468661	735506	10.28%	3.288%
10	8.631	912	917	924	rBV	80583	133435	1.87%	0.596%
11	9.084	988	994	1003	rBV	149064	251095	3.51%	1.122%
12	9.536	1065	1071	1074	rBV	5676	8173	0.11%	0.037%
13	9.813	1110	1118	1126	rBV	116052	191507	2.68%	0.856%
14	10.354	1202	1210	1224	rBV	146325	263638	3.69%	1.178%
15	10.736	1267	1275	1282	rBV	655784	1088847	15.22%	4.867%
16	10.872	1292	1298	1308	rVB2	20121	40827	0.57%	0.182%
17	13.971	1819	1825	1835	rBV	413842	590563	8.26%	2.640%
18	14.254	1867	1873	1884	rVB	383403	556633	7.78%	2.488%
19	14.560	1919	1925	1936	rBV	1086199	1616377	22.60%	7.225%
20	14.777	1955	1962	1966	rBV7	6550	14443	0.20%	0.065%
21	15.548	2087	2093	2106	rBV	571763	833963	11.66%	3.728%
22	15.665	2106	2113	2124	rBV	140286	222582	3.11%	0.995%
23	17.295	2384	2390	2401	rBV	1341940	1980412	27.69%	8.852%
24	17.395	2401	2407	2418	rVB2	684833	975413	13.64%	4.360%
25	18.195	2540	2543	2550	rVB6	8761	13482	0.19%	0.060%
26	19.242	2719	2721	2726	rBV5	6355	9519	0.13%	0.043%
27	19.612	2781	2784	2788	rVB5	11725	14635	0.20%	0.065%
28	19.677	2790	2795	2802	rBV	817547	1090348	15.25%	4.874%
29	21.459	3093	3098	3107	rBV	1367402	1733260	24.24%	7.747%
30	23.694	3472	3478	3483	rBV	381943	726182	10.15%	3.246%
31	23.847	3498	3504	3513	rVB2	772105	1507119	21.07%	6.737%




Sum of corrected areas: 22372210

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020122\
Data File : BM033968.D
Acq On : 02 Feb 2022 10:55
Operator : CG/JU
Sample : N1273-17DL 5X
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0HL5DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

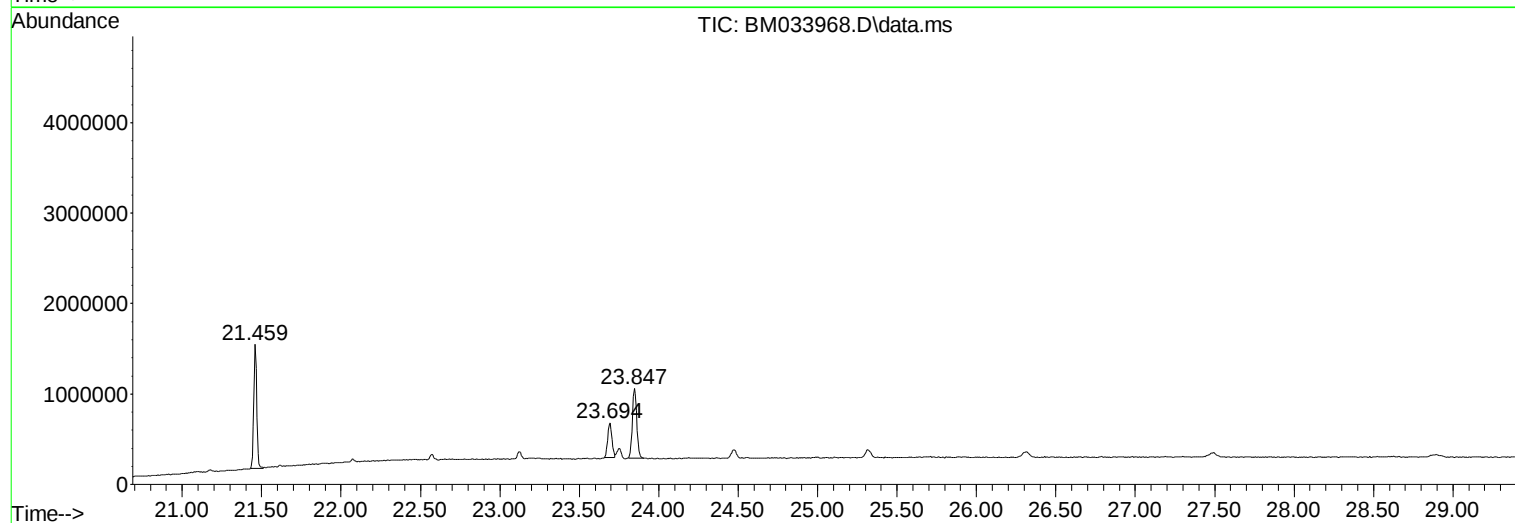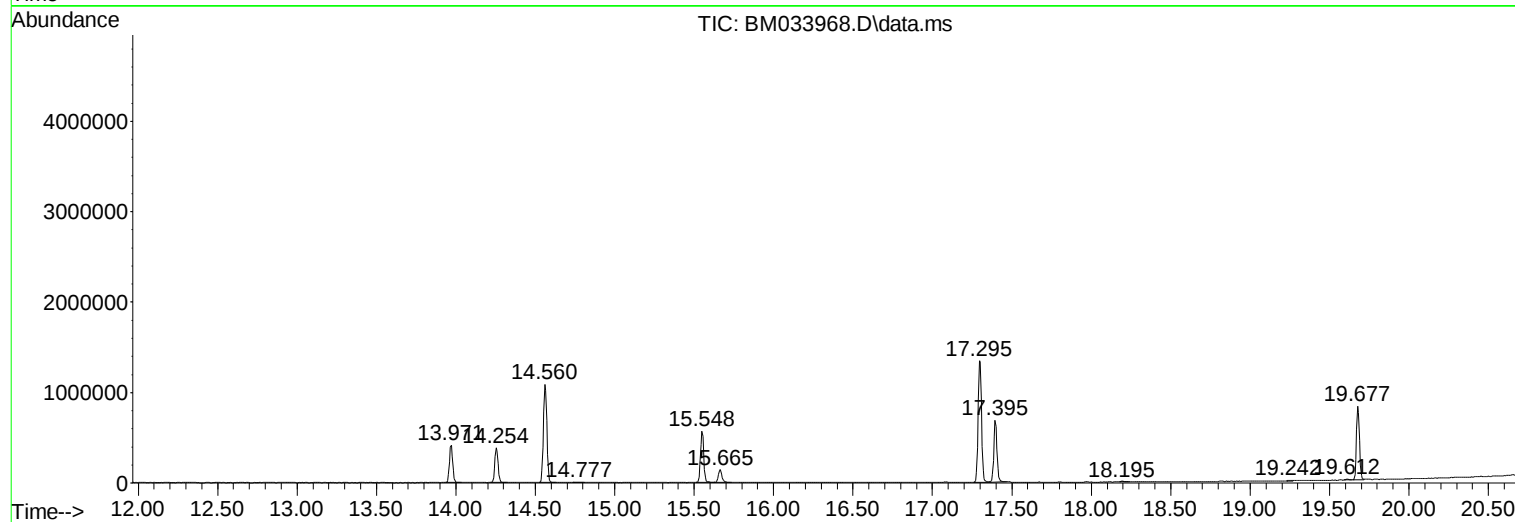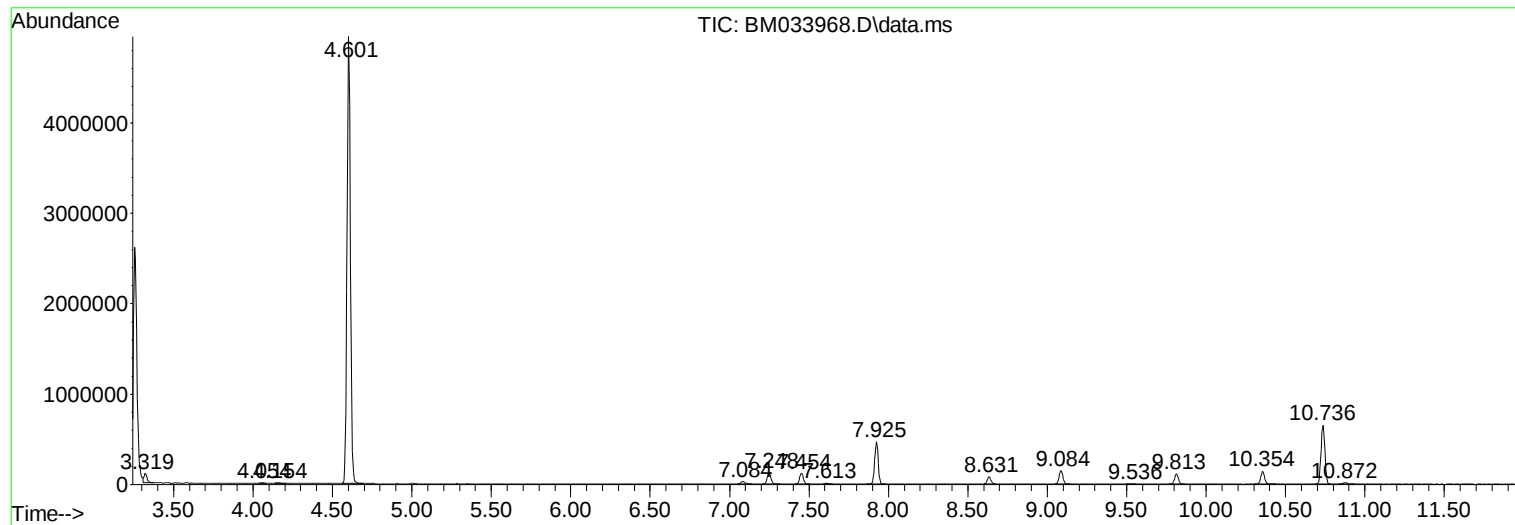

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020122\
Data File : BM033968.D
Acq On : 02 Feb 2022 10:55
Operator : CG/JU
Sample : N1273-17DL 5X
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0HL5DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected
