

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020122\
 Data File : BM033969.D
 Acq On : 02 Feb 2022 11:45
 Operator : CG/JU
 Sample : N1273-21DL 5X
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0HL9DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
 Title : SVOA CALIBRATION

Signal : TIC: BM033969.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.319	11	14	26	rVB	172638	222694	11.58%	1.425%
2	3.737	82	85	94	rBV	11278	22108	1.15%	0.142%
3	4.055	135	139	143	rBV2	7875	11667	0.61%	0.075%
4	4.178	155	160	165	rVB5	7927	10352	0.54%	0.066%
5	4.602	226	232	243	rVB	780244	1160258	60.35%	7.426%
6	5.337	353	357	364	rBV3	5775	11036	0.57%	0.071%
7	5.902	449	453	458	rBV6	1521	2536	0.13%	0.016%
8	7.084	648	654	664	rVB4	22534	46522	2.42%	0.298%
9	7.248	676	682	691	rBV	103238	163614	8.51%	1.047%
10	7.454	710	717	727	rBV	83882	140226	7.29%	0.898%
11	7.719	760	762	764	rBV3	2076	2038	0.11%	0.013%
12	7.925	789	797	807	rBV	450422	708879	36.87%	4.537%
13	7.995	807	809	812	rVV4	3452	3925	0.20%	0.025%
14	8.631	911	917	925	rBV	56029	98460	5.12%	0.630%
15	8.795	942	945	947	rBV4	1713	2564	0.13%	0.016%
16	9.084	988	994	1003	rBV	124523	203615	10.59%	1.303%
17	9.537	1065	1071	1077	rVB	22166	34587	1.80%	0.221%
18	9.813	1111	1118	1124	rBV	84797	139753	7.27%	0.895%
19	10.354	1204	1210	1221	rBV	109338	192475	10.01%	1.232%
20	10.525	1234	1239	1247	rBV4	10771	22257	1.16%	0.142%
21	10.672	1261	1264	1267	rBV4	2234	3138	0.16%	0.020%
22	10.736	1267	1275	1284	rVB	627021	1050642	54.65%	6.725%
23	10.801	1284	1286	1291	rBV5	1675	2058	0.11%	0.013%
24	10.872	1291	1298	1309	rBV	110512	203799	10.60%	1.304%
25	11.125	1340	1341	1346	rVB5	1712	2103	0.11%	0.013%
26	12.036	1489	1496	1503	rBV	17832	27419	1.43%	0.176%
27	12.201	1520	1524	1526	rVB3	2092	2358	0.12%	0.015%
28	12.331	1542	1546	1551	rBV5	2835	4223	0.22%	0.027%
29	12.742	1613	1616	1619	rBV3	1289	1955	0.10%	0.013%
30	12.936	1644	1649	1654	rBV5	2543	4895	0.25%	0.031%
31	13.178	1687	1690	1694	rBV4	2147	2713	0.14%	0.017%
32	13.413	1724	1730	1735	rBV3	30624	48836	2.54%	0.313%
33	13.472	1735	1740	1743	rVB3	2193	3244	0.17%	0.021%
34	13.883	1803	1810	1816	rBV7	4291	7967	0.41%	0.051%
35	13.972	1819	1825	1837	rBV	363191	507726	26.41%	3.250%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020122\
 Data File : BM033969.D
 Acq On : 02 Feb 2022 11:45
 Operator : CG/JU
 Sample : N1273-21DL 5X
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 COHL9DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
 Title : SVOA CALIBRATION

36	14.183	1855	1861	1868	rBV2	22040	58021	3.02%	0.371%
37	14.254	1868	1873	1885	rVB	339755	511474	26.60%	3.274%
38	14.460	1906	1908	1913	rVB6	2865	3152	0.16%	0.020%
39	14.566	1919	1926	1937	rBV	1077536	1569649	81.64%	10.047%
40	14.777	1956	1962	1967	rBV7	5867	12872	0.67%	0.082%
41	14.942	1986	1990	1997	rVB6	6123	10940	0.57%	0.070%
42	15.301	2047	2051	2057	rBV5	2459	3255	0.17%	0.021%
43	15.366	2060	2062	2066	rVB5	2783	3249	0.17%	0.021%
44	15.419	2066	2071	2073	rBV5	2056	2456	0.13%	0.016%
45	15.554	2088	2094	2107	rBV	470809	705117	36.67%	4.513%
46	15.666	2107	2113	2123	rVB	95617	147925	7.69%	0.947%
47	15.789	2132	2134	2143	rVB8	1702	2610	0.14%	0.017%
48	15.960	2158	2163	2164	rBV4	1547	2124	0.11%	0.014%
49	15.989	2167	2168	2172	rVB4	2815	3095	0.16%	0.020%
50	16.183	2197	2201	2204	rBV5	1245	2012	0.10%	0.013%
51	16.236	2206	2210	2213	rBV5	1876	2477	0.13%	0.016%
52	16.271	2213	2216	2219	rBV4	2373	2220	0.12%	0.014%
53	16.618	2272	2275	2279	rBV5	2504	2864	0.15%	0.018%
54	16.807	2301	2307	2311	rBV5	4347	6107	0.32%	0.039%
55	16.948	2328	2331	2337	rVB8	1136	1958	0.10%	0.013%
56	17.060	2347	2350	2351	rBV3	2242	2131	0.11%	0.014%
57	17.083	2352	2354	2358	rVB2	4670	5549	0.29%	0.036%
58	17.230	2375	2379	2381	rVB3	2084	2380	0.12%	0.015%
59	17.301	2384	2391	2401	rBV	1380200	1922625	100.00%	12.306%
60	17.395	2401	2407	2420	rVV	534069	797176	41.46%	5.102%
61	17.877	2486	2489	2491	rVB3	4755	4028	0.21%	0.026%
62	17.977	2500	2506	2512	rVB3	23874	33288	1.73%	0.213%
63	18.101	2523	2527	2530	rBV4	2805	4235	0.22%	0.027%
64	18.195	2539	2543	2548	rBV5	13994	20445	1.06%	0.131%
65	18.454	2585	2587	2590	rVV4	2765	2548	0.13%	0.016%
66	18.495	2590	2594	2597	rVB5	2416	3727	0.19%	0.024%
67	18.712	2629	2631	2633	rBV3	2145	2388	0.12%	0.015%
68	18.812	2646	2648	2653	rVB5	5614	7386	0.38%	0.047%
69	18.918	2664	2666	2669	rBV4	3305	3139	0.16%	0.020%
70	19.018	2679	2683	2685	rBV4	3640	4551	0.24%	0.029%
71	19.142	2700	2704	2708	rBV4	21929	25388	1.32%	0.163%
72	19.318	2732	2734	2737	rVB4	5282	4643	0.24%	0.030%
73	19.471	2757	2760	2762	rBV4	5969	6958	0.36%	0.045%
74	19.612	2779	2784	2790	rBV7	19156	30815	1.60%	0.197%
75	19.683	2790	2796	2802	rBV	640659	856180	44.53%	5.480%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020122\
Data File : BM033969.D
Acq On : 02 Feb 2022 11:45
Operator : CG/JU
Sample : N1273-21DL 5X
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0HL9DL

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
Title : SVOA CALIBRATION

76	21.459	3093	3098	3107	rBV	1304415	1716119	89.26%	10.984%
77	23.694	3473	3478	3484	rBV	292192	553831	28.81%	3.545%
78	23.853	3499	3505	3514	rVB2	739448	1487525	77.37%	9.521%




Sum of corrected areas: 15623274

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020122\
Data File : BM033969.D
Acq On : 02 Feb 2022 11:45
Operator : CG/JU
Sample : N1273-21DL 5X
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0HL9DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

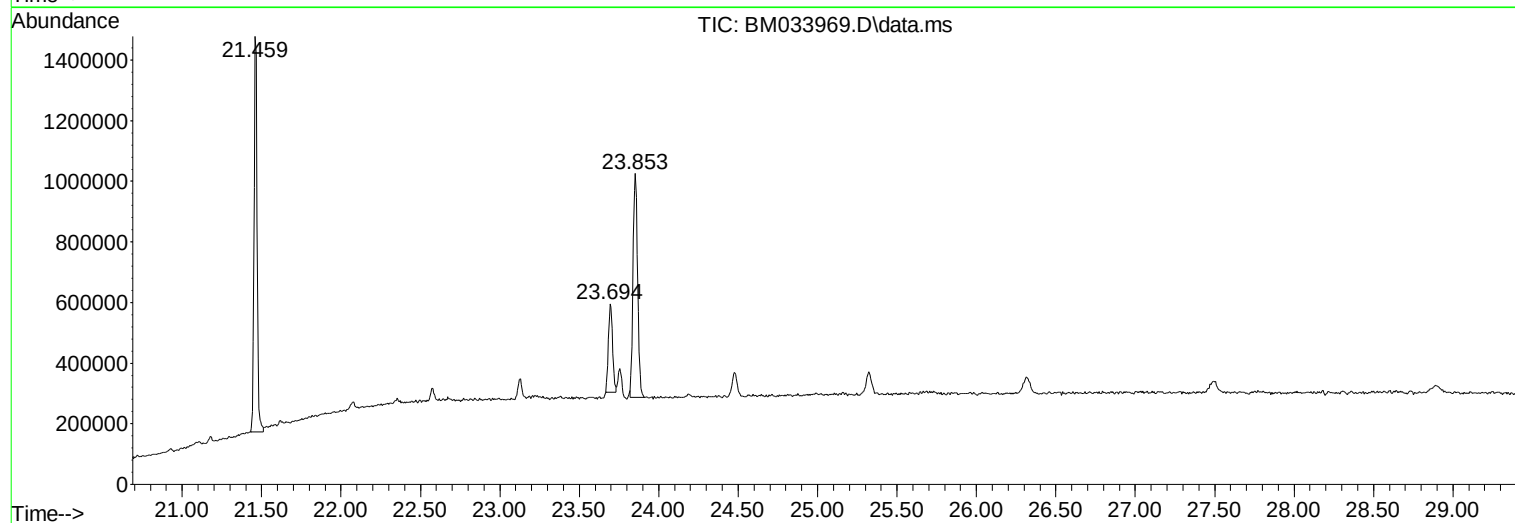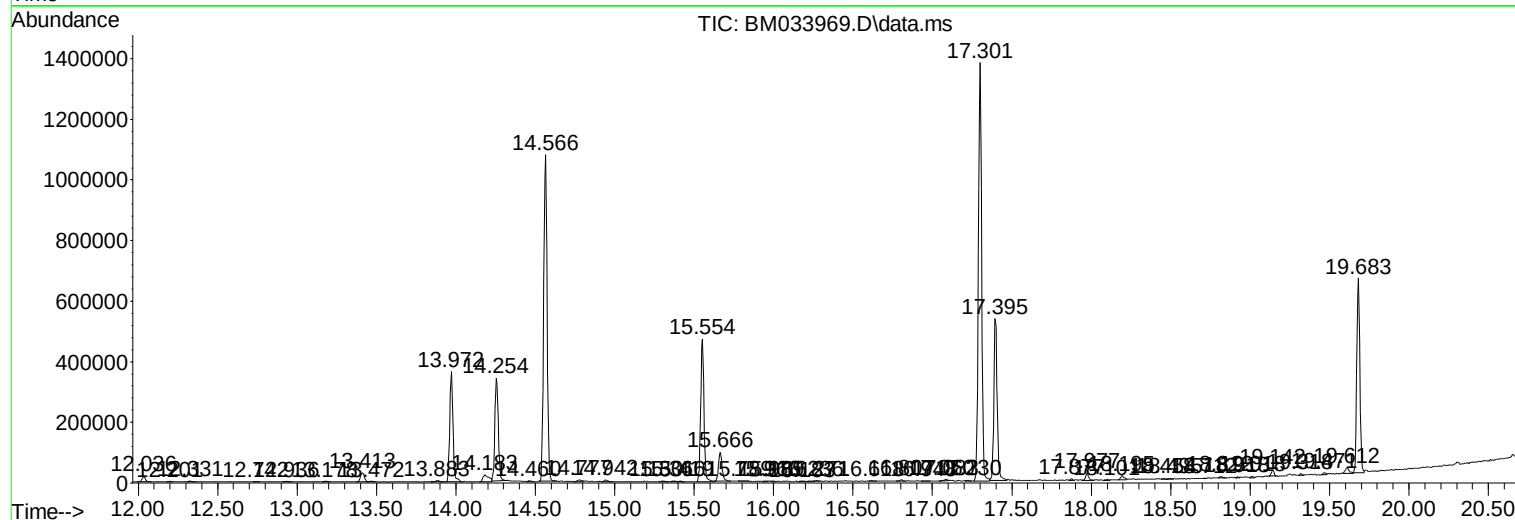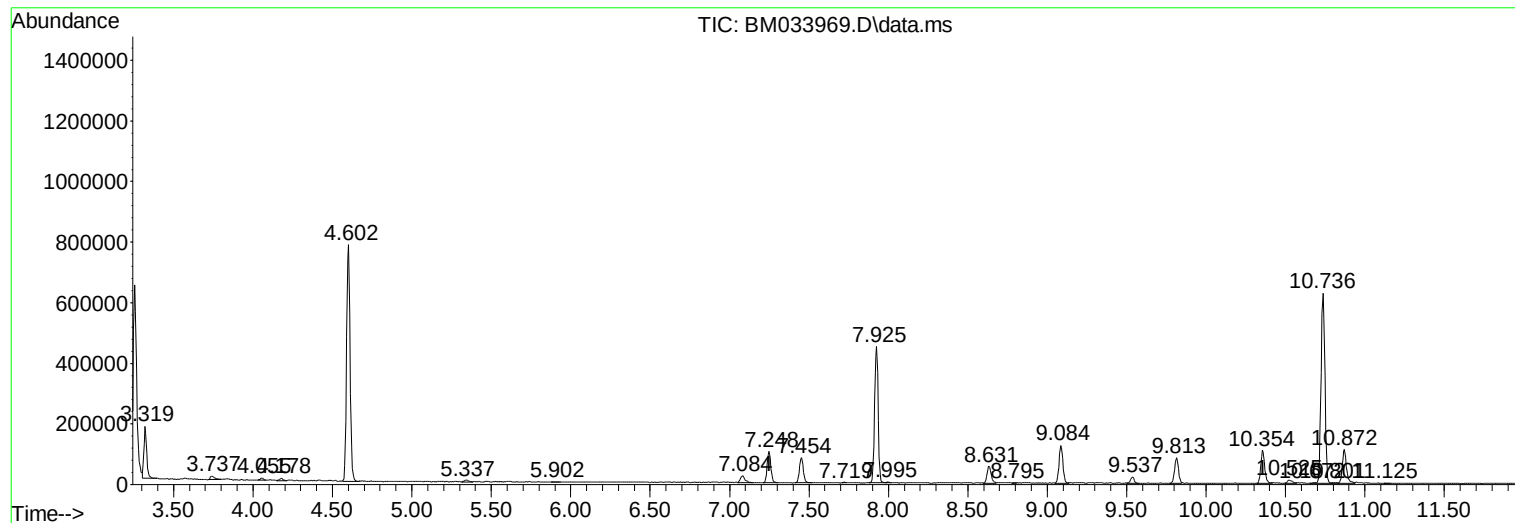

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020122\
Data File : BM033969.D
Acq On : 02 Feb 2022 11:45
Operator : CG/JU
Sample : N1273-21DL 5X
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0HL9DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020122\
Data File : BM033969.D
Acq On : 02 Feb 2022 11:45
Operator : CG/JU
Sample : N1273-21DL 5X
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0HL9DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

				---Internal Standard---				
TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
