

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020122\
 Data File : BM033970.D
 Acq On : 02 Feb 2022 12:20
 Operator : CG/JU
 Sample : N1328-03DL 10X
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0HM2DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
 Title : SVOA CALIBRATION

Signal : TIC: BM033970.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.319	11	14	25	rVB	222390	313346	6.96%	1.974%
2	4.054	136	139	145	rVB	7302	9049	0.20%	0.057%
3	4.154	153	156	161	rBV4	7006	10625	0.24%	0.067%
4	4.601	225	232	243	rBV	3152441	4501360	100.00%	28.359%
5	6.660	577	582	587	rBV8	3151	6877	0.15%	0.043%
6	7.084	649	654	661	rVB2	12779	22685	0.50%	0.143%
7	7.248	676	682	688	rBV	51104	83491	1.85%	0.526%
8	7.454	710	717	725	rBV	47388	78658	1.75%	0.496%
9	7.925	787	797	804	rBV	439766	700162	15.55%	4.411%
10	8.636	913	918	924	rBV2	29144	47698	1.06%	0.301%
11	9.083	988	994	1006	rVB	58455	101110	2.25%	0.637%
12	9.536	1065	1071	1075	rVB4	5572	8439	0.19%	0.053%
13	9.813	1112	1118	1125	rBV	39036	68850	1.53%	0.434%
14	10.360	1205	1211	1223	rVB	48519	89494	1.99%	0.564%
15	10.736	1267	1275	1286	rVB	618127	1029002	22.86%	6.483%
16	10.872	1293	1298	1311	rVB	34975	69289	1.54%	0.437%
17	13.466	1732	1739	1745	rBV3	6876	11497	0.26%	0.072%
18	13.971	1818	1825	1836	rBV	170241	247359	5.50%	1.558%
19	14.254	1868	1873	1883	rVB	162028	237994	5.29%	1.499%
20	14.560	1917	1925	1937	rBV	1033500	1530210	33.99%	9.640%
21	15.548	2087	2093	2104	rBV	238139	354723	7.88%	2.235%
22	15.665	2107	2113	2126	rVB	37660	66161	1.47%	0.417%
23	17.083	2348	2354	2361	rBV6	4655	9151	0.20%	0.058%
24	17.301	2384	2391	2401	rBV	1254230	1849944	41.10%	11.655%
25	17.395	2401	2407	2415	rVB	257106	390274	8.67%	2.459%
26	17.971	2501	2505	2512	rBV2	8761	13869	0.31%	0.087%
27	18.201	2540	2544	2549	rBV8	5447	9847	0.22%	0.062%
28	19.142	2700	2704	2708	rBV5	20419	22735	0.51%	0.143%
29	19.271	2724	2726	2729	rVB4	6757	5583	0.12%	0.035%
30	19.465	2757	2759	2761	rBV3	5221	4677	0.10%	0.029%
31	19.612	2781	2784	2788	rBV5	12994	17282	0.38%	0.109%
32	19.683	2790	2796	2801	rBV	307461	432993	9.62%	2.728%
33	21.459	3093	3098	3109	rBV	1341716	1660752	36.89%	10.463%
34	23.694	3474	3478	3483	rVV2	129584	208757	4.64%	1.315%
35	23.753	3484	3488	3494	rVB2	116628	196487	4.37%	1.238%
36	23.847	3498	3504	3516	rVB2	691550	1462438	32.49%	9.213%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020122\
Data File : BM033970.D
Acq On : 02 Feb 2022 12:20
Operator : CG/JU
Sample : N1328-03DL 10X
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0HM2DL

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
Title : SVOA CALIBRATION




Sum of corrected areas: 15872868

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020122\
Data File : BM033970.D
Acq On : 02 Feb 2022 12:20
Operator : CG/JU
Sample : N1328-03DL 10X
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0HM2DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

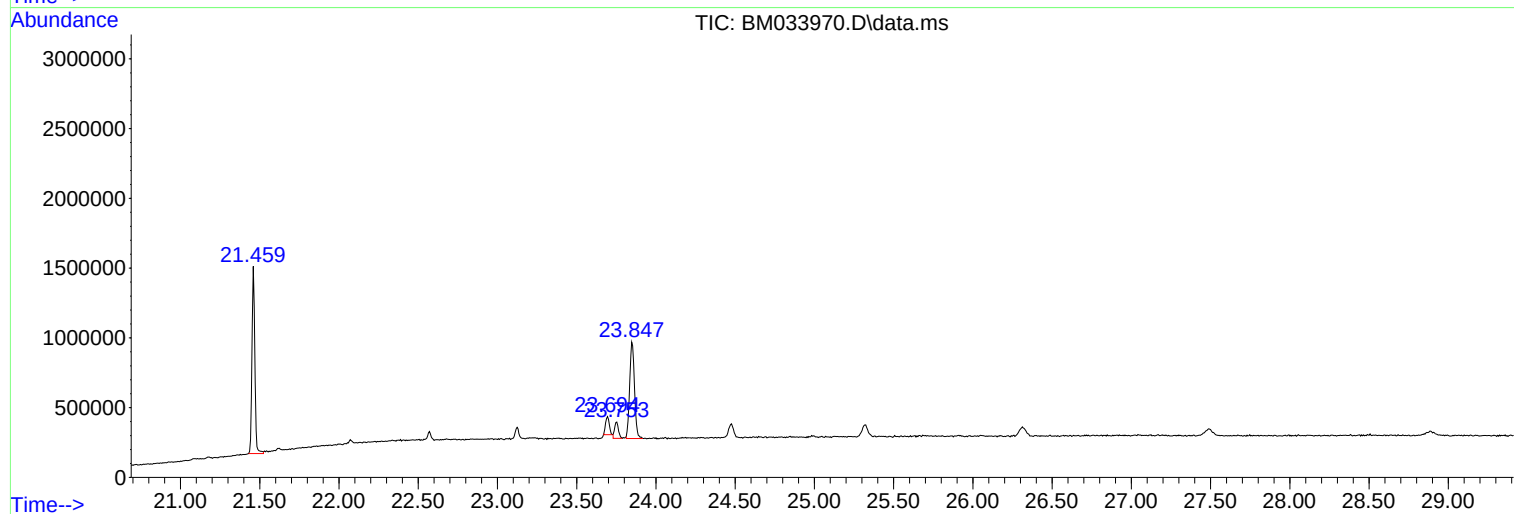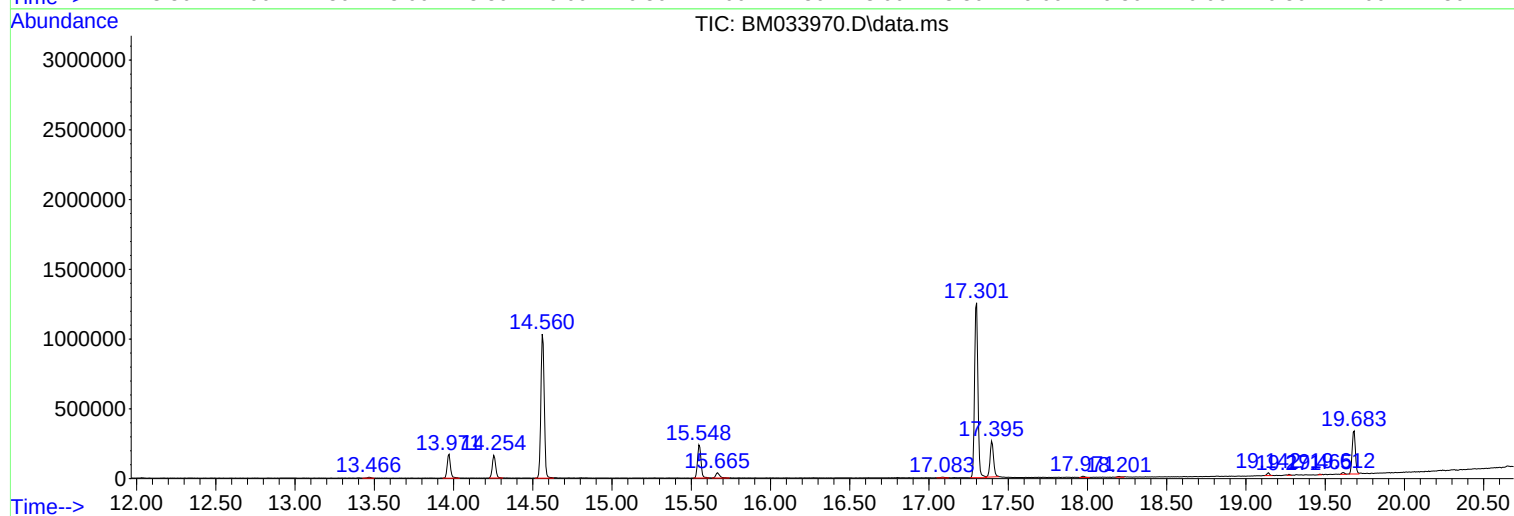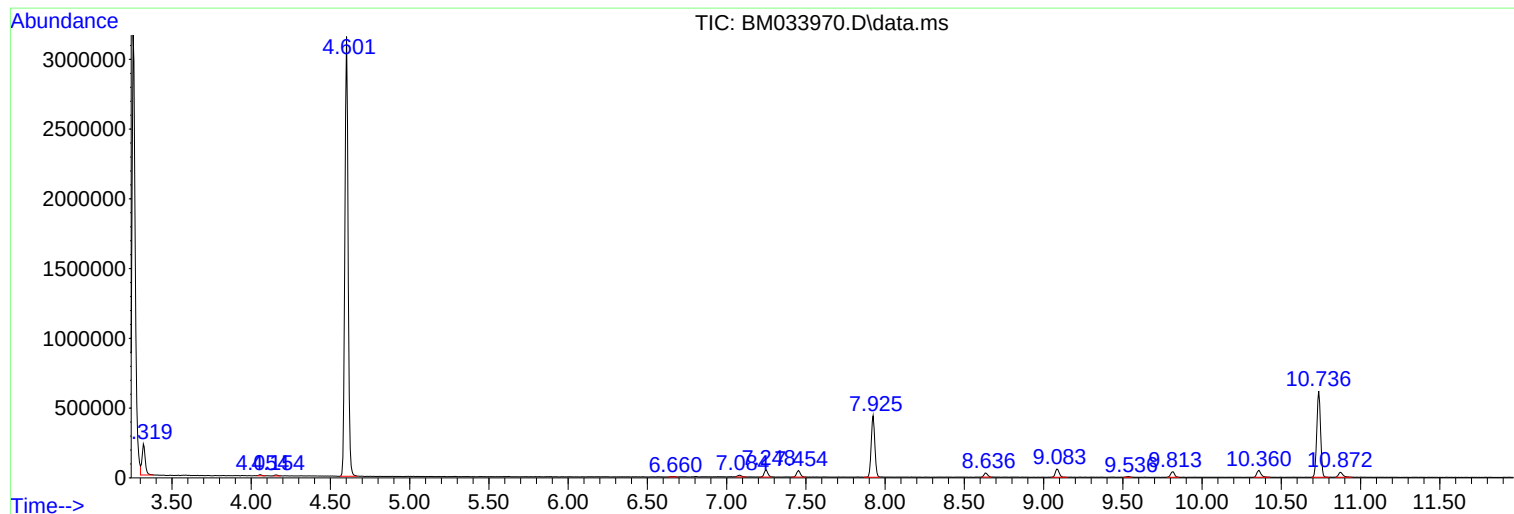

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020122\
Data File : BM033970.D
Acq On : 02 Feb 2022 12:20
Operator : CG/JU
Sample : N1328-03DL 10X
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0HM2DL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 (DEL) Alkane: Straight-Chai... Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
23.753	2.69 ng/ul	196487	Perylene-d12	23.847

Hit#	of 5	Tentative ID	MW	MolForm	CAS#	Qual
1		Octadecane	254	C18H38	000593-45-3	98
2		Dotriacontane, 1-iodo-	576	C32H65I	1000406-32-4	81
3		Tetracosane, 11-decyl-	479	C34H70	055429-84-0	81
4		Docosane, 11-decyl-	451	C32H66	055401-55-3	81
5		Docosane, 1-iodo-	436	C22H45I	1000406-31-9	81

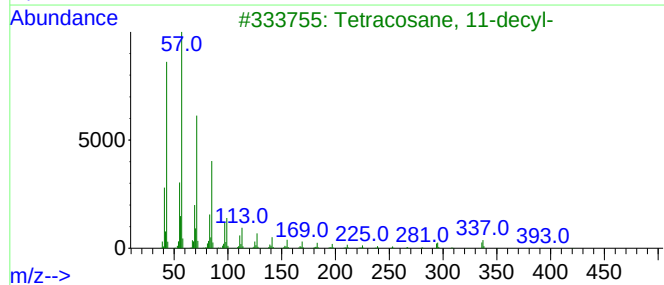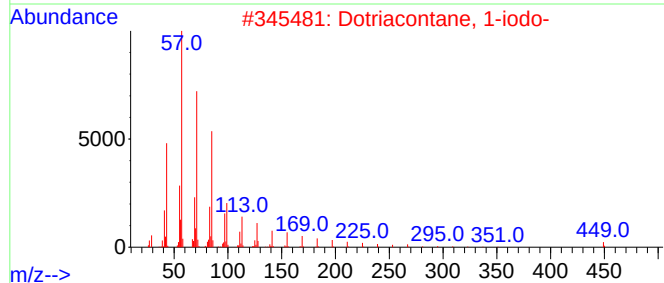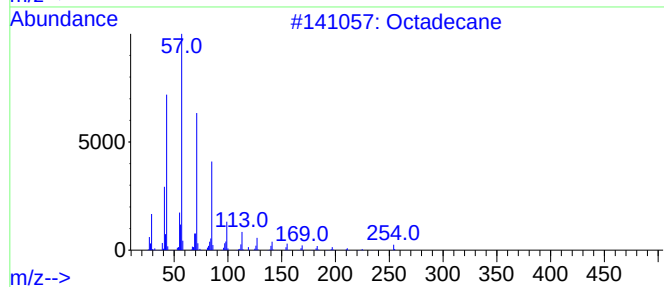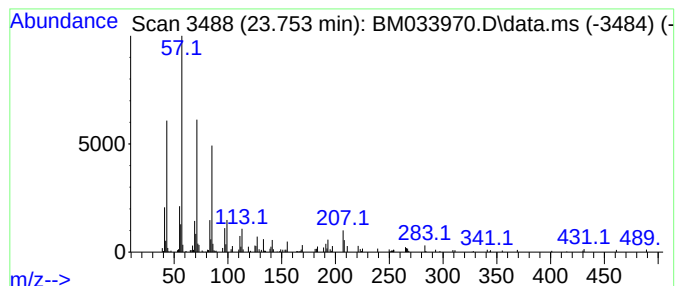

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020122\
Data File : BM033970.D
Acq On : 02 Feb 2022 12:20
Operator : CG/JU
Sample : N1328-03DL 10X
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0HM2DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: S...	23.753	2.7	ng/u1	196487	6	23.847	1462440	20.0