

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020122\
 Data File : BM033972.D
 Acq On : 02 Feb 2022 13:32
 Operator : CG/JU
 Sample : N1307-07DL 10X
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0Q47DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
 Title : SVOA CALIBRATION

Signal : TIC: BM033972.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.054	137	139	145	rVB2	8165	10597	0.22%	0.064%
2	7.084	648	654	660	rVB2	11947	20178	0.42%	0.121%
3	7.248	677	682	691	rBV	40459	64536	1.33%	0.388%
4	7.454	707	717	725	rBV	39375	71661	1.48%	0.430%
5	7.925	790	797	804	rBV	488162	755663	15.57%	4.537%
6	7.995	806	809	814	rVB4	6886	9829	0.20%	0.059%
7	8.636	913	918	927	rBV	29336	49230	1.01%	0.296%
8	9.089	989	995	1002	rBV	45810	79299	1.63%	0.476%
9	9.813	1113	1118	1125	rBV2	31526	54428	1.12%	0.327%
10	10.360	1205	1211	1217	rBV	47501	86320	1.78%	0.518%
11	10.736	1268	1275	1283	rBV	698223	1158203	23.87%	6.954%
12	10.872	1292	1298	1306	rBV	39005	79942	1.65%	0.480%
13	11.842	1459	1463	1469	rBV7	2915	5700	0.12%	0.034%
14	12.766	1616	1620	1624	rBV4	4227	6723	0.14%	0.040%
15	13.007	1654	1661	1666	rBV3	11992	20176	0.42%	0.121%
16	13.401	1721	1728	1732	rBV6	8359	11844	0.24%	0.071%
17	13.536	1746	1751	1759	rVB8	2512	6738	0.14%	0.040%
18	13.848	1800	1804	1809	rBV7	4398	5612	0.12%	0.034%
19	13.971	1819	1825	1831	rBV	151825	214290	4.42%	1.287%
20	14.254	1866	1873	1884	rVB	142515	215179	4.43%	1.292%
21	14.560	1919	1925	1938	rBV	1147367	1711029	35.26%	10.274%
22	14.736	1951	1955	1957	rBV5	3825	6267	0.13%	0.038%
23	14.871	1971	1978	1979	rBV5	3236	5434	0.11%	0.033%
24	15.101	2011	2017	2022	rVV	113114	169411	3.49%	1.017%
25	15.183	2026	2031	2043	rVV	158157	245446	5.06%	1.474%
26	15.295	2043	2050	2058	rVV7	7425	17699	0.36%	0.106%
27	15.371	2058	2063	2071	rVV10	4863	12318	0.25%	0.074%
28	15.548	2088	2093	2100	rBV	220684	307398	6.34%	1.846%
29	15.660	2107	2112	2120	rBV	44953	73024	1.50%	0.438%
30	15.889	2146	2151	2152	rBV4	3474	5218	0.11%	0.031%
31	15.965	2160	2164	2170	rBV6	7349	12933	0.27%	0.078%
32	16.465	2242	2249	2251	rBV7	3006	5829	0.12%	0.035%
33	16.695	2283	2288	2291	rBV7	4466	8194	0.17%	0.049%
34	16.948	2325	2331	2347	rBV	3374152	4852237	100.00%	29.135%
35	17.065	2347	2351	2359	rVV7	17006	48609	1.00%	0.292%
36	17.124	2359	2361	2368	rVB8	4426	6978	0.14%	0.042%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020122\
Data File : BM033972.D
Acq On : 02 Feb 2022 13:32
Operator : CG/JU
Sample : N1307-07DL 10X
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0Q47DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
Title : SVOA CALIBRATION

37	17.301	2384	2391	2402	rBV	1396681	2032903	41.90%	12.207%
38	17.395	2402	2407	2418	rVB	228344	335027	6.90%	2.012%
39	17.924	2490	2497	2501	rBV9	6248	13475	0.28%	0.081%
40	17.965	2501	2504	2507	rBV5	3982	5399	0.11%	0.032%
41	18.189	2538	2542	2550	rBV7	22094	35312	0.73%	0.212%
42	19.465	2756	2759	2763	rBV3	16285	16612	0.34%	0.100%
43	19.618	2782	2785	2790	rVB7	13713	16941	0.35%	0.102%
44	19.683	2790	2796	2802	rBV	251090	354781	7.31%	2.130%
45	21.459	3093	3098	3108	rBV	1371299	1731648	35.69%	10.398%
46	23.694	3475	3478	3483	rVB2	100603	152779	3.15%	0.917%
47	23.847	3498	3504	3514	rVB2	766938	1545189	31.84%	9.278%




Sum of corrected areas: 16654238

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020122\
Data File : BM033972.D
Acq On : 02 Feb 2022 13:32
Operator : CG/JU
Sample : N1307-07DL 10X
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0Q47DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

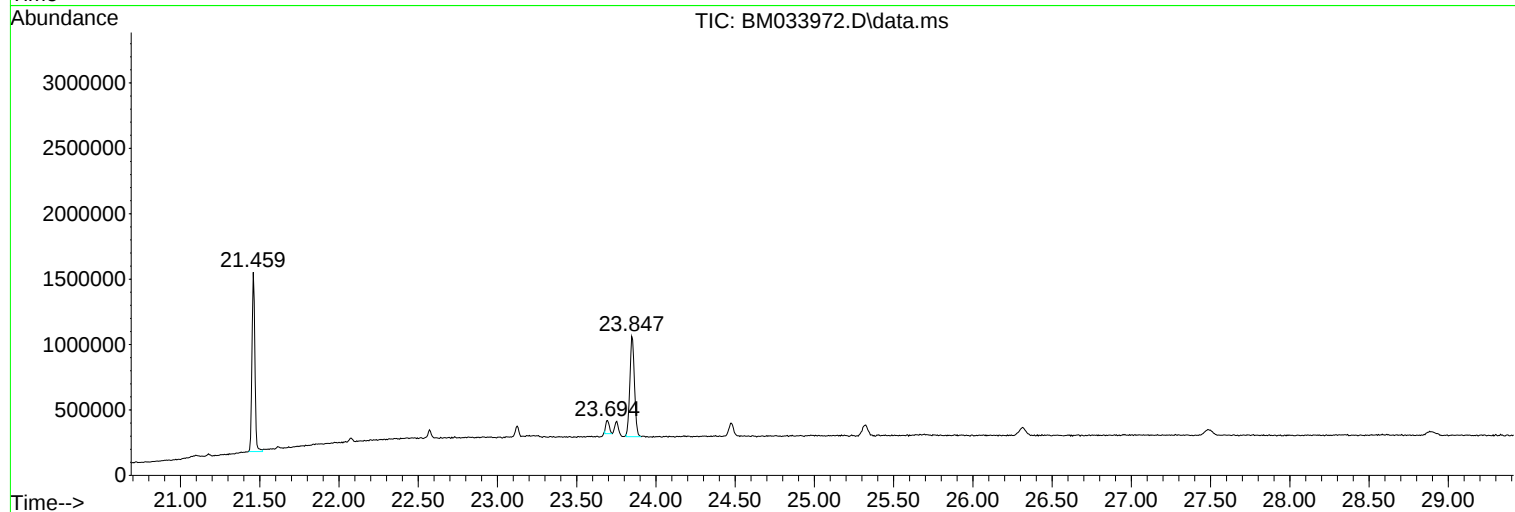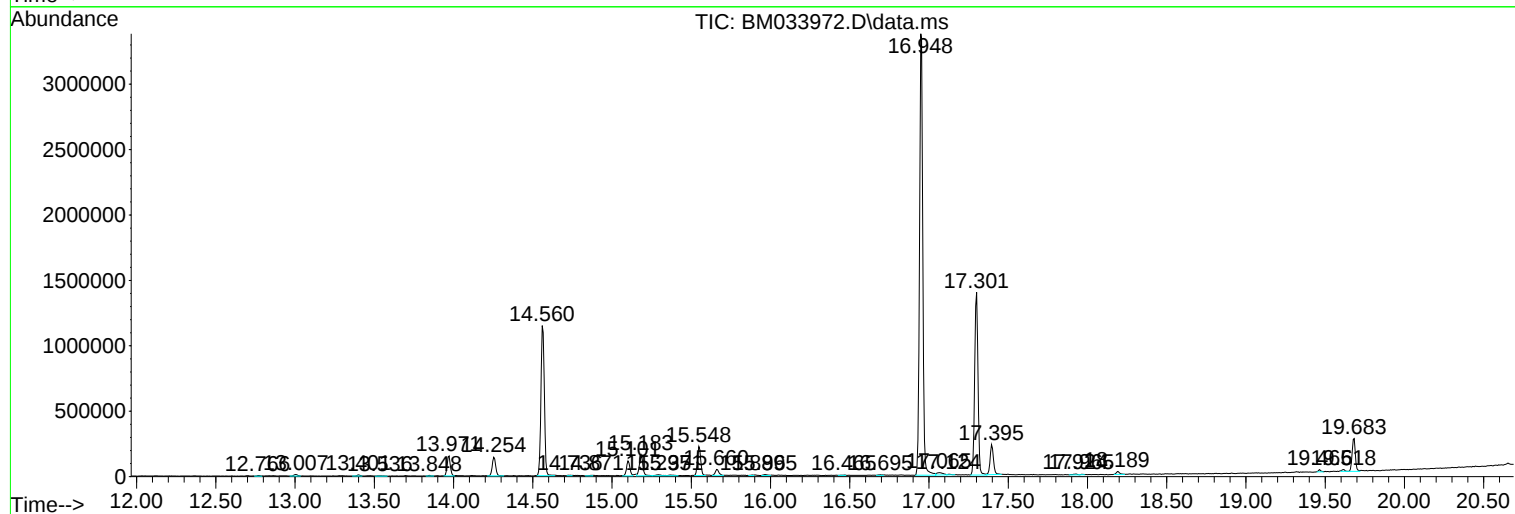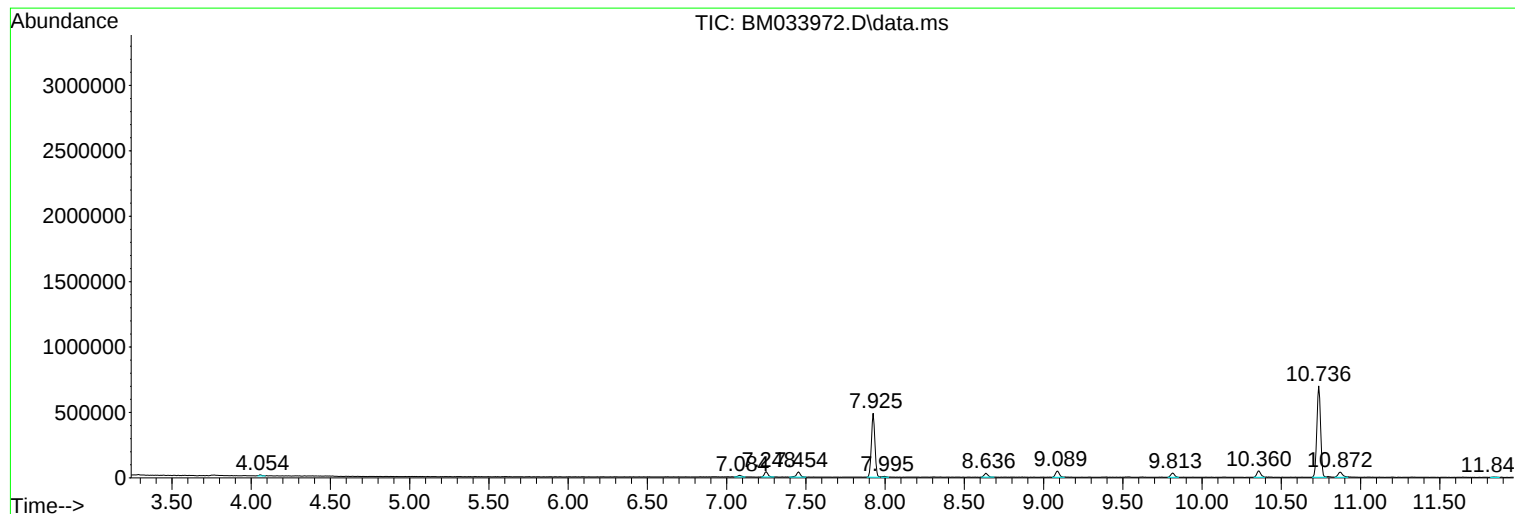

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020122\
Data File : BM033972.D
Acq On : 02 Feb 2022 13:32
Operator : CG/JU
Sample : N1307-07DL 10X
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0Q47DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020122\
Data File : BM033972.D
Acq On : 02 Feb 2022 13:32
Operator : CG/JU
Sample : N1307-07DL 10X
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0Q47DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc