

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020122\
 Data File : BM033974.D
 Acq On : 02 Feb 2022 14:43
 Operator : CG/JU
 Sample : N1307-09DL 20X
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0Q50DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
 Title : SVOA CALIBRATION

Signal : TIC: BM033974.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.055	136	139	146	rVB2	6806	10571	0.40%	0.088%
2	5.002	297	300	303	rBV5	1933	3137	0.12%	0.026%
3	7.084	649	654	659	rVB5	4337	6838	0.26%	0.057%
4	7.248	677	682	689	rVB2	20511	31302	1.20%	0.260%
5	7.454	711	717	725	rBV	18453	31009	1.19%	0.258%
6	7.925	790	797	809	rBV	419061	667358	25.53%	5.548%
7	8.048	814	818	824	rVB5	4601	6937	0.27%	0.058%
8	8.301	857	861	867	rBV2	5413	8927	0.34%	0.074%
9	8.637	914	918	926	rVV3	10159	18158	0.69%	0.151%
10	8.872	957	958	965	rVB7	1828	3051	0.12%	0.025%
11	9.090	990	995	1003	rBV2	18961	34315	1.31%	0.285%
12	9.384	1038	1045	1049	rBV7	2597	5552	0.21%	0.046%
13	9.566	1073	1076	1079	rVV5	2265	2878	0.11%	0.024%
14	9.613	1081	1084	1092	rVB6	1714	3697	0.14%	0.031%
15	9.819	1113	1119	1127	rBV2	13073	23367	0.89%	0.194%
16	9.984	1143	1147	1152	rBV3	3073	4016	0.15%	0.033%
17	10.137	1168	1173	1177	rBV3	3819	5778	0.22%	0.048%
18	10.360	1205	1211	1217	rBV3	15483	30140	1.15%	0.251%
19	10.736	1268	1275	1282	rBV	596918	994489	38.04%	8.268%
20	10.789	1282	1284	1290	rVB4	5050	7379	0.28%	0.061%
21	10.878	1290	1299	1312	rVB3	14880	44254	1.69%	0.368%
22	11.848	1458	1464	1467	rBV7	2685	4005	0.15%	0.033%
23	12.295	1536	1540	1544	rVB4	4143	5811	0.22%	0.048%
24	12.619	1589	1595	1599	rVB2	8002	13733	0.53%	0.114%
25	13.078	1668	1673	1679	rBV4	9817	17328	0.66%	0.144%
26	13.278	1703	1707	1718	rBV6	7963	17960	0.69%	0.149%
27	13.401	1725	1728	1733	rVB2	8508	11651	0.45%	0.097%
28	13.542	1746	1752	1754	rBV6	1779	2798	0.11%	0.023%
29	13.583	1754	1759	1762	rVV4	6521	11285	0.43%	0.094%
30	13.613	1762	1764	1772	rVB8	4755	8679	0.33%	0.072%
31	13.972	1818	1825	1831	rBV	75923	112823	4.32%	0.938%
32	14.030	1833	1835	1840	rVB6	2047	2838	0.11%	0.024%
33	14.119	1847	1850	1853	rBV2	3938	4904	0.19%	0.041%
34	14.254	1867	1873	1878	rBV	67456	102000	3.90%	0.848%
35	14.560	1919	1925	1935	rVV	993622	1498812	57.33%	12.461%
36	14.960	1987	1993	1999	rVB4	6866	12536	0.48%	0.104%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020122\
 Data File : BM033974.D
 Acq On : 02 Feb 2022 14:43
 Operator : CG/JU
 Sample : N1307-09DL 20X
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0Q50DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
 Title : SVOA CALIBRATION

37	15.030	1999	2005	2008	rBV6	2709	5113	0.20%	0.043%
38	15.101	2013	2017	2021	rVB5	4560	5844	0.22%	0.049%
39	15.148	2021	2025	2027	rBV5	4244	6232	0.24%	0.052%
40	15.183	2027	2031	2039	rVB2	39719	59781	2.29%	0.497%
41	15.548	2084	2093	2099	rBV	96706	151863	5.81%	1.263%
42	15.607	2099	2103	2108	rVV2	15948	25658	0.98%	0.213%
43	15.677	2108	2115	2127	rVV	122378	215056	8.23%	1.788%
44	15.760	2127	2129	2133	rVB3	4737	5389	0.21%	0.045%
45	15.901	2148	2153	2158	rVB5	4108	7130	0.27%	0.059%
46	16.136	2187	2193	2197	rBV6	2689	5273	0.20%	0.044%
47	16.583	2264	2269	2272	rBV6	6539	10663	0.41%	0.089%
48	16.654	2277	2281	2283	rBV4	5706	7399	0.28%	0.062%
49	16.760	2294	2299	2302	rVB7	3469	5431	0.21%	0.045%
50	16.948	2325	2331	2349	rBV	1852832	2614212	100.00%	21.734%
51	17.083	2351	2354	2357	rVV4	7854	11653	0.45%	0.097%
52	17.113	2357	2359	2366	rVB3	5345	7690	0.29%	0.064%
53	17.295	2384	2390	2401	rBV	1264810	1845886	70.61%	15.346%
54	17.395	2402	2407	2418	rVV	110709	179556	6.87%	1.493%
55	17.495	2421	2424	2427	rVB4	3375	4390	0.17%	0.036%
56	17.707	2456	2460	2461	rBV4	2395	3096	0.12%	0.026%
57	19.677	2790	2795	2801	rBV	136158	188473	7.21%	1.567%
58	21.459	3093	3098	3105	rBV	1230861	1549899	59.29%	12.885%
59	23.847	3498	3504	3515	rVB2	695929	1342323	51.35%	11.160%




Sum of corrected areas: 12028326

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020122\
Data File : BM033974.D
Acq On : 02 Feb 2022 14:43
Operator : CG/JU
Sample : N1307-09DL 20X
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0Q50DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

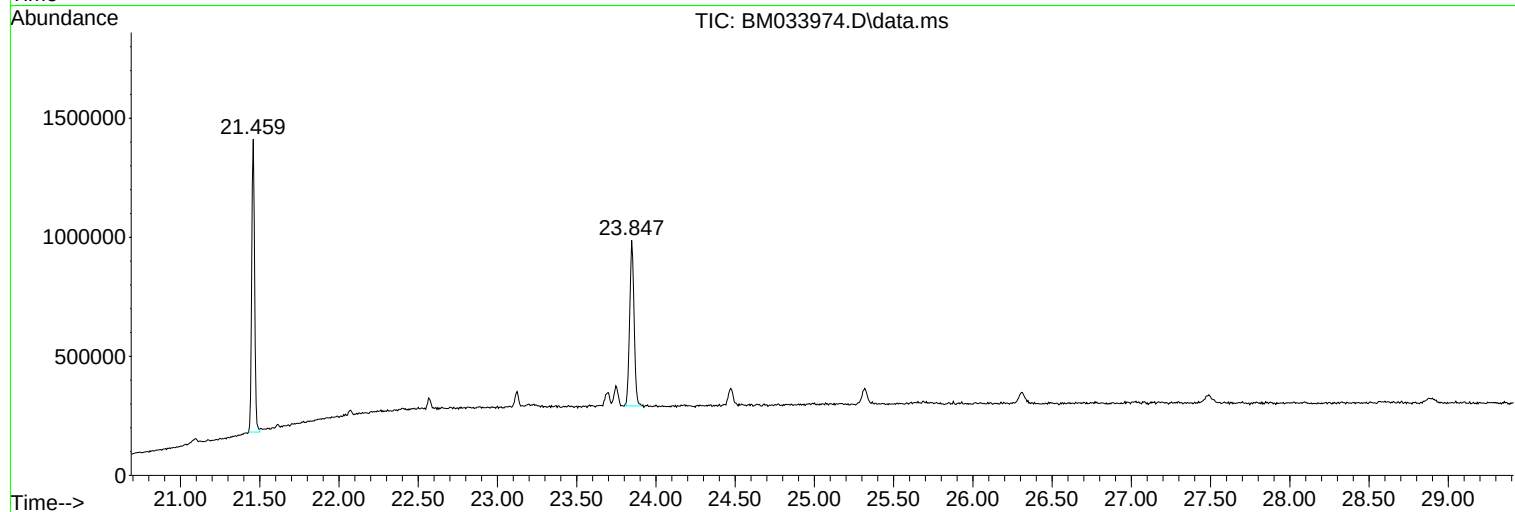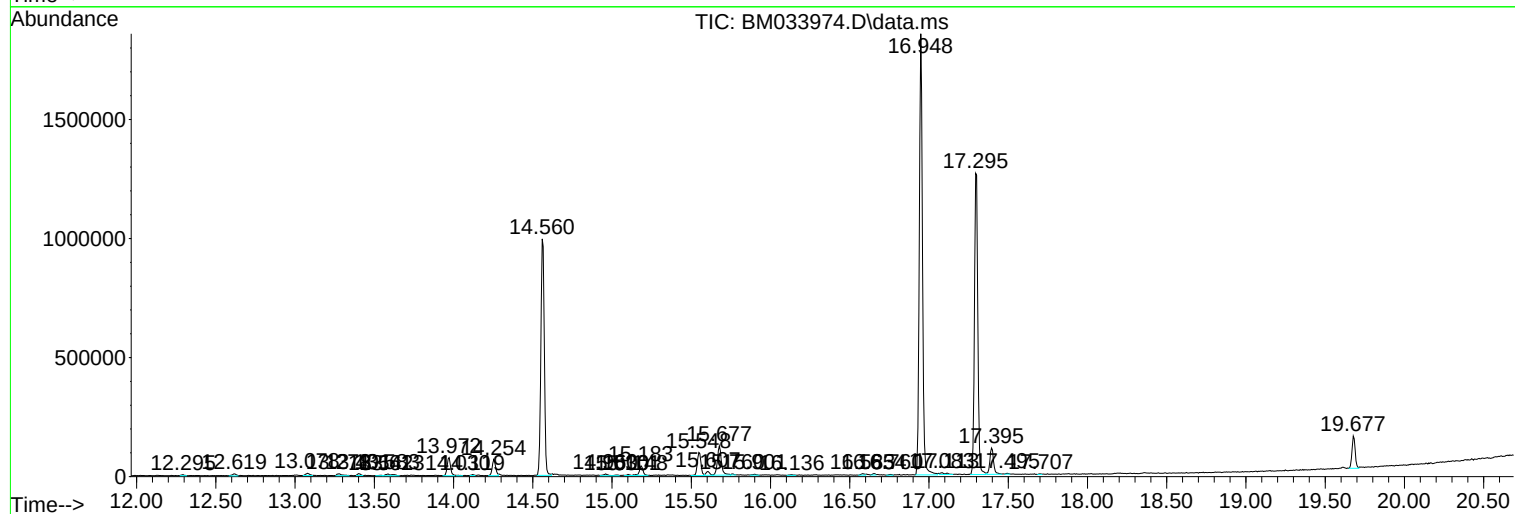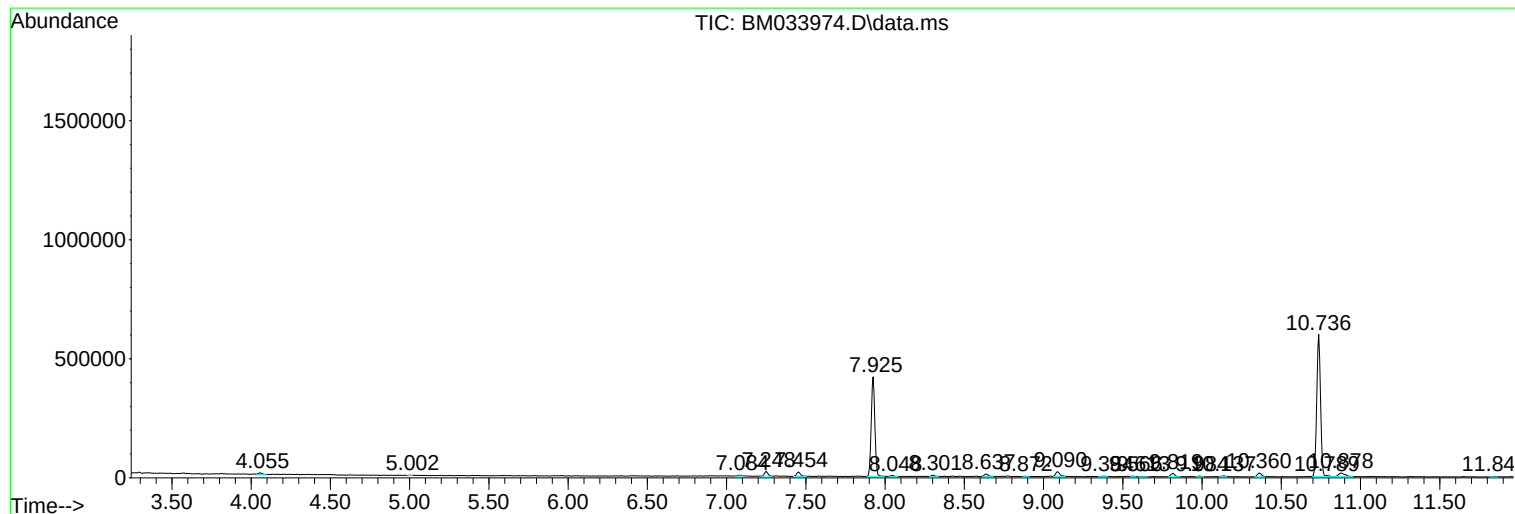

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020122\
Data File : BM033974.D
Acq On : 02 Feb 2022 14:43
Operator : CG/JU
Sample : N1307-09DL 20X
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0Q50DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020122\
Data File : BM033974.D
Acq On : 02 Feb 2022 14:43
Operator : CG/JU
Sample : N1307-09DL 20X
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0Q50DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc