

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020122\
 Data File : BM033975.D
 Acq On : 02 Feb 2022 15:19
 Operator : CG/JU
 Sample : N1307-05DL 30X
 Misc :
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0Q38DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
 Title : SVOA CALIBRATION

Signal : TIC: BM033975.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.054	137	139	143	rVB3	6807	8098	0.27%	0.071%
2	7.084	651	654	658	rVB5	2442	3652	0.12%	0.032%
3	7.248	677	682	687	rBV	12383	19746	0.65%	0.173%
4	7.454	711	717	724	rBV	12296	22074	0.73%	0.193%
5	7.925	790	797	804	rBV	410380	643844	21.34%	5.636%
6	8.637	914	918	923	rBV4	6080	9816	0.33%	0.086%
7	9.089	990	995	1002	rBV	12473	23429	0.78%	0.205%
8	9.813	1114	1118	1126	rBV5	8104	14821	0.49%	0.130%
9	10.366	1207	1212	1223	rBV5	7159	15247	0.51%	0.133%
10	10.736	1268	1275	1284	rVB	569833	963558	31.93%	8.435%
11	10.878	1295	1299	1300	rBV5	3659	3255	0.11%	0.028%
12	11.860	1458	1466	1467	rBV5	2126	3057	0.10%	0.027%
13	12.295	1535	1540	1546	rBV5	2370	3044	0.10%	0.027%
14	13.971	1818	1825	1830	rBV	45369	67147	2.23%	0.588%
15	14.254	1866	1873	1879	rBV	41358	64464	2.14%	0.564%
16	14.560	1918	1925	1934	rBV	978880	1456556	48.27%	12.751%
17	15.107	2014	2018	2021	rBV3	9282	12241	0.41%	0.107%
18	15.183	2026	2031	2043	rVB2	32502	50319	1.67%	0.441%
19	15.548	2087	2093	2100	rBV	56963	89194	2.96%	0.781%
20	15.677	2109	2115	2126	rBV7	17363	40663	1.35%	0.356%
21	16.948	2325	2331	2343	rBV	2165641	3017337	100.00%	26.415%
22	17.065	2348	2351	2352	rVV3	5803	7035	0.23%	0.062%
23	17.083	2352	2354	2360	rVB5	5689	9978	0.33%	0.087%
24	17.301	2384	2391	2402	rVV	1219318	1772638	58.75%	15.518%
25	17.395	2402	2407	2416	rVB	71831	111223	3.69%	0.974%
26	18.195	2540	2543	2548	rBV7	5627	9980	0.33%	0.087%
27	19.606	2781	2783	2787	rVB5	7692	7908	0.26%	0.069%
28	19.683	2791	2796	2800	rBV	79571	109187	3.62%	0.956%
29	21.459	3093	3098	3107	rBV	1240763	1565291	51.88%	13.703%
30	23.847	3498	3504	3513	rVB2	663729	1298044	43.02%	11.364%




Sum of corrected areas: 11422846

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020122\
Data File : BM033975.D
Acq On : 02 Feb 2022 15:19
Operator : CG/JU
Sample : N1307-05DL 30X
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0Q38DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

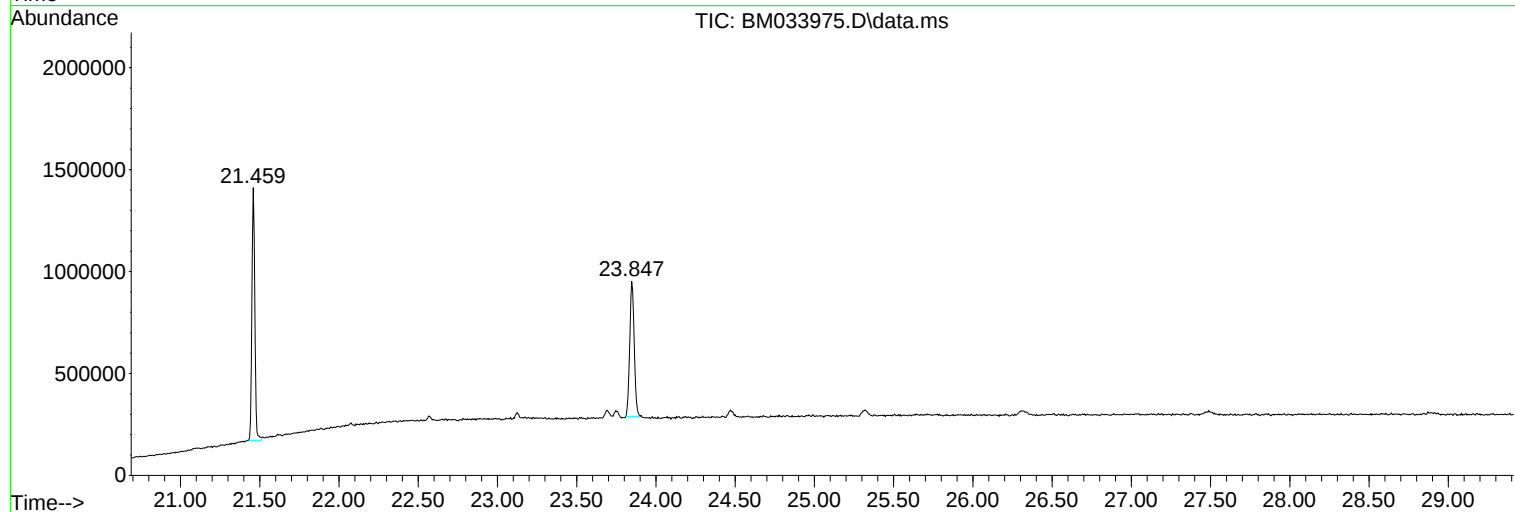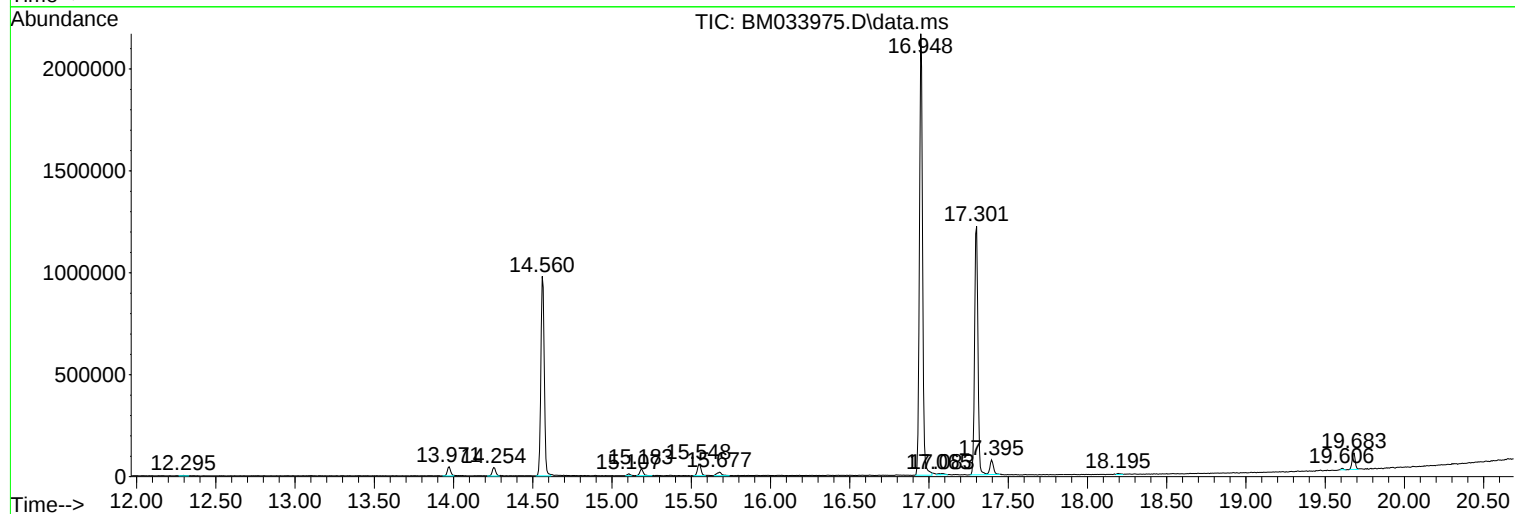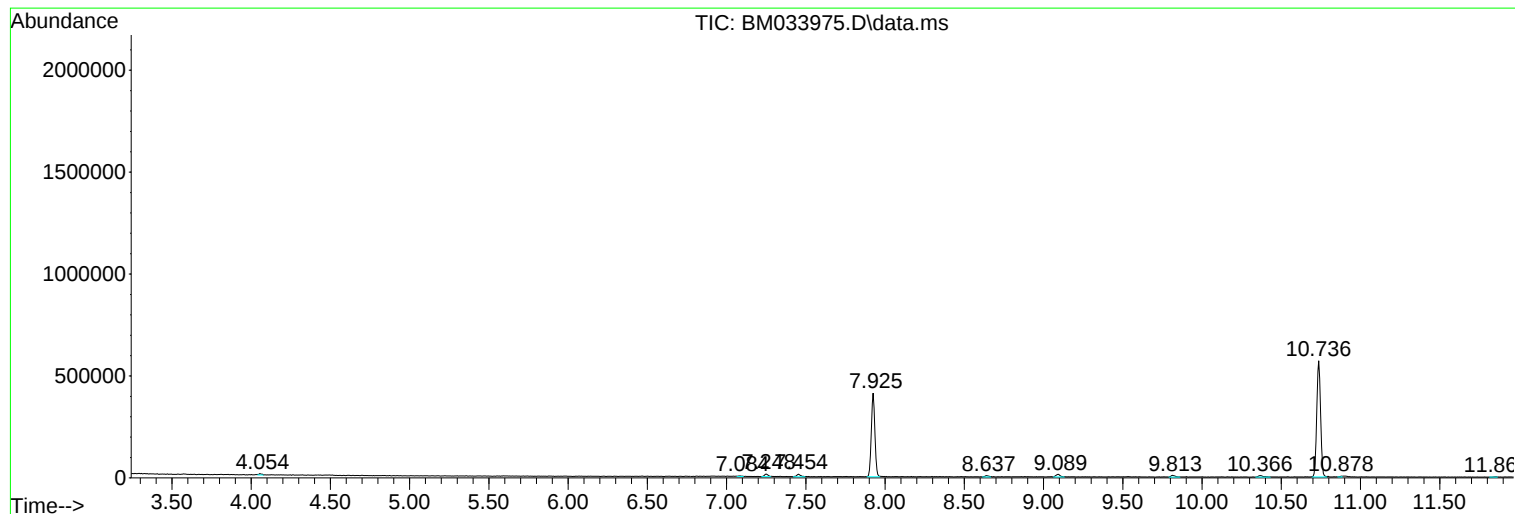

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020122\
Data File : BM033975.D
Acq On : 02 Feb 2022 15:19
Operator : CG/JU
Sample : N1307-05DL 30X
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0Q38DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020122\
Data File : BM033975.D
Acq On : 02 Feb 2022 15:19
Operator : CG/JU
Sample : N1307-05DL 30X
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0Q38DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------