

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020122\
 Data File : BM033977.D
 Acq On : 02 Feb 2022 16:38
 Operator : CG/JU
 Sample : PB142419BL
 Misc :
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK419

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
 Title : SVOA CALIBRATION

Signal : TIC: BM033977.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.284	4	8	14	rVB	29978	40627	1.40%	0.135%
2	3.713	77	81	102	rBV	383015	594124	20.40%	1.970%
3	4.055	136	139	146	rVB4	8312	12810	0.44%	0.042%
4	7.078	647	653	662	rBV	464343	728637	25.02%	2.415%
5	7.249	674	682	691	rBV	382918	588694	20.22%	1.952%
6	7.449	709	716	726	rBV	483872	764160	26.24%	2.533%
7	7.925	789	797	805	rVB	404245	629815	21.63%	2.088%
8	8.301	855	861	863	rBV6	1381	3042	0.10%	0.010%
9	8.631	910	917	929	rBV	591614	944539	32.44%	3.131%
10	9.084	986	994	1004	rBV	481337	788296	27.07%	2.613%
11	9.813	1109	1118	1126	rBV	406899	661901	22.73%	2.194%
12	10.354	1202	1210	1224	rBV	567585	969675	33.30%	3.214%
13	10.737	1267	1275	1283	rBV	568236	947822	32.55%	3.142%
14	10.866	1290	1297	1310	rBV	601326	1050051	36.06%	3.481%
15	11.407	1383	1389	1394	rBV4	1323	3386	0.12%	0.011%
16	12.325	1541	1545	1554	rBV3	8946	15942	0.55%	0.053%
17	13.972	1818	1825	1838	rBV	1334674	1787465	61.38%	5.925%
18	14.254	1867	1873	1882	rBV	1348568	1908325	65.54%	6.326%
19	14.560	1917	1925	1939	rVB	958148	1419810	48.76%	4.707%
20	14.748	1951	1957	1978	rBV	379748	742665	25.50%	2.462%
21	15.548	2087	2093	2103	rBV	1706303	2455133	84.31%	8.139%
22	15.660	2106	2112	2128	rVV	536874	790545	27.15%	2.621%
23	15.789	2130	2134	2138	rVB2	10903	12822	0.44%	0.043%
24	17.083	2350	2354	2359	rBV3	3984	6444	0.22%	0.021%
25	17.295	2384	2390	2397	rBV	1240672	1726105	59.28%	5.722%
26	17.395	2401	2407	2417	rBV2	1906475	2673739	91.82%	8.864%
27	17.965	2500	2504	2505	rBV4	2672	3612	0.12%	0.012%
28	18.207	2541	2545	2548	rBV5	3329	5299	0.18%	0.018%
29	18.424	2580	2582	2584	rBV3	2899	3319	0.11%	0.011%
30	19.248	2718	2722	2727	rBV	22745	27552	0.95%	0.091%
31	19.318	2730	2734	2738	rVV	20281	25009	0.86%	0.083%
32	19.683	2789	2796	2803	rBV	2147701	2911904	100.00%	9.653%
33	21.459	3093	3098	3107	rBV	1215659	1556507	53.45%	5.160%
34	23.695	3471	3478	3485	rBV2	1079081	2079714	71.42%	6.894%
35	23.847	3498	3504	3514	rVB2	649448	1286185	44.17%	4.264%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020122\
Data File : BM033977.D
Acq On : 02 Feb 2022 16:38
Operator : CG/JU
Sample : PB142419BL
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK419

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
Title : SVOA CALIBRATION


Sum of corrected areas: 30165675

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020122\
Data File : BM033977.D
Acq On : 02 Feb 2022 16:38
Operator : CG/JU
Sample : PB142419BL
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK419

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

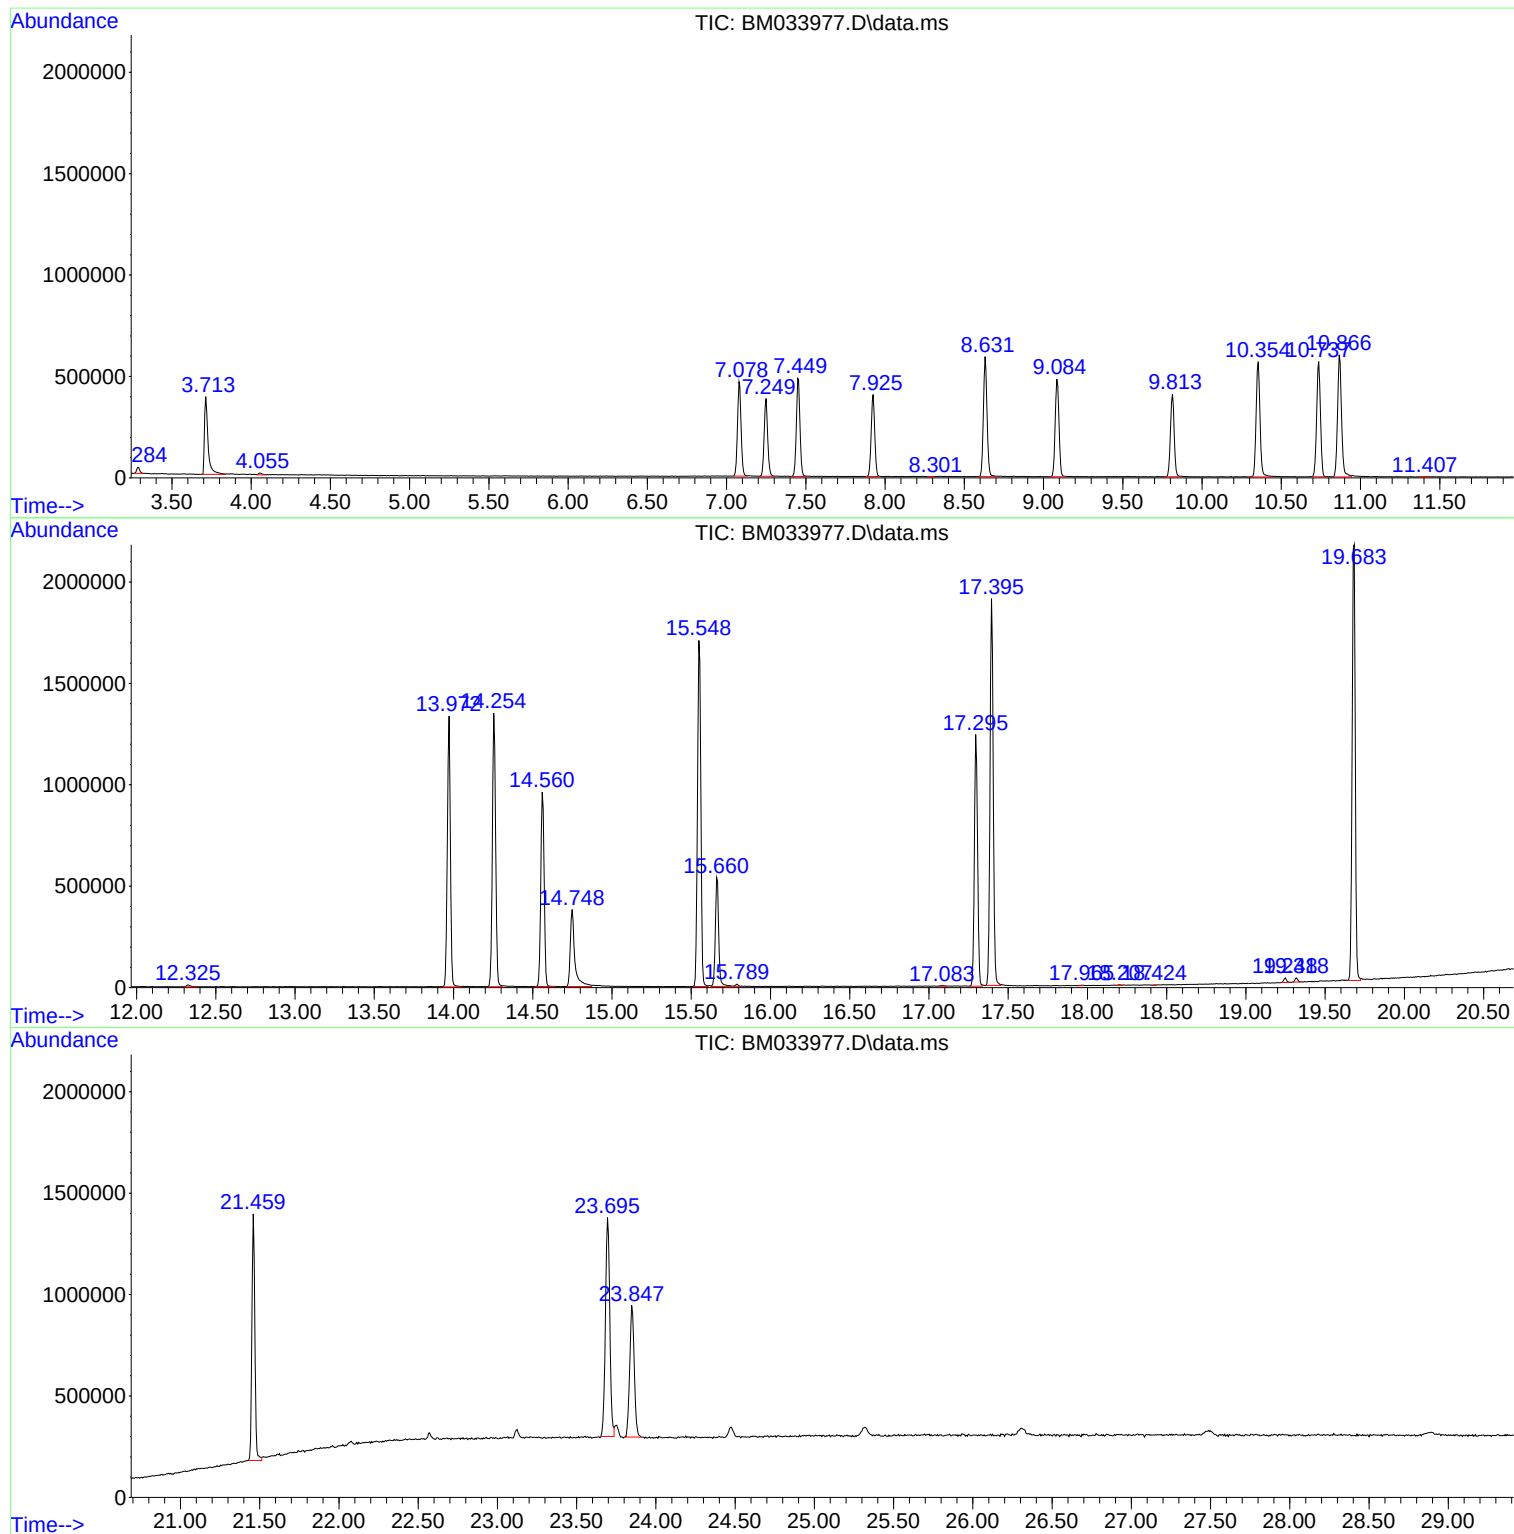

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020122\
Data File : BM033977.D
Acq On : 02 Feb 2022 16:38
Operator : CG/JU
Sample : PB142419BL
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK419

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020122\
Data File : BM033977.D
Acq On : 02 Feb 2022 16:38
Operator : CG/JU
Sample : PB142419BL
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK419

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------