
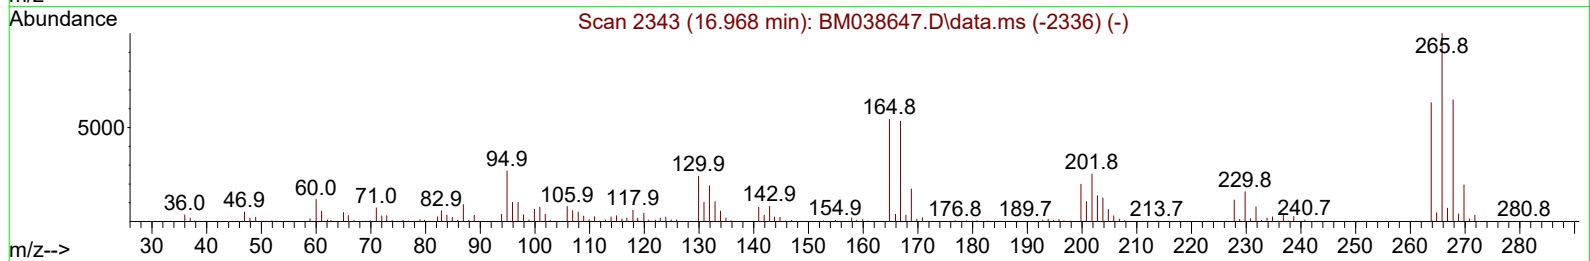
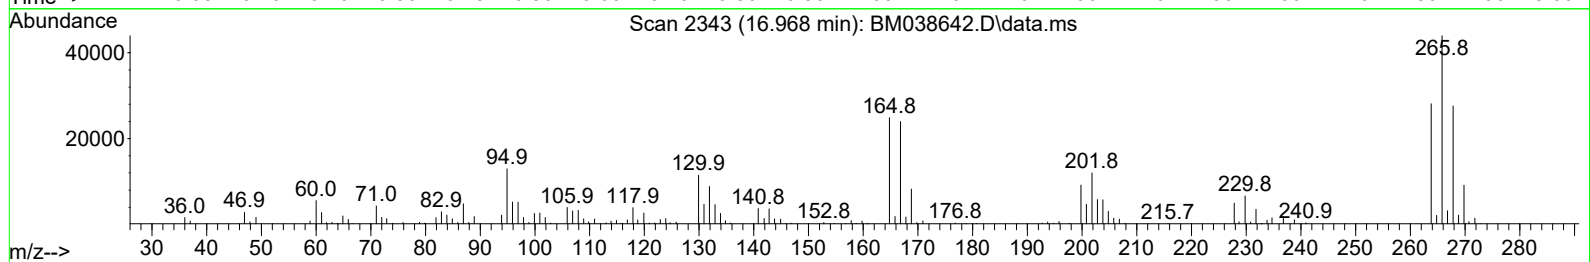


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020123\
Data File : BM038642.D
Acq On : 01 Feb 2023 14:43
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 02 05:39:39 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM020123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 02 03:31:45 2023
Response via : Initial Calibration

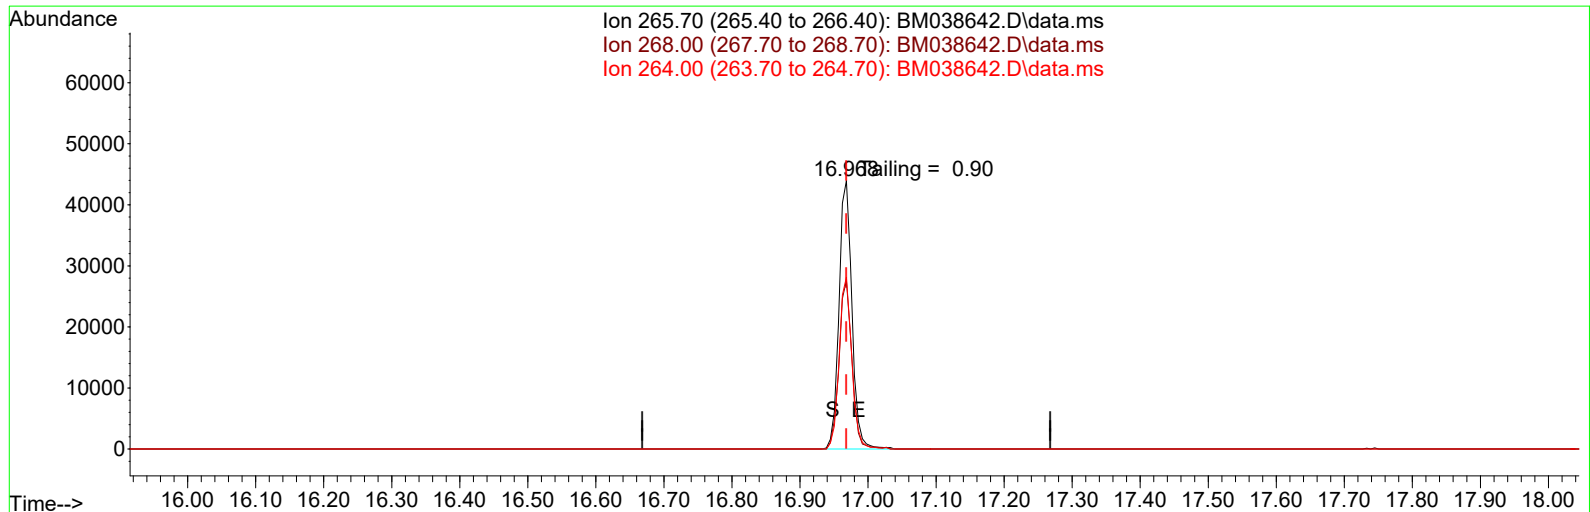

TIC: BM038642.D\data.ms

(70) Pentachlorophenol (C)




16.968min (+ 0.000) 0.00 ng

response 58010

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.70	62.81
264.00	63.30	63.96
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020123\
Data File : BM038642.D
Acq On : 01 Feb 2023 14:43
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 02 05:39:39 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM020123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 02 03:31:45 2023
Response via : Initial Calibration

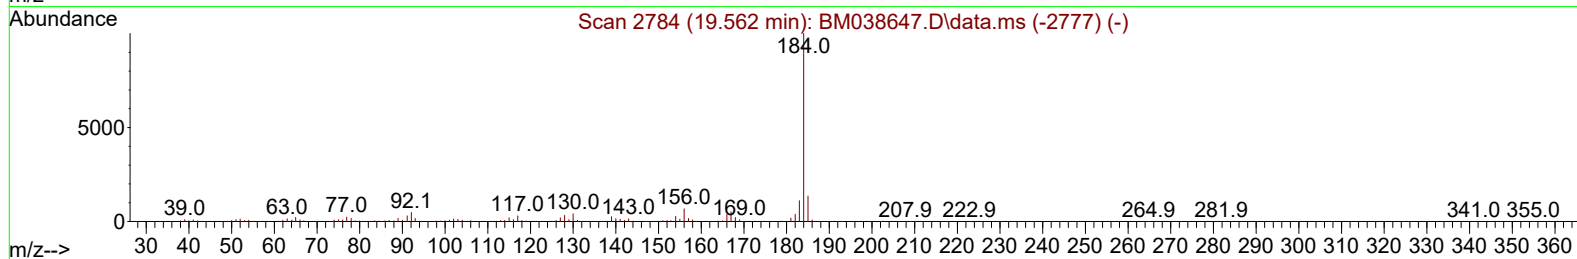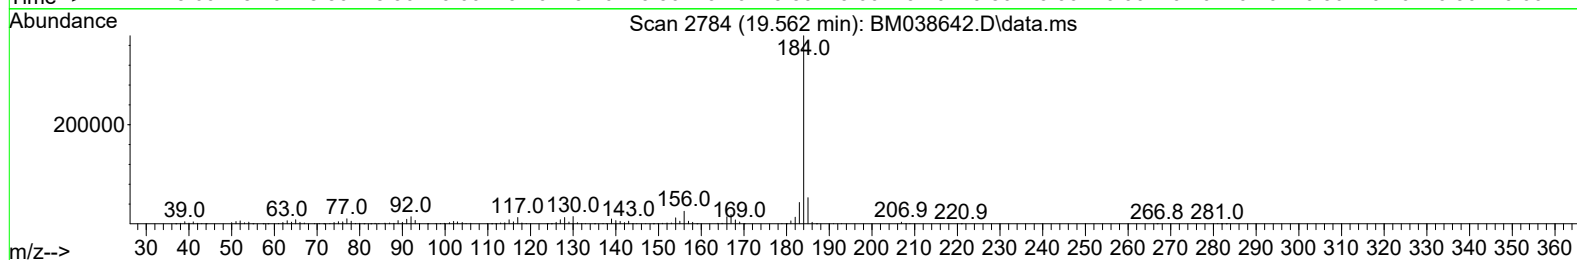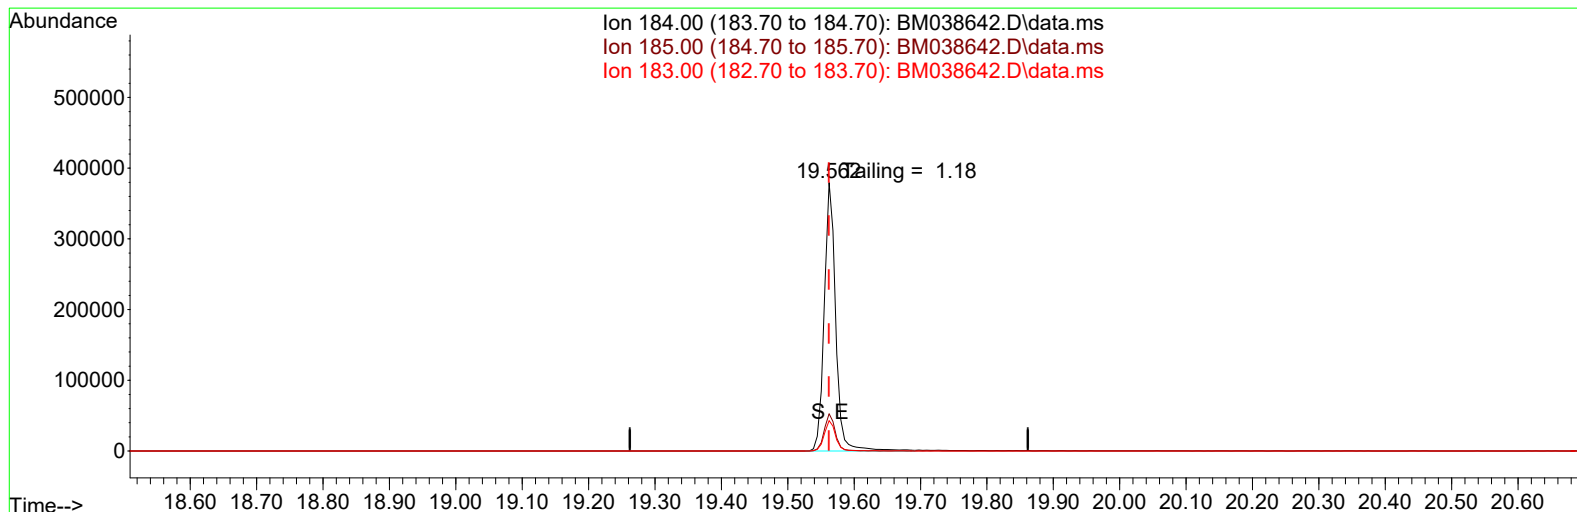

TIC: BM038642.D\data.ms

(77) Benzidine**19.562min (+ 0.000) 0.00 ng****response 457171**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.50	13.94
183.00	11.00	11.37
0.00	0.00	0.00