

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020123\
 Data File : BM038655.D
 Acq On : 01 Feb 2023 23:21
 Operator : CG/JU
 Sample : PB150362BL
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB150362BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM020123.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM038655.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.022	307	312	321	rBV	234773	314757	12.00%	2.659%
2	5.493	386	392	404	rBV	689150	943230	35.97%	7.969%
3	7.105	658	666	676	rBV	600158	901690	34.38%	7.618%
4	7.934	801	807	814	rBV	211975	325752	12.42%	2.752%
5	9.110	999	1007	1020	rBV	534716	859002	32.75%	7.258%
6	10.746	1278	1285	1300	rBV	235292	384427	14.66%	3.248%
7	13.198	1696	1702	1713	rBV	1697020	2287798	87.23%	19.330%
8	14.575	1930	1936	1947	rVB	384191	519230	19.80%	4.387%
9	16.063	2183	2189	2198	rBV	694484	955493	36.43%	8.073%
10	17.316	2396	2402	2412	rBV	397079	530391	20.22%	4.481%
11	19.933	2841	2847	2852	rBV	2280385	2622615	100.00%	22.159%
12	21.492	3107	3112	3117	rBV	414453	537941	20.51%	4.545%
13	23.886	3513	3519	3531	rVB2	327369	653241	24.91%	5.519%




Sum of corrected areas: 11835567

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020123\
Data File : BM038655.D
Acq On : 01 Feb 2023 23:21
Operator : CG/JU
Sample : PB150362BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB150362BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM020123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

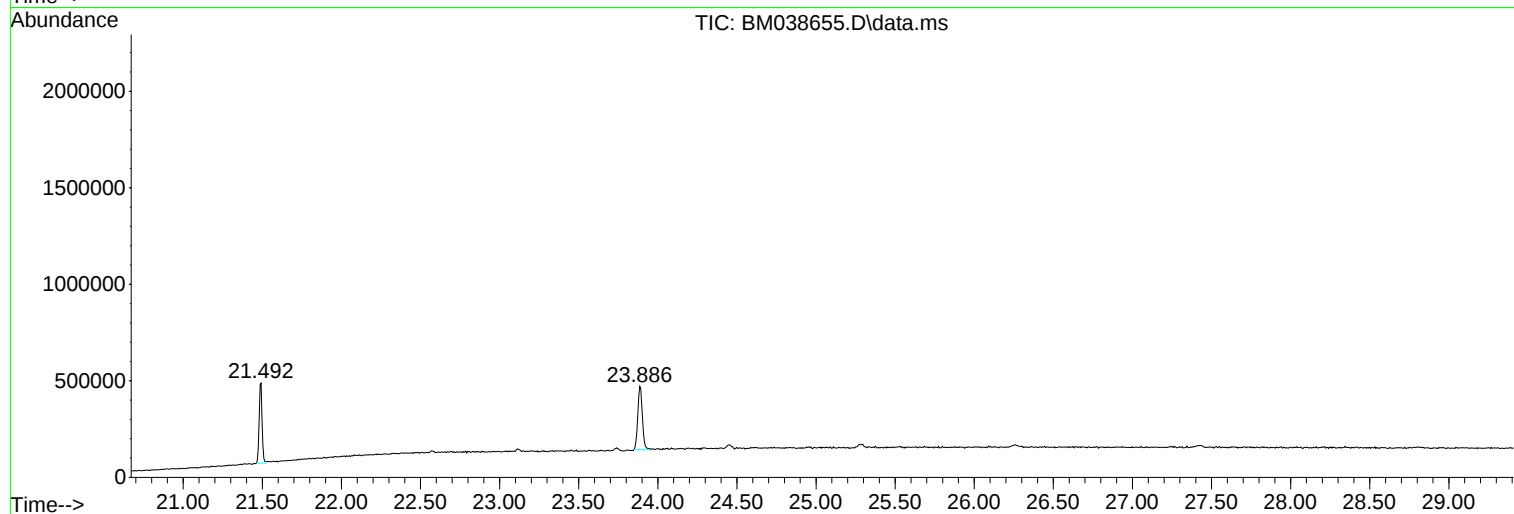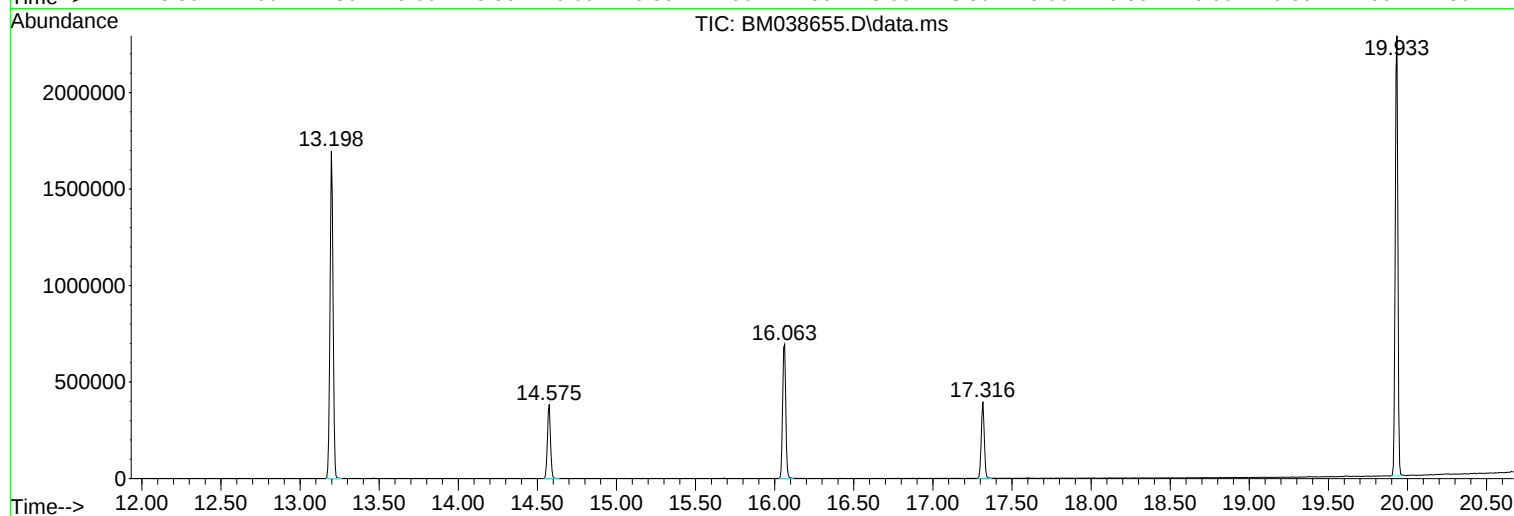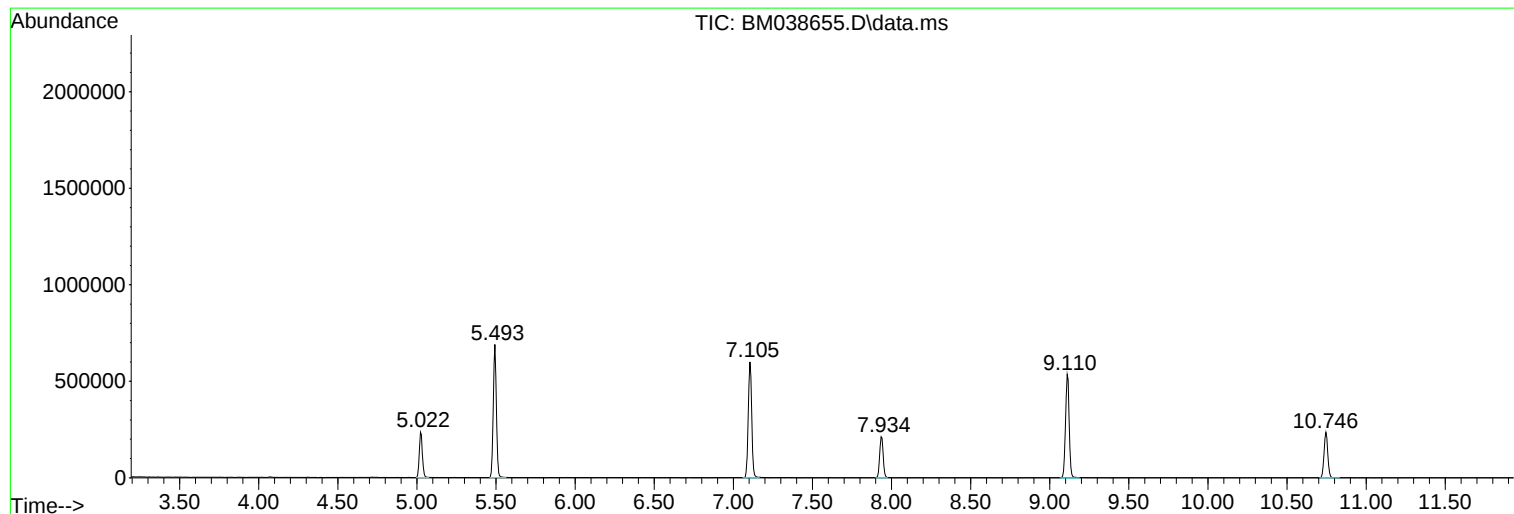

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020123\
Data File : BM038655.D
Acq On : 01 Feb 2023 23:21
Operator : CG/JU
Sample : PB150362BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB150362BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM020123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.022	19.32 ng	314757	1,4-Dichlorobenzene-d4	7.934

Hit#	of 5	Tentative ID	MW	MolForm	CAS#	Qual
1		2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	56
2		2,3-Butanedione, monooxime	101	C4H7NO2	000057-71-6	25
3		1-Propen-2-ol, acetate	100	C5H8O2	000108-22-5	10
4		Butane, 1-ethoxy-	102	C6H14O	000628-81-9	9
5		Propanenitrile, 3-ethoxy-	99	C5H9NO	002141-62-0	9

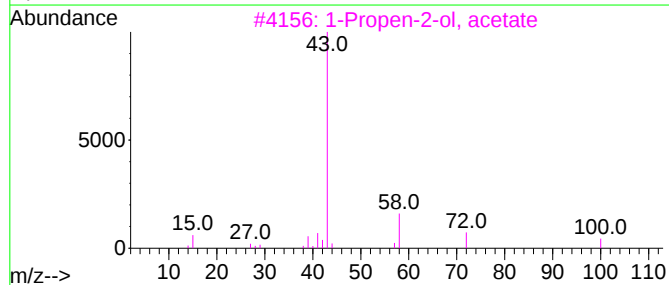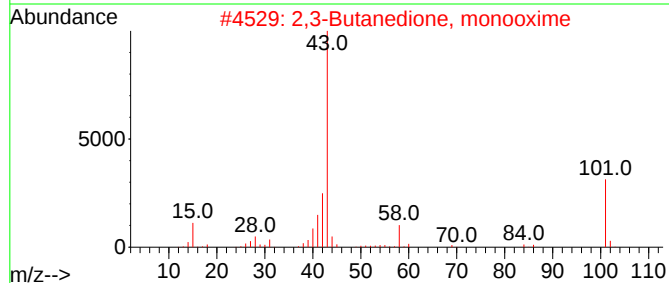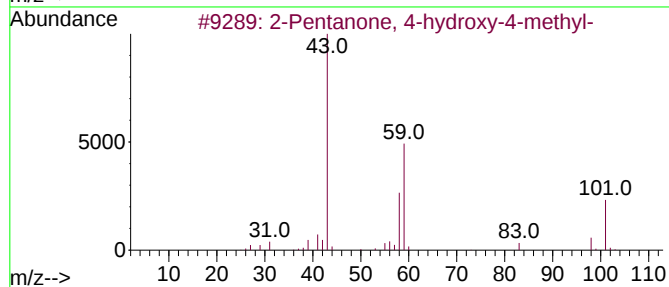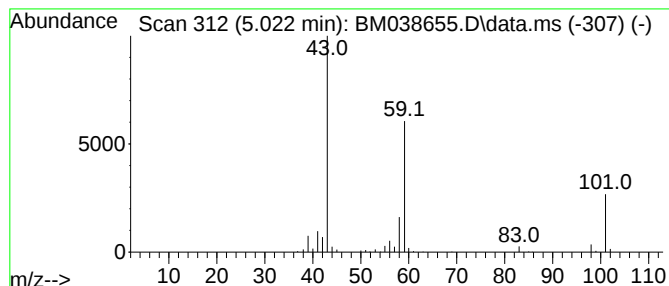

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020123\
Data File : BM038655.D
Acq On : 01 Feb 2023 23:21
Operator : CG/JU
Sample : PB150362BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB150362BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM020123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	5.022	19.3	ng	314757	1	7.934	325752	20.0