


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020123\
Data File : BM038642.D
Acq On : 01 Feb 2023 14:43
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM020123.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Feb 02 03:31:45 2023

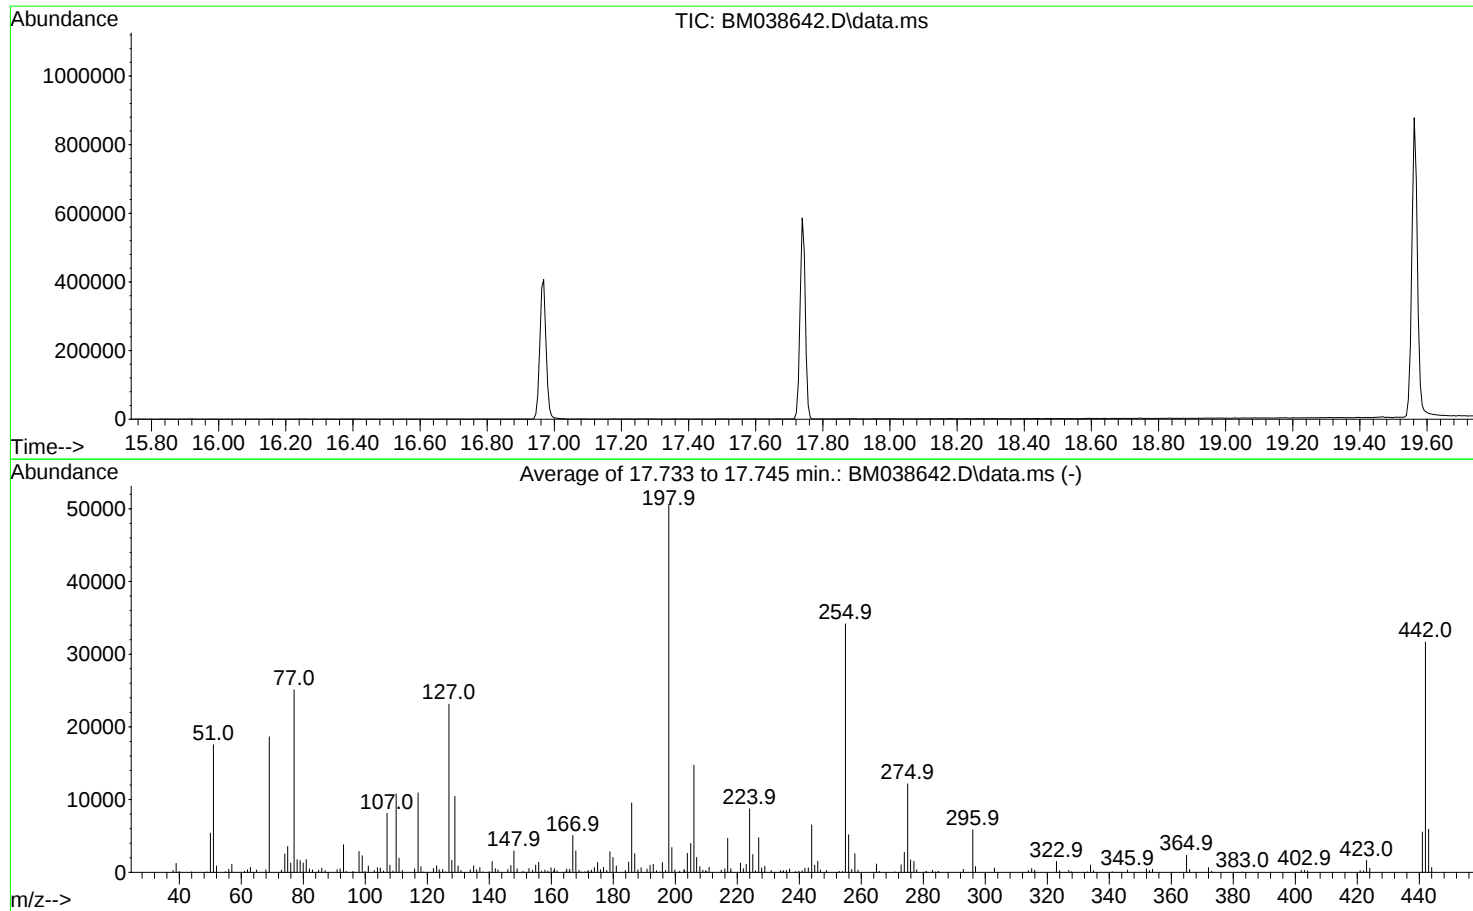




AutoFind: Scans 2473, 2474, 2475; Background Corrected with Scan 2467

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.7	17557	PASS
68	69	0.00	2	1.8	338	PASS
69	198	0.00	100	36.8	18643	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	45.7	23115	PASS
197	198	0.00	2	0.5	249	PASS
198	198	100	100	100.0	50603	PASS
199	198	5	9	6.7	3404	PASS
275	198	10	60	24.0	12159	PASS
365	198	1	100	4.6	2342	PASS
441	198	0.01	100	10.9	5534	PASS
442	442	50	100	100.0	31661	PASS
443	442	15	24	18.7	5915	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020123\
Data File : BM038642.D
Acq On : 01 Feb 2023 14:43
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Feb 02 05:39:39 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM020123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 02 03:31:45 2023
Response via : Initial Calibration

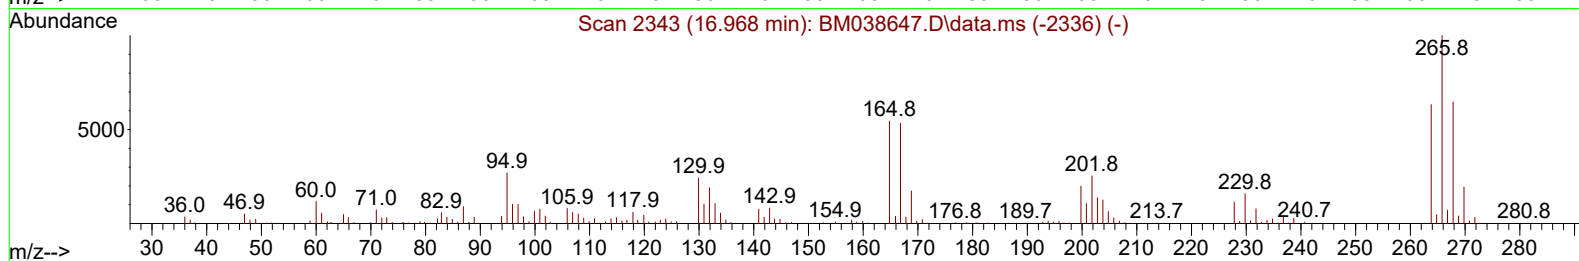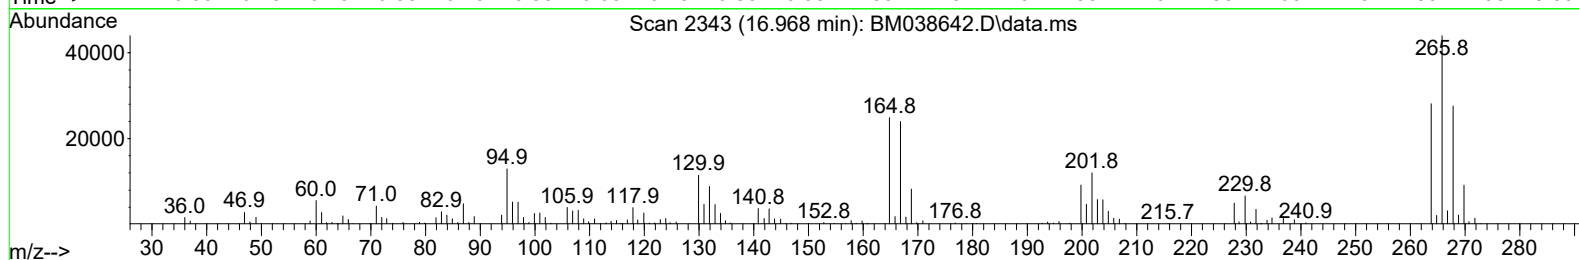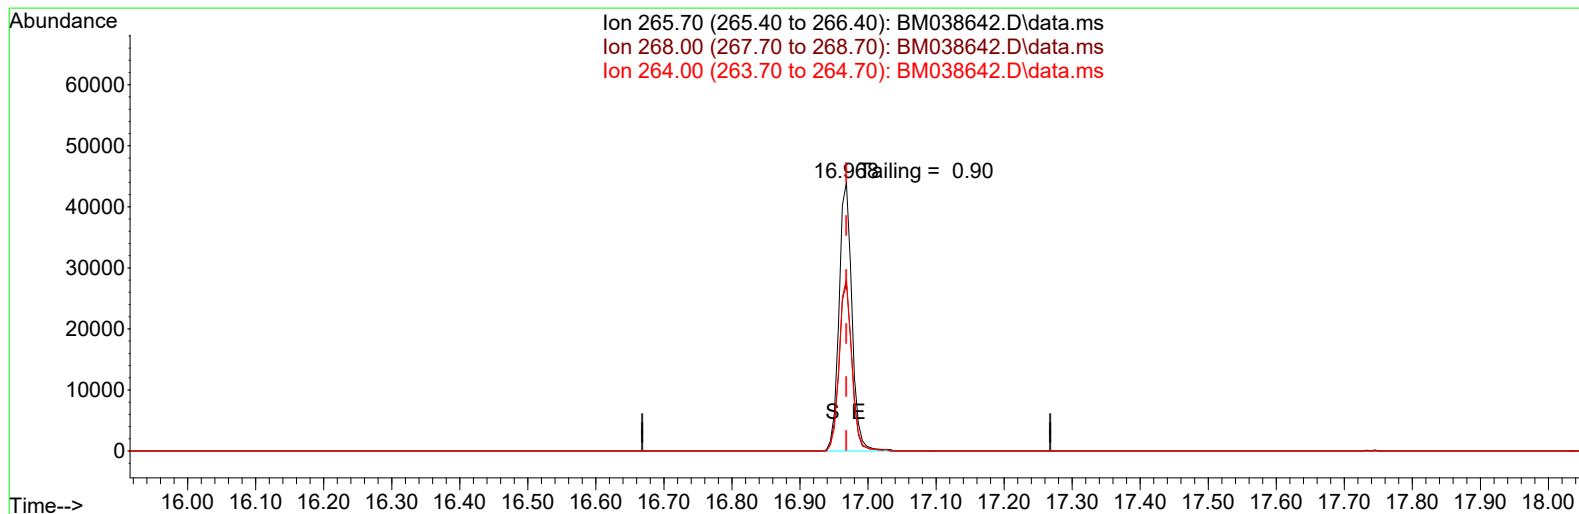

TIC: BM038642.D\data.ms

(70) Pentachlorophenol (C)

16.968min (+ 0.000) 0.00 ng




response 58010

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.70	62.81
264.00	63.30	63.96
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020123\
Data File : BM038642.D
Acq On : 01 Feb 2023 14:43
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Feb 02 05:39:39 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM020123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 02 03:31:45 2023
Response via : Initial Calibration

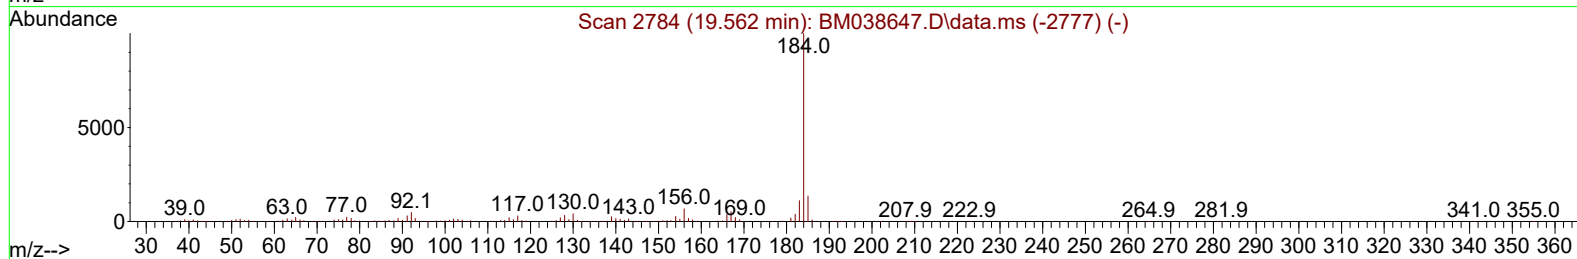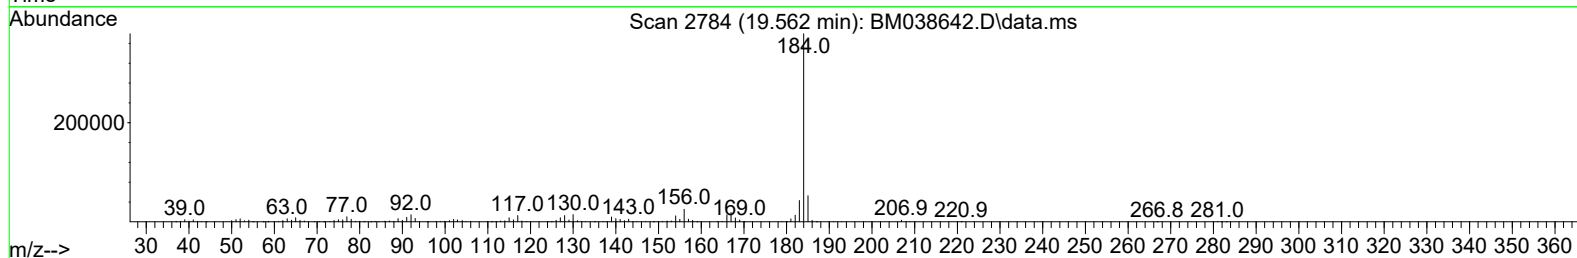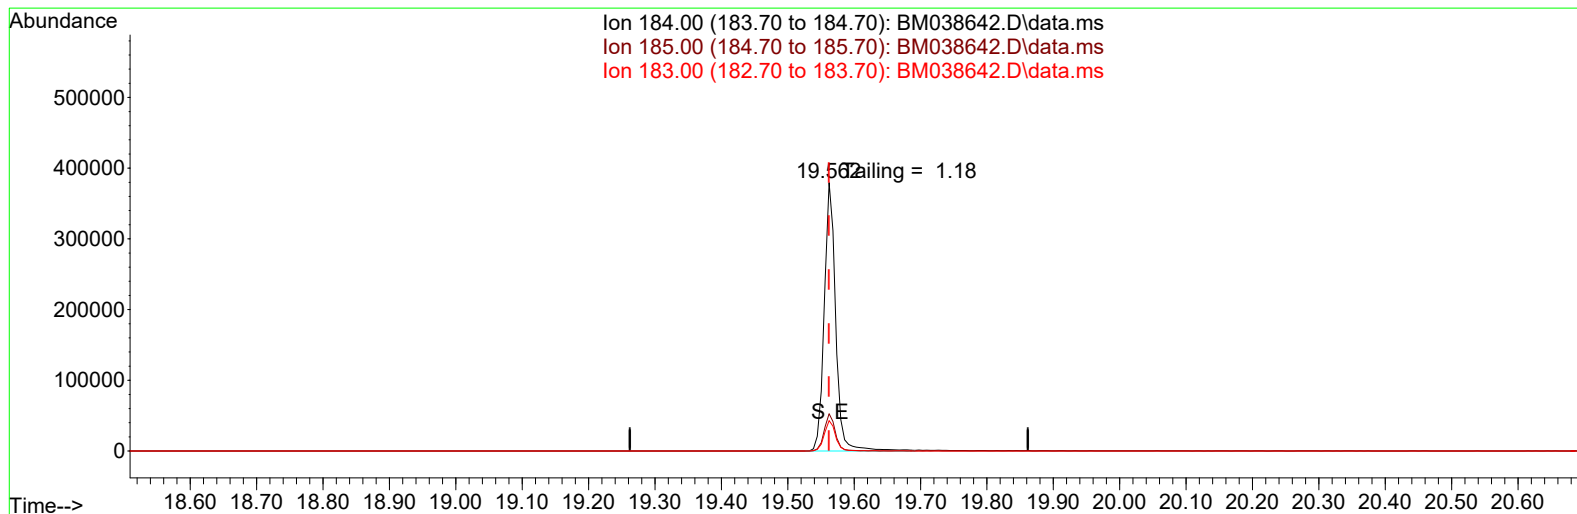

TIC: BM038642.D\data.ms

(77) Benzidine

19.562min (+ 0.000) 0.00 ng

response 457171

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.50	13.94
183.00	11.00	11.37
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/1/2023	BNA_M	<u>BM038642.D</u>
Compound Name	Response	Retention Time
DDT	182210	20.786
DDD	1226	20.397
DDE	0	19.868
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
1226	183436	0.67

Instrument :
BNA_M
ClientSampleId :
DFTPP