
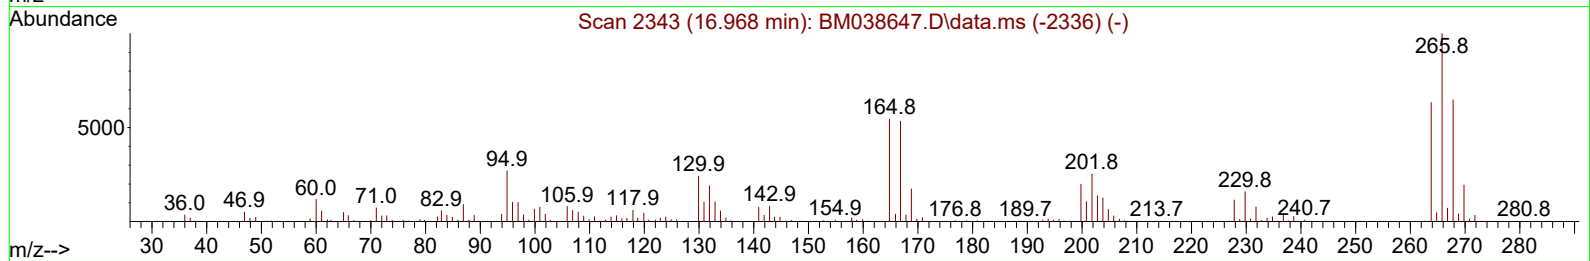
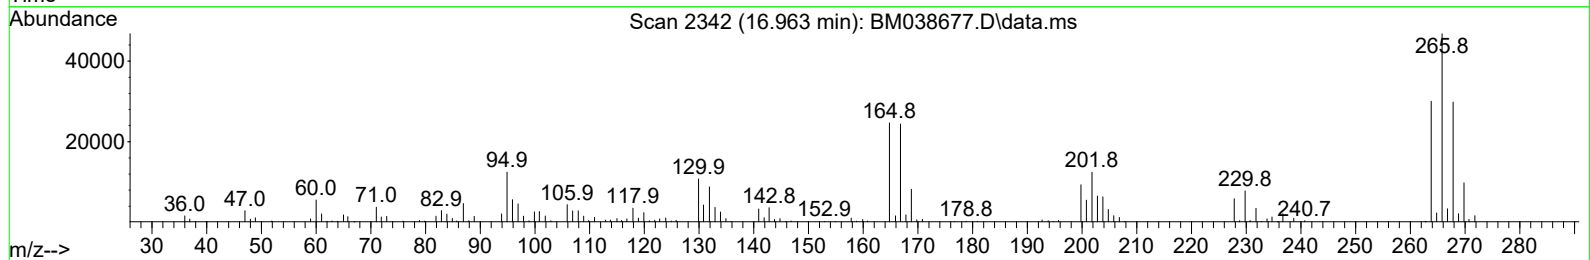


Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM020323\  
Data File : BM038677.D  
Acq On : 03 Feb 2023 12:36  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 04 04:21:23 2023  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM020123.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Feb 02 03:31:45 2023  
Response via : Initial Calibration

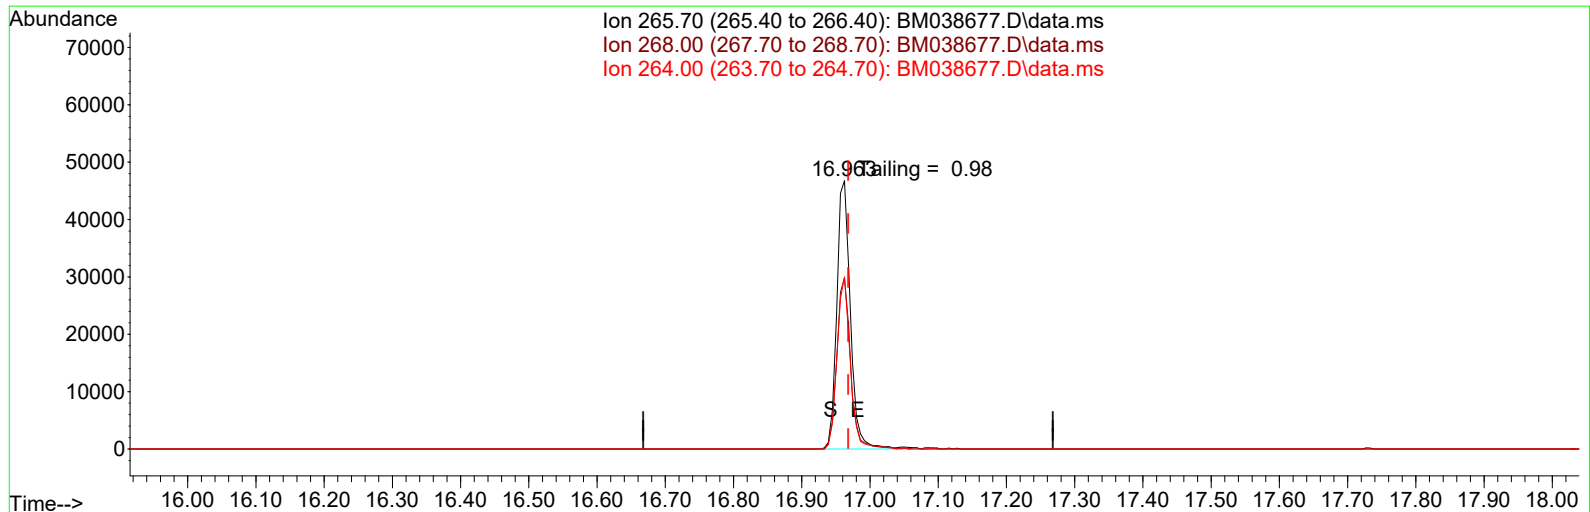

TIC: BM038677.D\data.ms

**(70) Pentachlorophenol (C)**




16.963min (-0.005) 0.00 ng

response 64777

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 64.70  | 63.78  |
| 264.00 | 63.30  | 64.18  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM020323\  
Data File : BM038677.D  
Acq On : 03 Feb 2023 12:36  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 04 04:21:23 2023  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM020123.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Feb 02 03:31:45 2023  
Response via : Initial Calibration

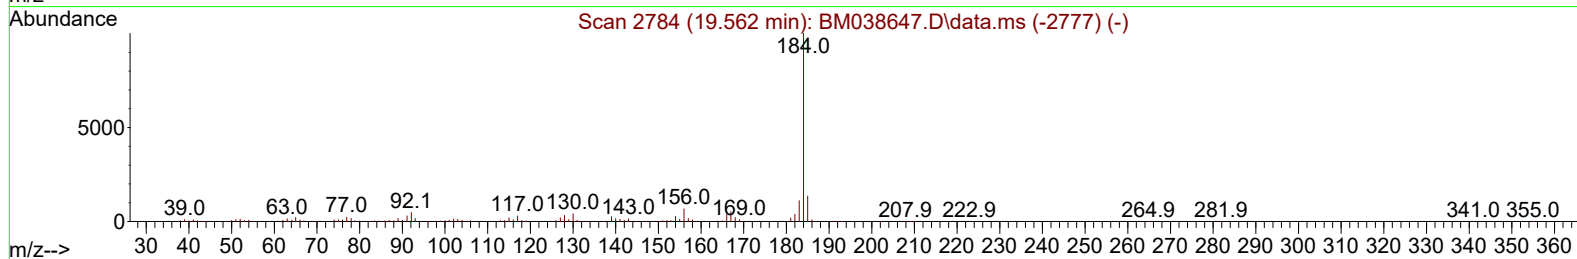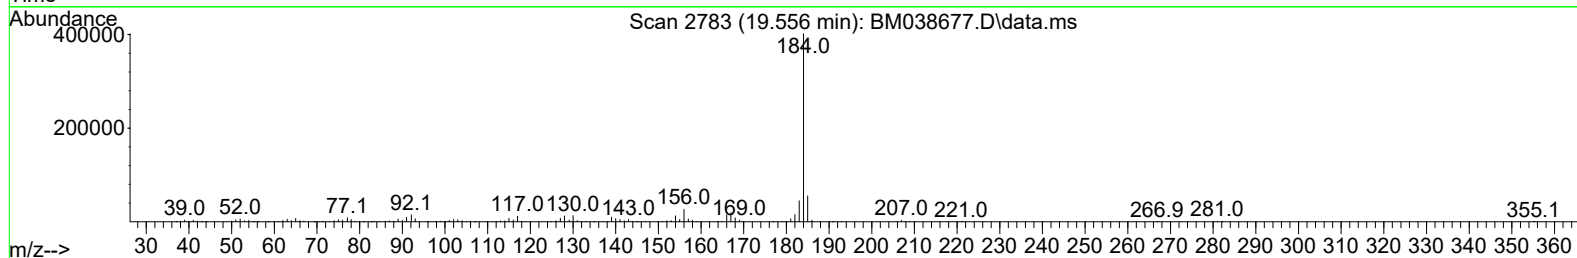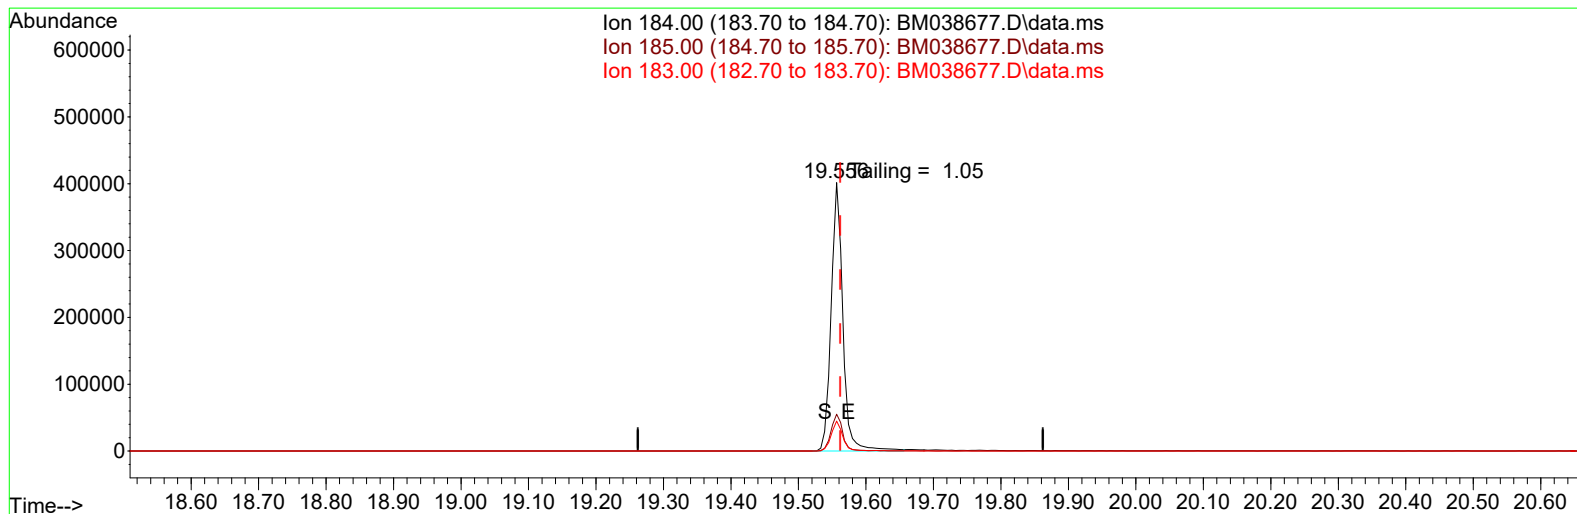

TIC: BM038677.D\data.ms

**(77) Benzidine**

19.556min (-0.006) 0.00 ng

response 484405

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 13.50  | 13.72  |
| 183.00 | 11.00  | 11.16  |
| 0.00   | 0.00   | 0.00   |