

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020323\
 Data File : BM038679.D
 Acq On : 03 Feb 2023 14:06
 Operator : CG/JU
 Sample : PB150629BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB150629BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM020123.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM038679.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.010	305	310	320	rVB	230855	310135	11.30%	2.582%
2	5.487	385	391	401	rBV	688755	946325	34.48%	7.880%
3	7.104	659	666	680	rBV	576574	898486	32.73%	7.481%
4	7.928	799	806	815	rVB	204745	322119	11.74%	2.682%
5	9.098	998	1005	1019	rBV	520651	852180	31.05%	7.096%
6	10.733	1274	1283	1291	rBV	231597	376217	13.71%	3.133%
7	13.192	1694	1701	1714	rBV	1744452	2365654	86.18%	19.698%
8	14.563	1928	1934	1947	rBV	366822	516250	18.81%	4.299%
9	16.057	2182	2188	2201	rBV	658569	932735	33.98%	7.767%
10	17.309	2394	2401	2411	rBV	399630	533829	19.45%	4.445%
11	19.927	2840	2846	2851	rBV	2490690	2744915	100.00%	22.856%
12	21.486	3106	3111	3117	rBV	447268	539131	19.64%	4.489%
13	23.880	3512	3518	3531	rBV	346666	671522	24.46%	5.592%




Sum of corrected areas: 12009498

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020323\
Data File : BM038679.D
Acq On : 03 Feb 2023 14:06
Operator : CG/JU
Sample : PB150629BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB150629BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM020123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

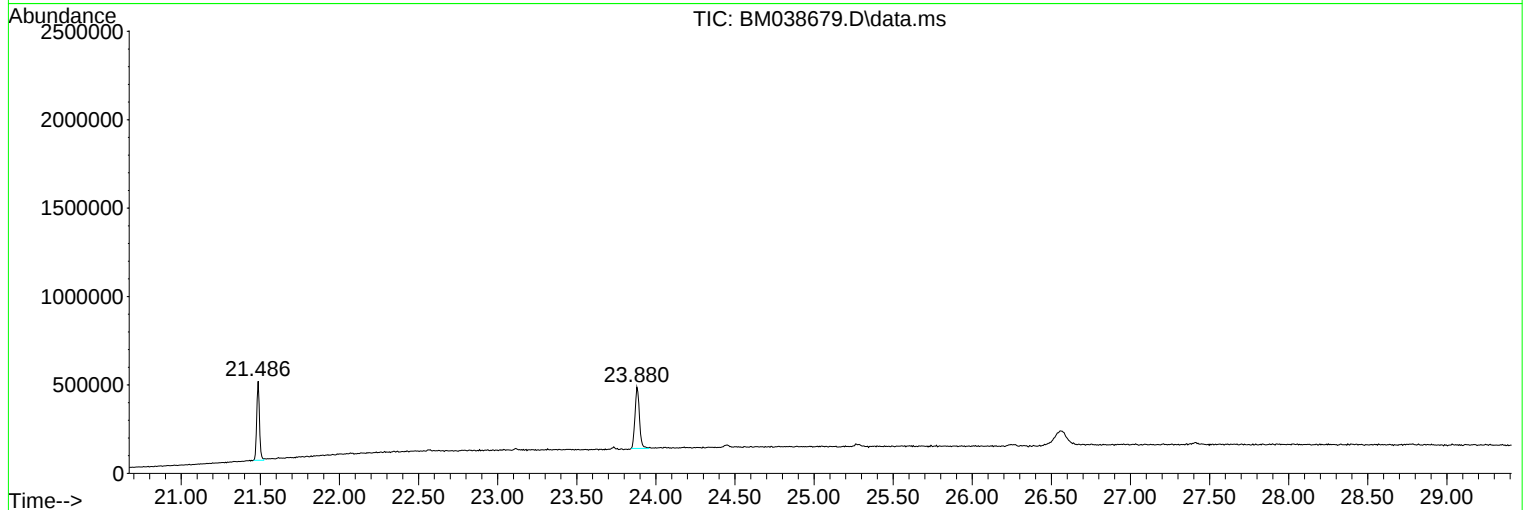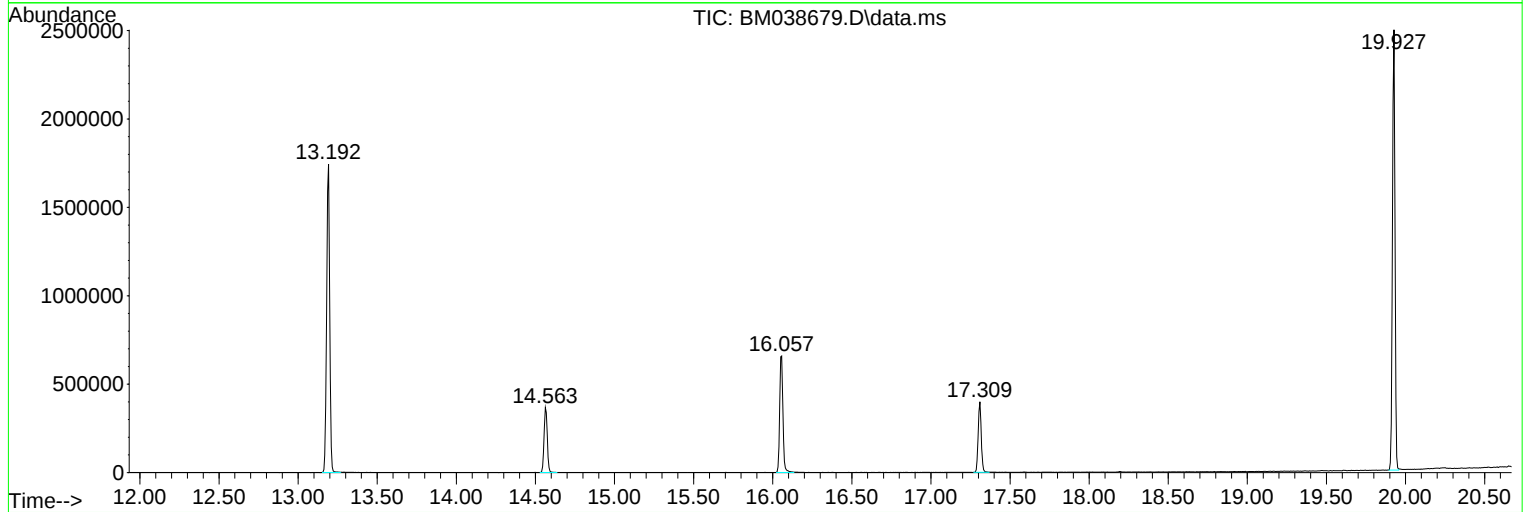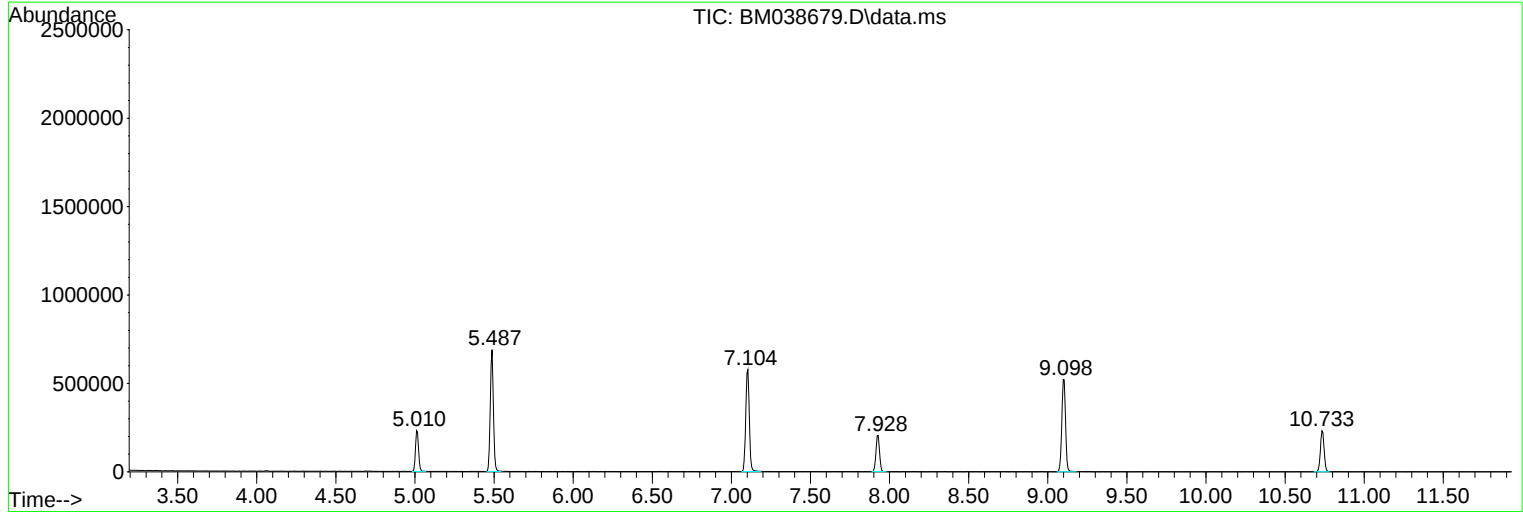

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020323\
Data File : BM038679.D
Acq On : 03 Feb 2023 14:06
Operator : CG/JU
Sample : PB150629BL
Misc :
ALS Vial : 3 Sample Multiplier: 1










Instrument :
BNA_M
ClientSampleId :
PB150629BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM020123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.	
5.010	19.26 ng	310135	1,4-Dichlorobenzene-d4	7.928	
Hit# of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	72
2	2,3-Butanedione, monooxime	101	C4H7NO2	000057-71-6	25
3	Acetic acid, cyano-, 1,1-dimethy...	141	C7H11NO2	001116-98-9	25
4	1-Propen-2-ol, acetate	100	C5H8O2	000108-22-5	10
5	Morpholine, 4-methyl-	101	C5H11NO	000109-02-4	9

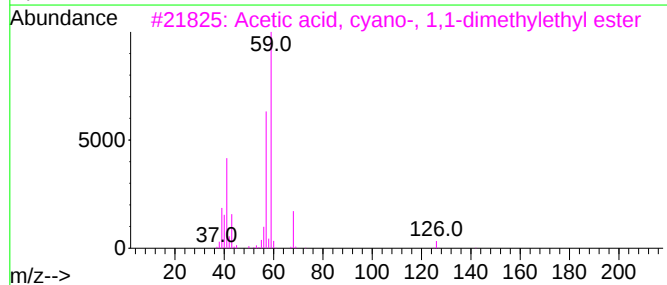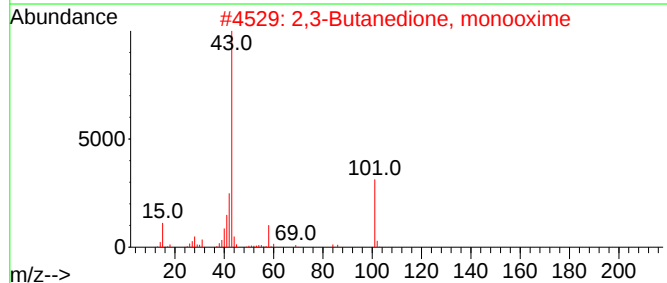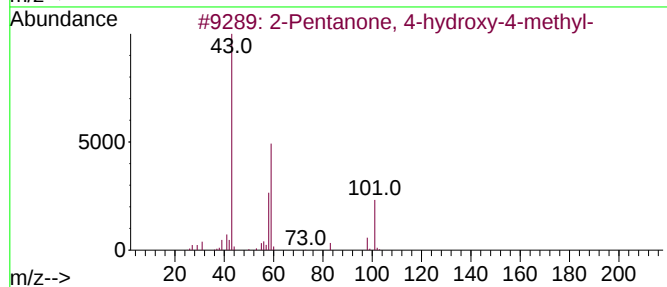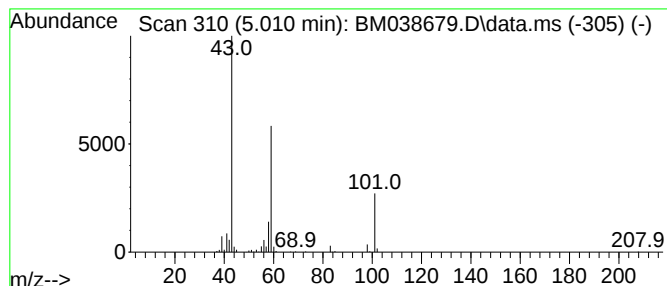

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020323\
Data File : BM038679.D
Acq On : 03 Feb 2023 14:06
Operator : CG/JU
Sample : PB150629BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB150629BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM020123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	5.010	19.3	ng	310135	1	7.928	322119	20.0