


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020323\
Data File : BM038677.D
Acq On : 03 Feb 2023 12:36
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM020123.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Sat Feb 04 05:17:53 2023

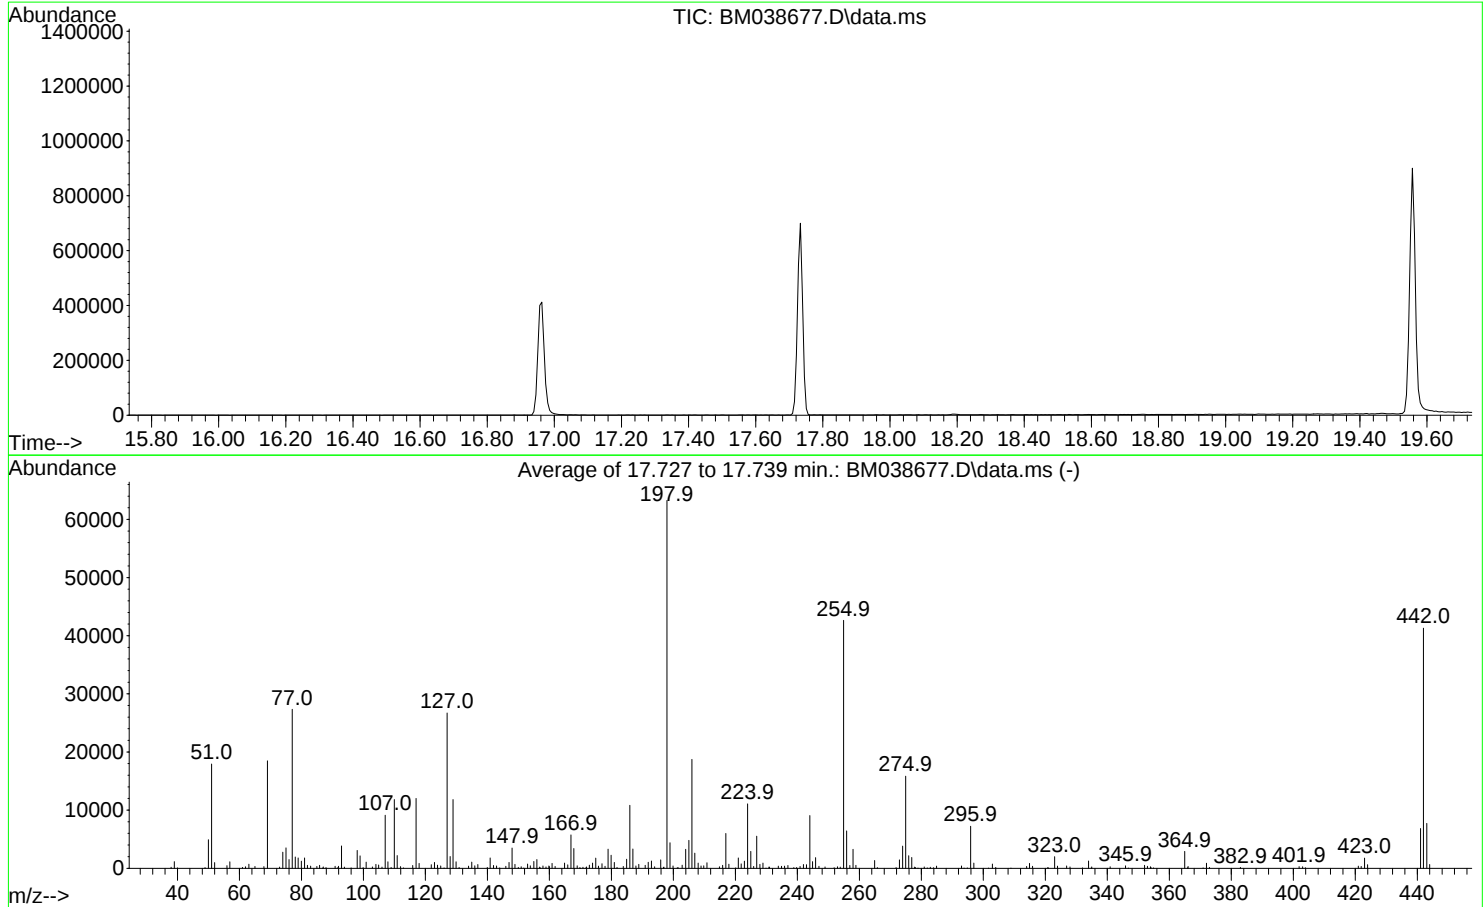




AutoFind: Scans 2472, 2473, 2474; Background Corrected with Scan 2466

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.3	17916	PASS
68	69	0.00	2	1.6	291	PASS
69	198	0.00	100	29.2	18485	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	42.2	26717	PASS
197	198	0.00	2	0.3	206	PASS
198	198	100	100	100.0	63267	PASS
199	198	5	9	6.9	4382	PASS
275	198	10	60	25.0	15830	PASS
365	198	1	100	4.6	2918	PASS
441	198	0.01	100	10.8	6843	PASS
442	442	50	100	100.0	41304	PASS
443	442	15	24	18.7	7728	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020323\
Data File : BM038677.D
Acq On : 03 Feb 2023 12:36
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Feb 04 04:21:23 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM020123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 02 03:31:45 2023
Response via : Initial Calibration

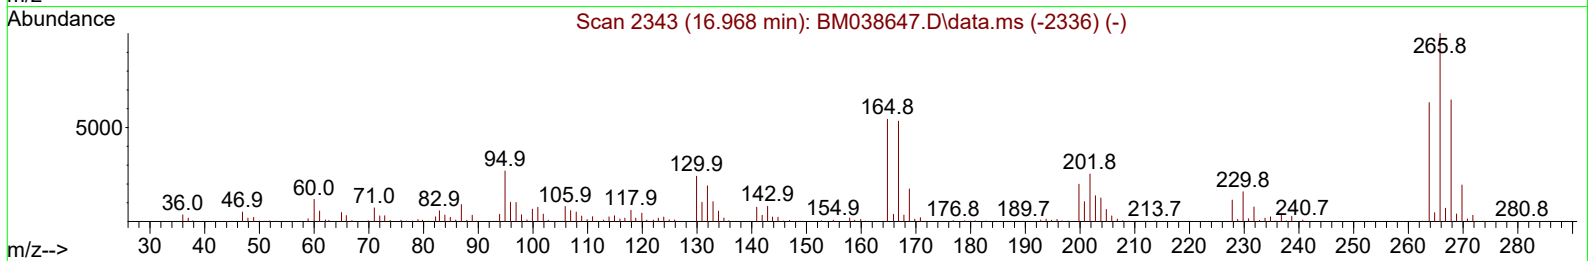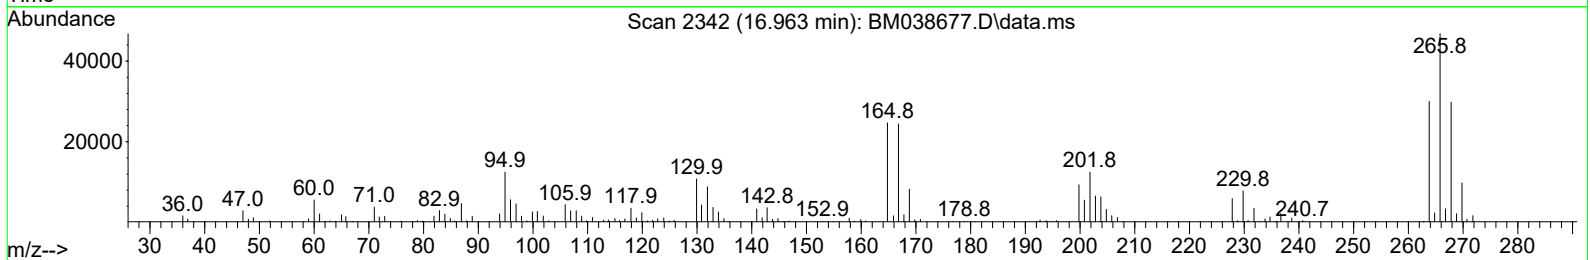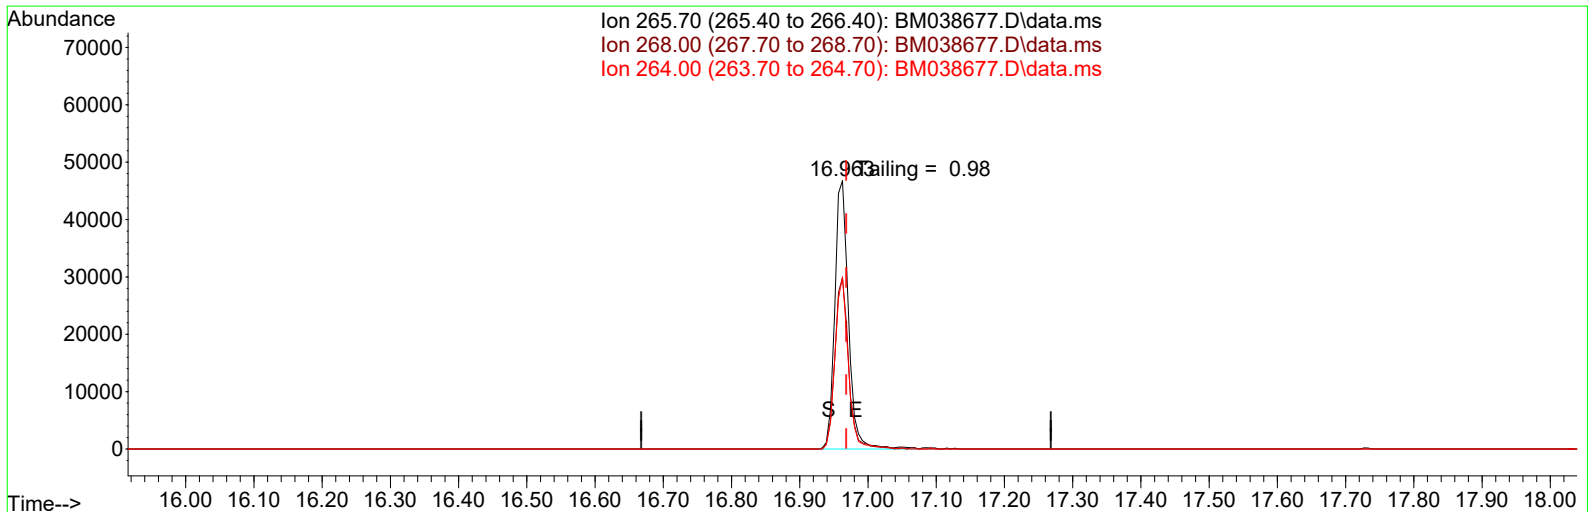

TIC: BM038677.D\data.ms

(70) Pentachlorophenol (C)

16.963min (-0.005) 0.00 ng




response 64777

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.70	63.78
264.00	63.30	64.18
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020323\
Data File : BM038677.D
Acq On : 03 Feb 2023 12:36
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Feb 04 04:21:23 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM020123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 02 03:31:45 2023
Response via : Initial Calibration

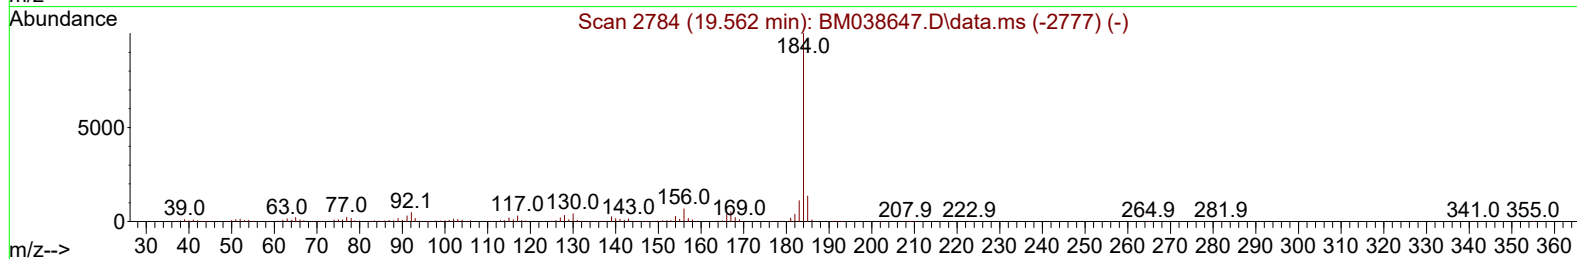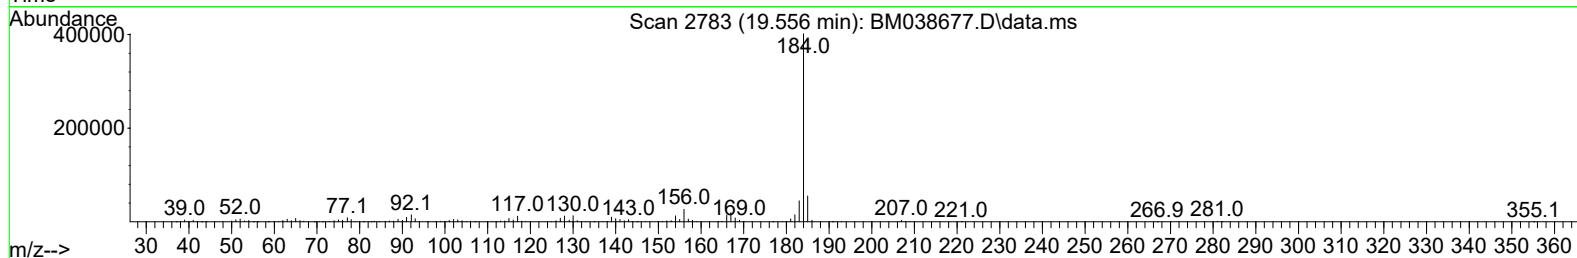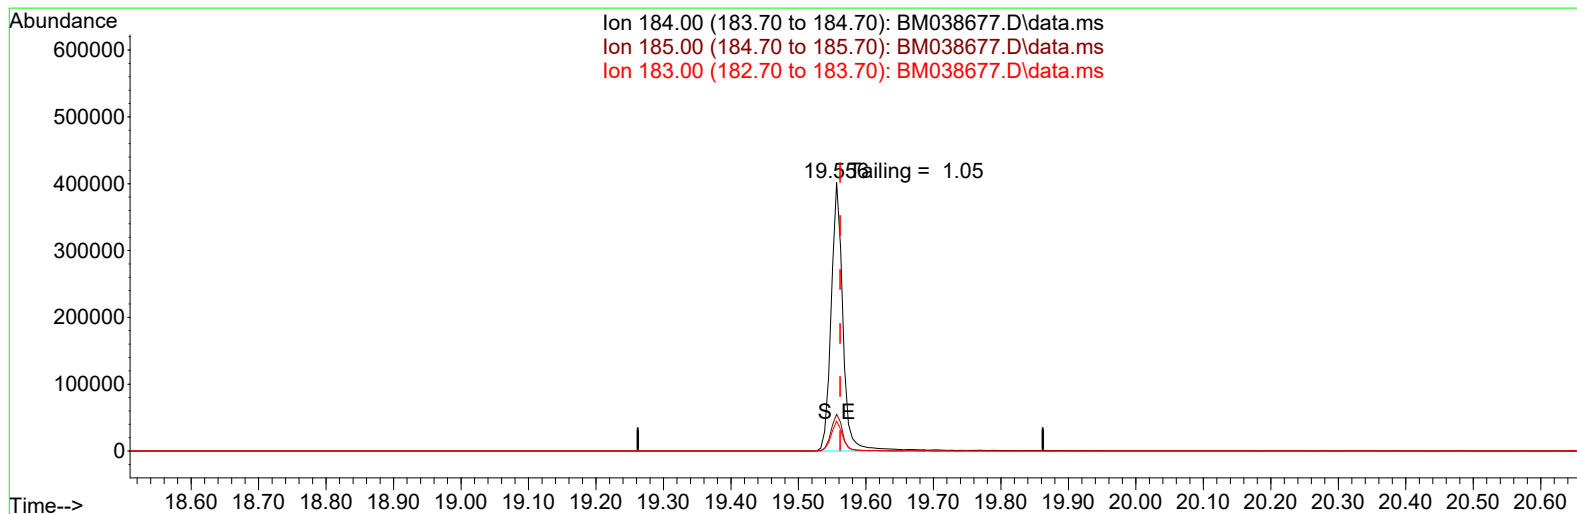

TIC: BM038677.D\data.ms

(77) Benzidine

19.556min (-0.006) 0.00 ng

response 484405

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.50	13.72
183.00	11.00	11.16
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/3/2023	BNA_M	<u>BM038677.D</u>
Compound Name	Response	Retention Time
DDT	237774	20.774
DDD	2486	20.386
DDE	0	19.868
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
2486	240260	1.03

Instrument :
BNA_M
ClientSampleId :
DFTPP