

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM020620\
 Data File : BM024784.D
 Acq On : 08 Feb 2020 05:29
 Operator : CG/JU
 Sample : L1400-04
 Misc :
 ALS Vial : 63 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Feb 10 00:10:42 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM020620MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Feb 07 07:38:13 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.40	152	306444	20.00	ng/ul	0.00
18) Naphthalene-d8	10.16	136	1195392	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.06	164	797857	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.81	188	1745854	20.00	ng/ul	0.00
78) Chrysene-d12	21.02	240	1763230	20.00	ng/ul	-0.01
86) Perylene-d12	23.13	264	1826597	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.02	96	25106	3.94	ng/uL	0.00
5) Phenol-d5	6.60	99	371434	18.25	ng/ul	-0.01
7) Bis-(2-Chloroethyl)ether-d	6.76	67	253934	22.09	ng/ul	0.00
9) 2-Chlorophenol-d4	6.95	132	349783	19.18	ng/ul	0.00
13) 4-Methylphenol-d8	8.12	113	326489	19.01	ng/ul	-0.01
19) Nitrobenzene-d5	8.54	128	187456	21.69	ng/ul	-0.01
22) 2-Nitrophenol-d4	9.26	143	214625	21.01	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.79	165	371392	18.03	ng/ul	-0.01
29) 4-Chloroaniline-d4	10.30	131	464378	24.09	ng/ul	0.00
44) Dimethylphthalate-d6	13.48	166	1384418	22.99	ng/ul	0.00
47) Acenaphthylene-d8	13.75	160	1388136	19.74	ng/ul	0.00
52) 4-Nitrophenol-d4	14.28	143	168124	17.18	ng/ul	0.00
58) Fluorene-d10	15.06	176	1099627	20.62	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.19	200	197991	17.40	ng/ul	0.00
71) Anthracene-d10	16.91	188	1593337	19.99	ng/ul	0.00
79) Pyrene-d10	19.22	212	1704979	19.33	ng/ul	0.00
90) Benzo(a)pyrene-d12	22.99	264	1728464	18.84	ng/ul	-0.01

Target Compounds


					Ovalue	
70) Phenanthrene	16.85	178	203881	2.142	ng/ul	99
77) Fluoranthene	18.88	202	311414	2.665	ng/ul	99
80) Pyrene	19.24	202	247540	2.121	ng/ul	98
83) Benzo(a)anthracene	21.01	228	158094	1.331	ng/ul	97
85) Chrysene	21.06	228	154873	1.324	ng/ul	99
88) Benzo(b)fluoranthene	22.51	252	195191	1.681	ng/ul#	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM020620\
Data File : BM024784.D
Acq On : 08 Feb 2020 05:29
Operator : CG/JU
Sample : L1400-04
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Feb 10 00:10:42 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM020620MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Feb 07 07:38:13 2020
Response via : Initial Calibration

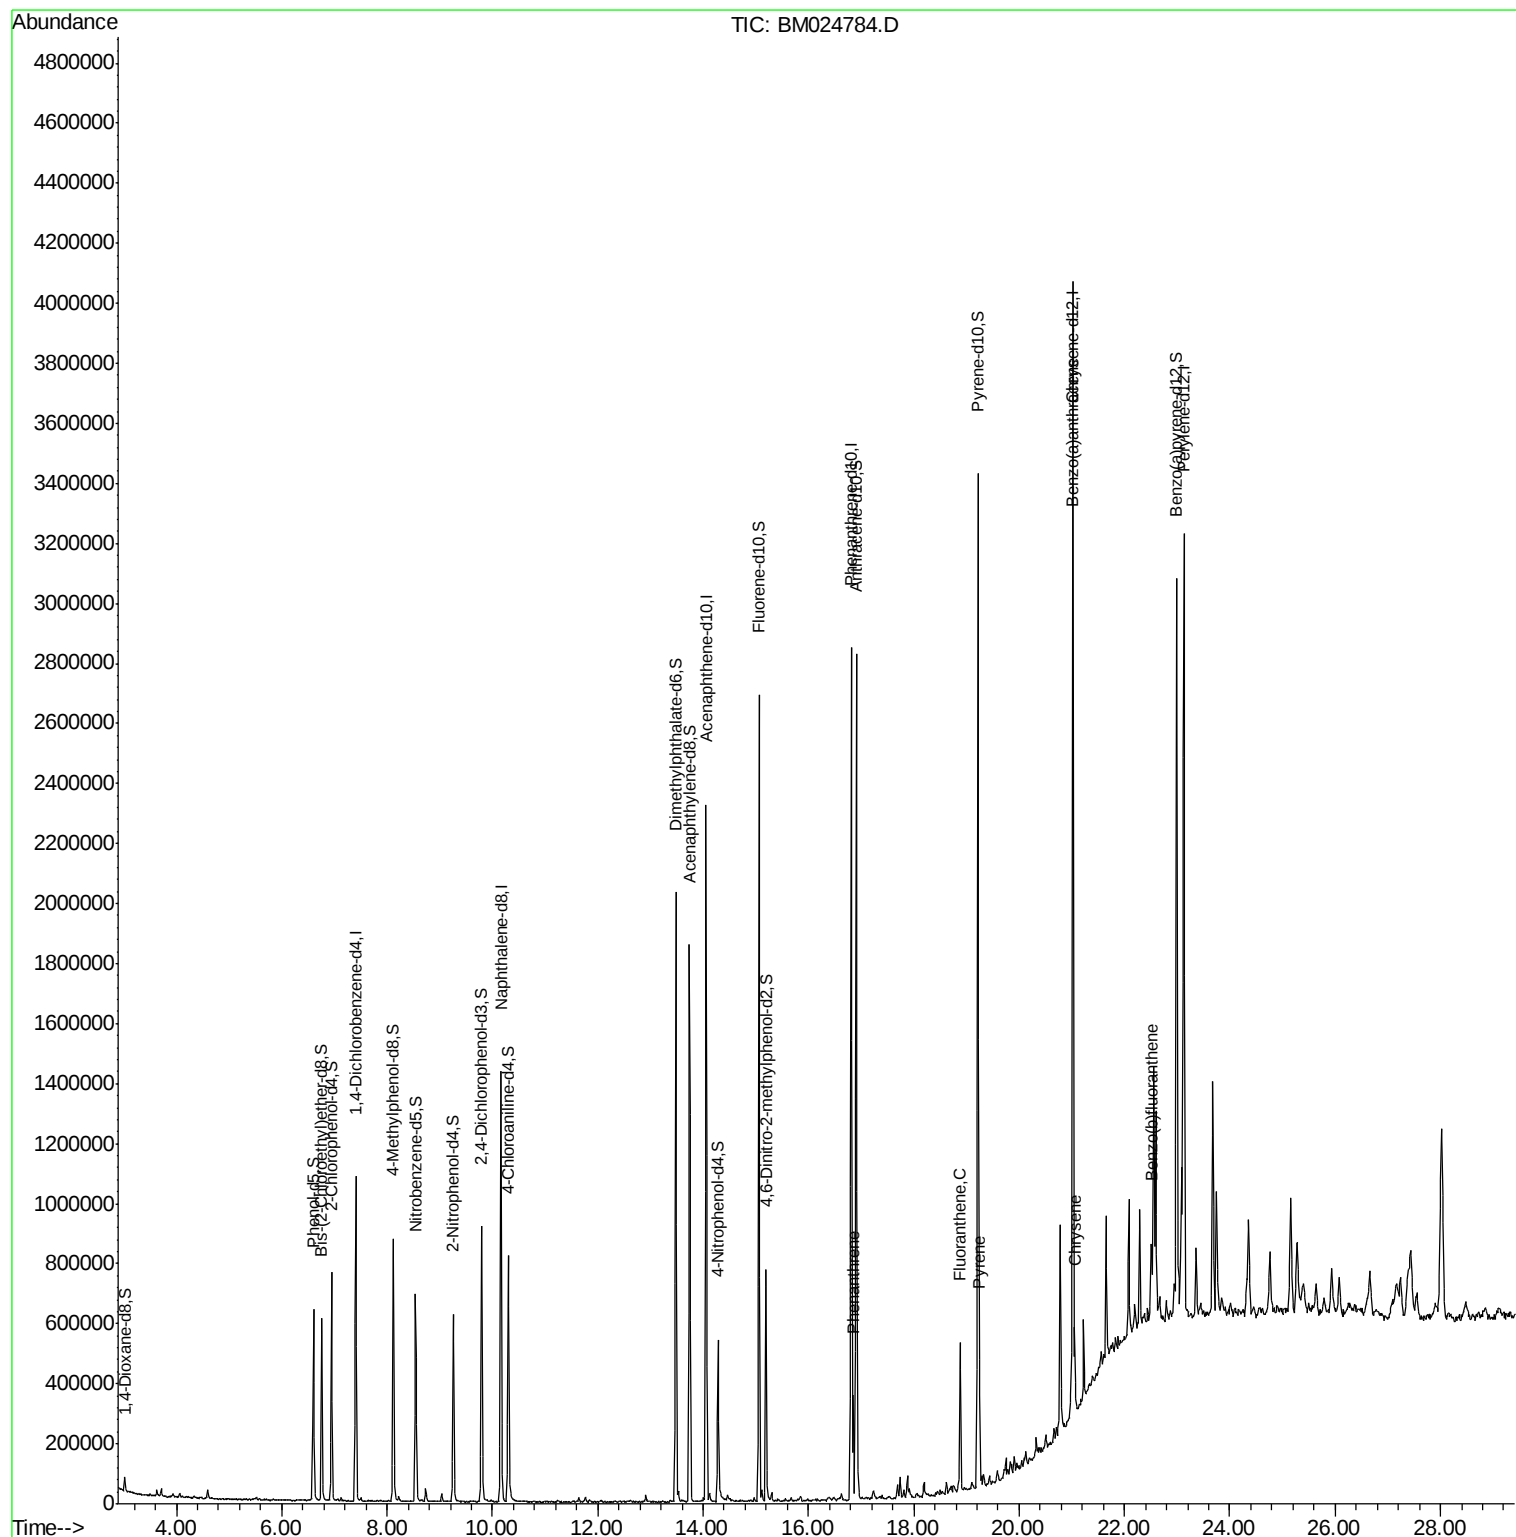

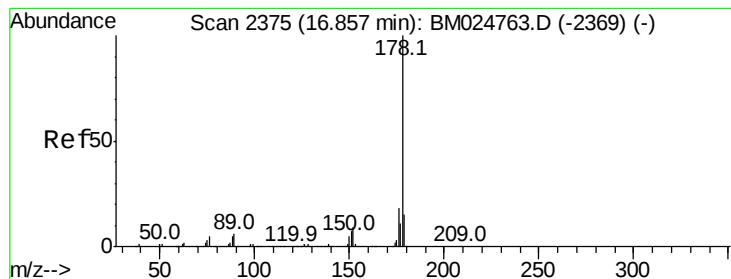

#70

Phenanthrene

Concen: 2.142 ng/ul

RT: 16.85 min Scan# 2374

Delta R.T. -0.01 min

Lab File: BM024784.D

Acq: 08 Feb 2020 05:29


Instrument :

BNA_M

ClientSampleId :

Tot Ion:178 Resp: 203881

Ion	Ratio	Lower	Upper
178	100		
179	15.9	12.2	18.2
176	18.3	14.5	21.7

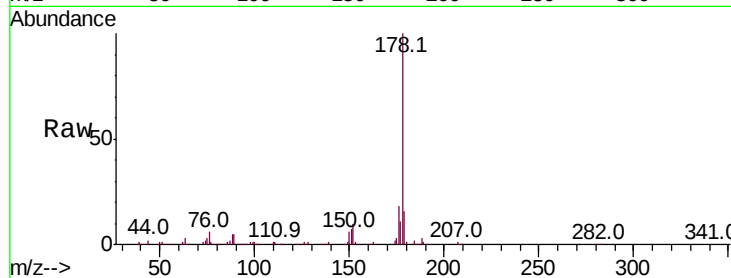


Abundance



Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

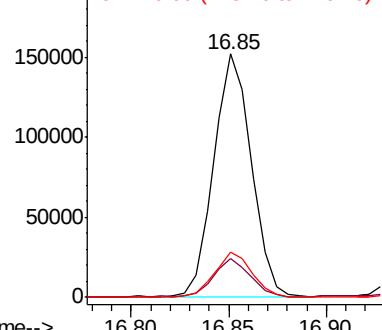

Time-->

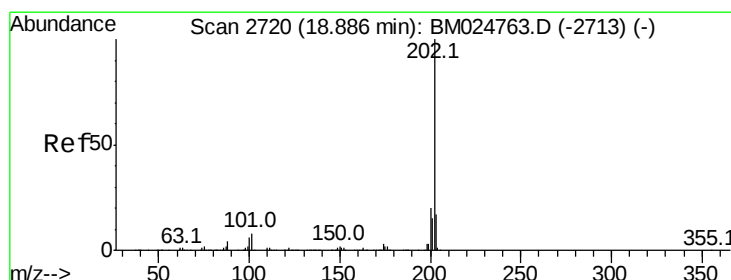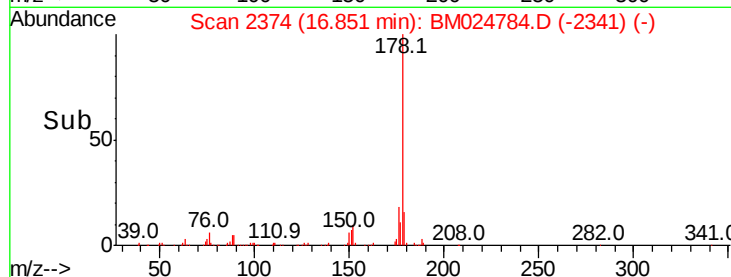

#77

Fluoranthene

Concen: 2.665 ng/ul

RT: 18.88 min Scan# 2719


Delta R.T. -0.01 min

Lab File: BM024784.D

Acq: 08 Feb 2020 05:29

Tgt Ion:202 Resp: 311414

Ion	Ratio	Lower	Upper
202	100		
101	7.9	6.1	9.1
100	5.9	4.8	7.2

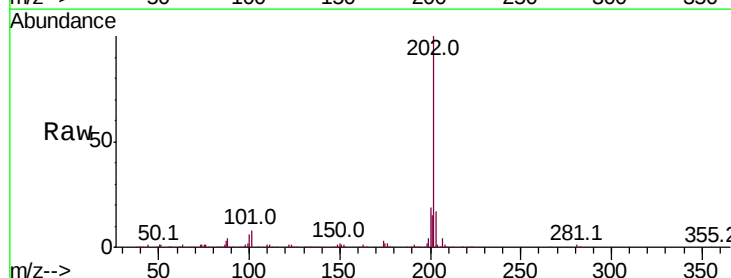


Abundance


Ion 202.00 (201.70 to 202.70): E


Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): E

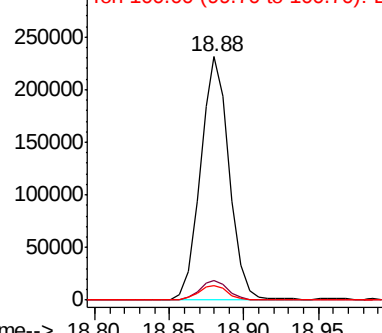

Time-->

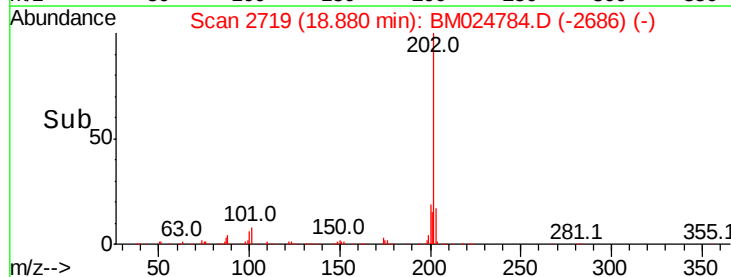


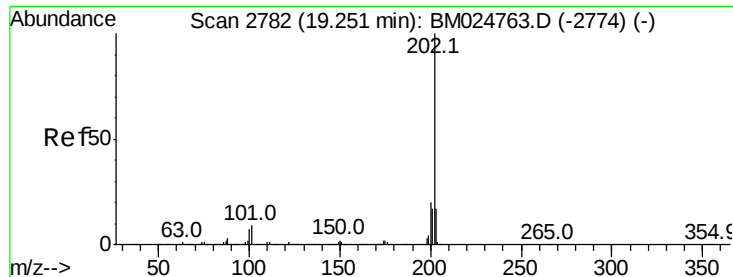




#80
Pvrene
Concen: 2.121 ng/ul
RT: 19.24 min Scan# 2781
Delta R.T. -0.01 min
Lab File: BM024784.D
Acq: 08 Feb 2020 05:29

Instrument :
BNA_M
ClientSampleId :

Tot Ion:	202	Resp:	247540
Ion	Ratio	Lower	Upper
202	100		
101	9.2	7.0	10.4
100	8.1	5.8	8.8

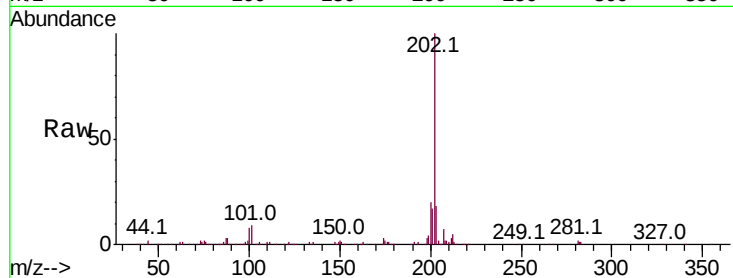


Abundance Ion 202.00 (201.70 to 202.70): E
Ion 101.00 (100.70 to 101.70): E
Ion 100.00 (99.70 to 100.70): B

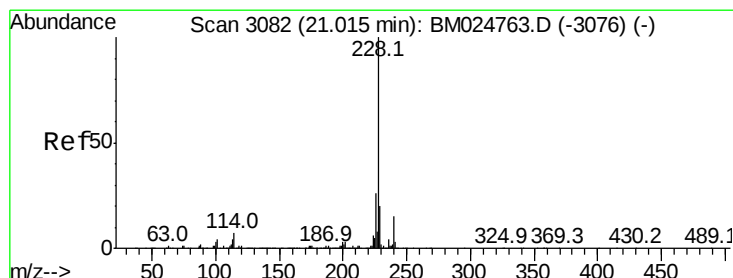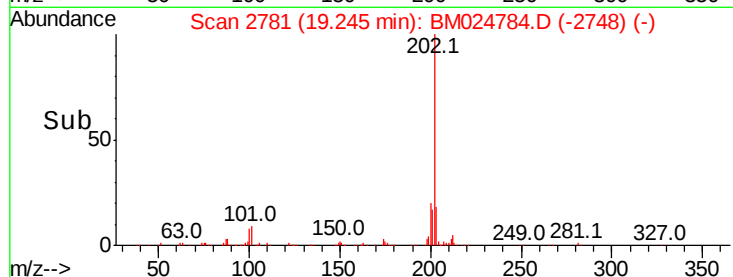
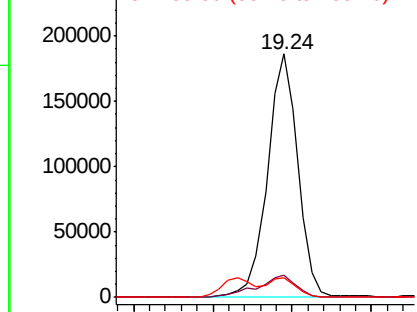



#83
Benzo(a)anthracene
Concen: 1.331 ng/ul
RT: 21.01 min Scan# 3081
Delta R.T. -0.01 min
Lab File: BM024784.D
Acq: 08 Feb 2020 05:29

Tgt Ion:	228	Resp:	158094
Ion	Ratio	Lower	Upper
228	100		
229	20.0	15.9	23.9
226	28.6	20.8	31.2

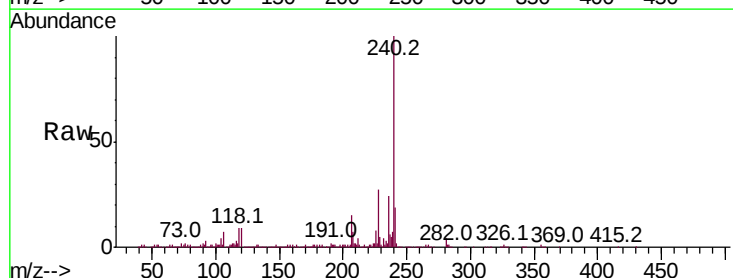

Abundance Ion 228.00 (227.70 to 228.70): E
Ion 229.00 (228.70 to 229.70): E
Ion 226.00 (225.70 to 226.70): E

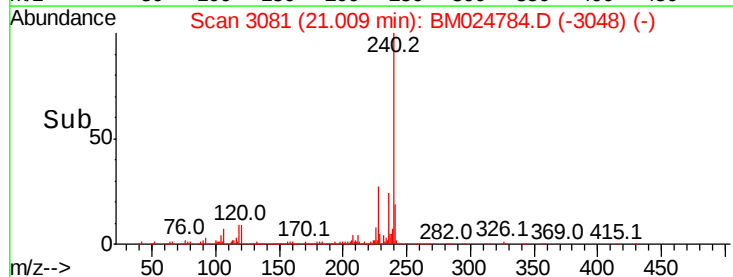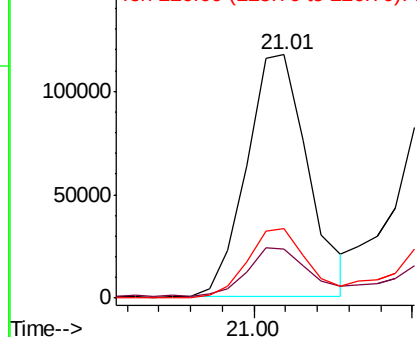

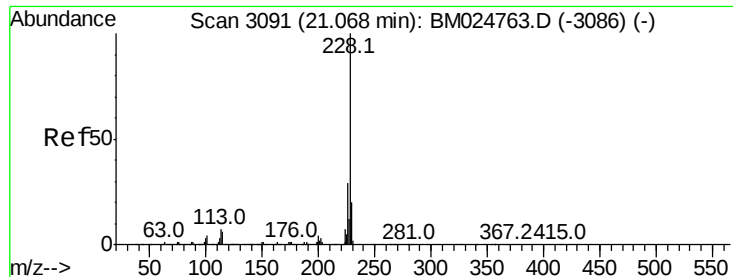

#85

Chrysene

Concen: 1.324 ng/ul

RT: 21.06 min Scan# 3089

Delta R.T. -0.01 min

Lab File: BM024784.D

Acq: 08 Feb 2020 05:29

Instrument :

BNA_M

ClientSampleId :


Tot Ion:228 Resp: 154873

Ion	Ratio	Lower	Upper
228	100		
226	29.1	23.0	34.4
229	19.4	15.8	23.8

228 100

226 29.1 23.0 34.4

229 19.4 15.8 23.8



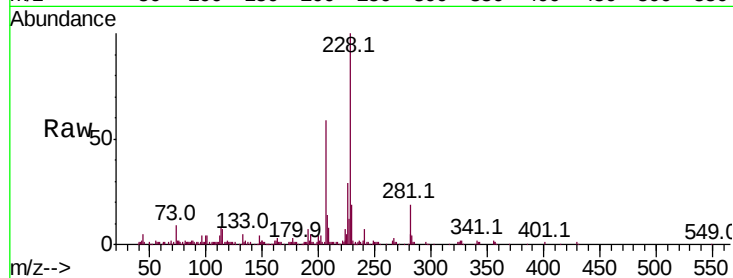


Abundance

Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

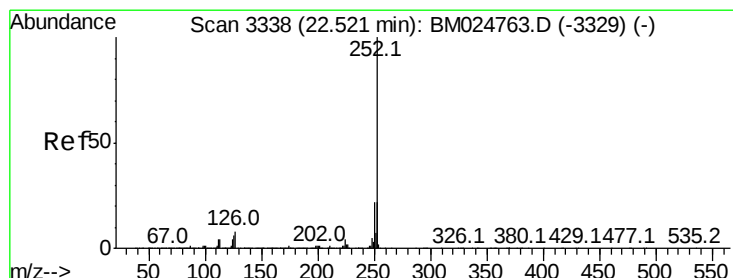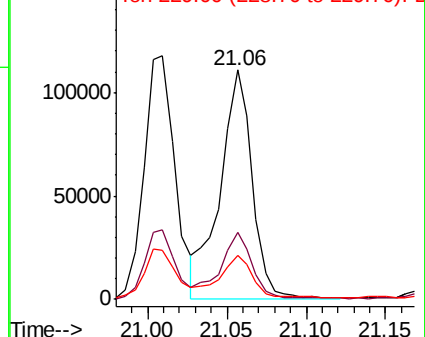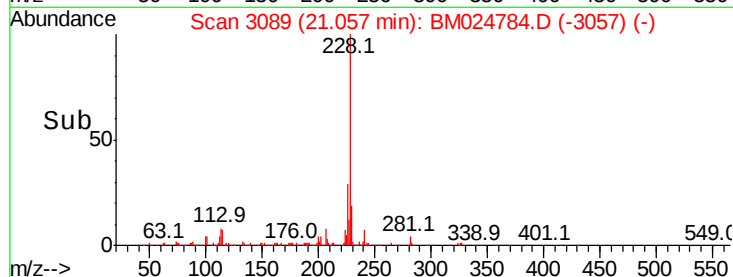

#88

Benzo(b)fluoranthene

Concen: 1.681 ng/ul

RT: 22.51 min Scan# 3336

Delta R.T. -0.01 min

Lab File: BM024784.D

Acq: 08 Feb 2020 05:29


Tgt Ion:252 Resp: 195191

Ion	Ratio	Lower	Upper
252	100		
253	21.5	17.3	25.9
125	8.5	5.1	7.7#

252 100

253 21.5 17.3 25.9

125 8.5 5.1 7.7#

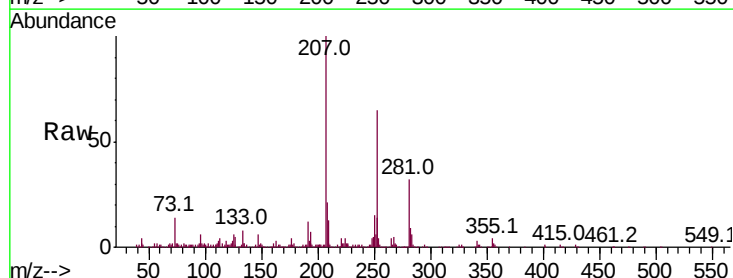

Abundance

Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

