

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM020620\
Data File : BM024787.D
Acq On : 08 Feb 2020 07:16
Operator : CG/JU
Sample : L1400-07
Misc :
ALS Vial : 66 Sample Multiplier: 1


Quant Time: Feb 15 06:07:38 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM020620MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Feb 07 07:38:13 2020
Response via : Initial Calibration

Instrument :

BNA_M

Client Sample Id :

CB6H3

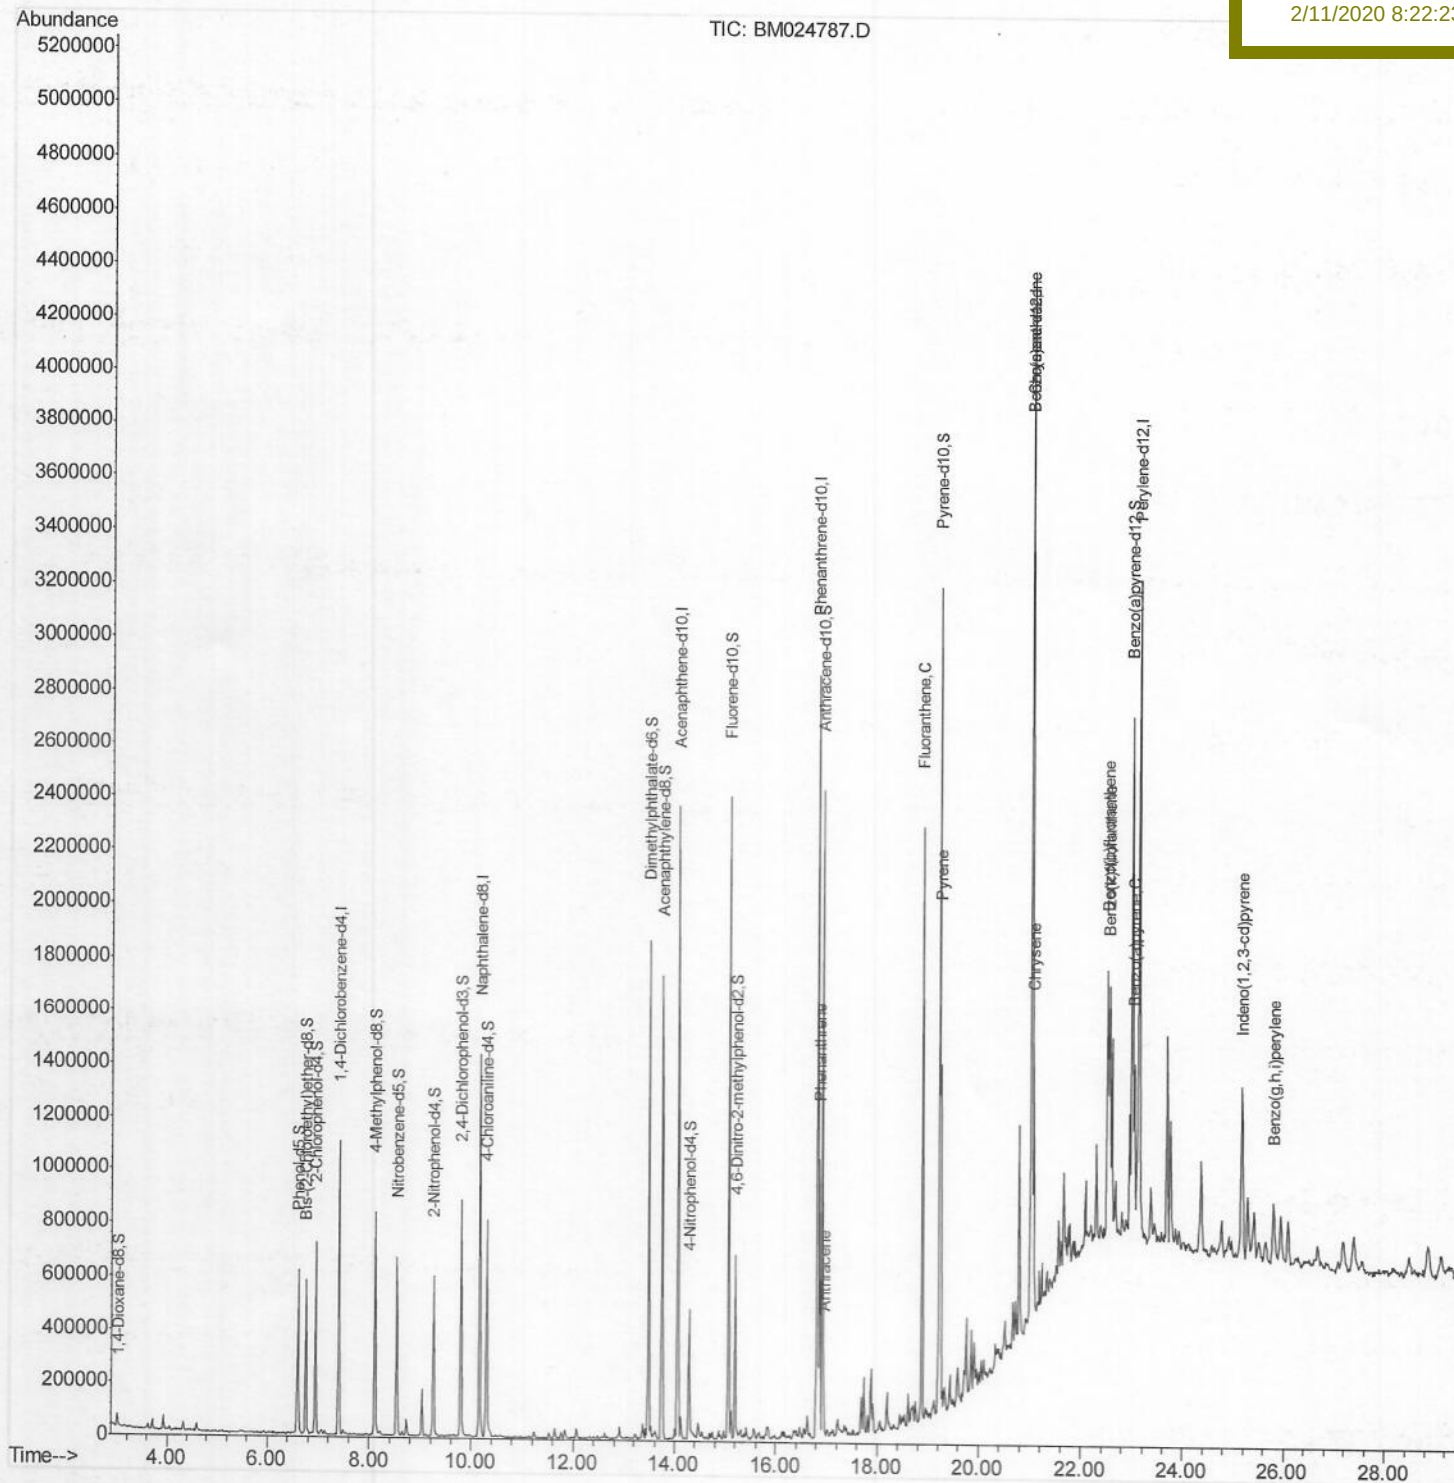Manual Integrations
APPROVEDmohammad
2/11/2020 8:22:23 AM

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM020620\
 Data File : BM024787.D
 Acq On : 08 Feb 2020 07:16
 Operator : CG/JU
 Sample : L1400-07
 Misc :
 ALS Vial : 66 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 CB6H3

Manual Integrations
 APPROVED

mohammad
 2/11/2020 8:22:23 AM

Quant Time: Feb 10 00:11:06 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM020620MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Feb 07 07:38:13 2020
 Response via : Initial Calibration

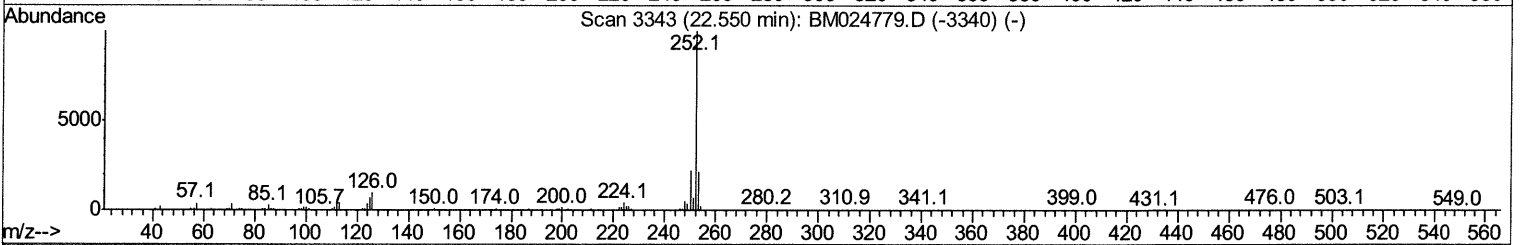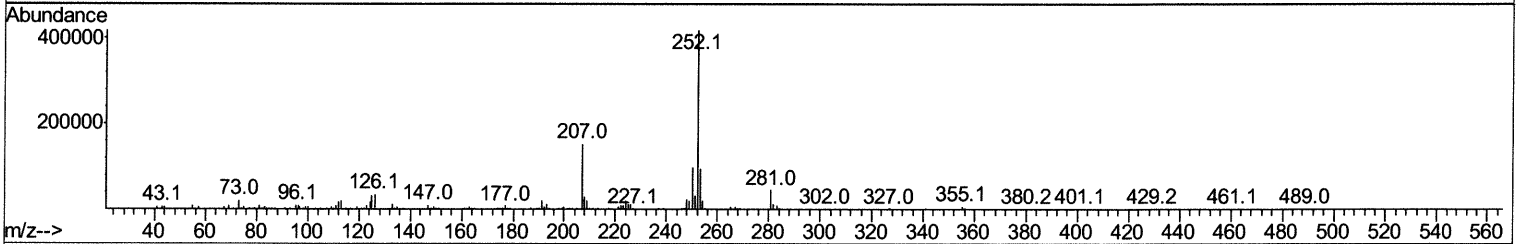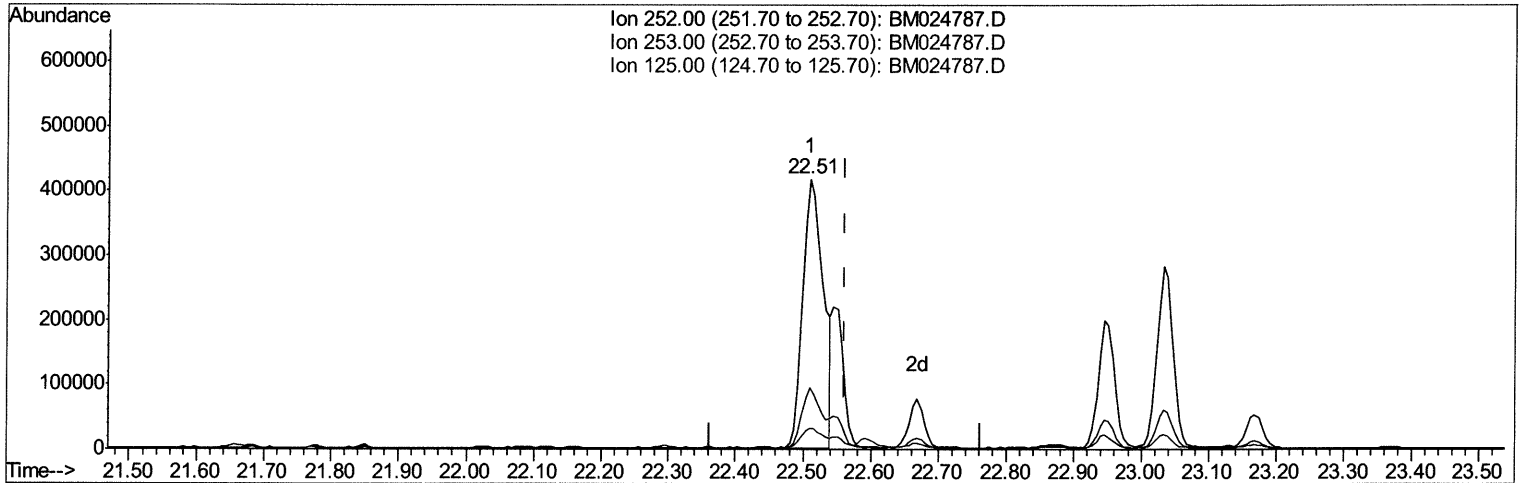

TIC: BM024787.D

(89) Benzo(k)fluoranthene
 22.509min (-0.052) 8.24ng/ul
 response 883207

Ion	Exp%	Act%
252.00	100	100
253.00	21.70	22.63
125.00	6.40	7.85#
0.00	0.00	0.00




Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM020620\
 Data File : BM024787.D
 Acq On : 08 Feb 2020 07:16
 Operator : CG/JU
 Sample : L1400-07
 Misc :
 ALS Vial : 66 Sample Multiplier: 1

Quant Time: Feb 10 00:11:06 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM020620MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Feb 07 07:38:13 2020
 Response via : Initial Calibration

Instrument :
 BNA_M
 ClientSampleId :
 CB6H3

Manual Integrations
 APPROVED

mohammad
 2/11/2020 8:22:23 AM

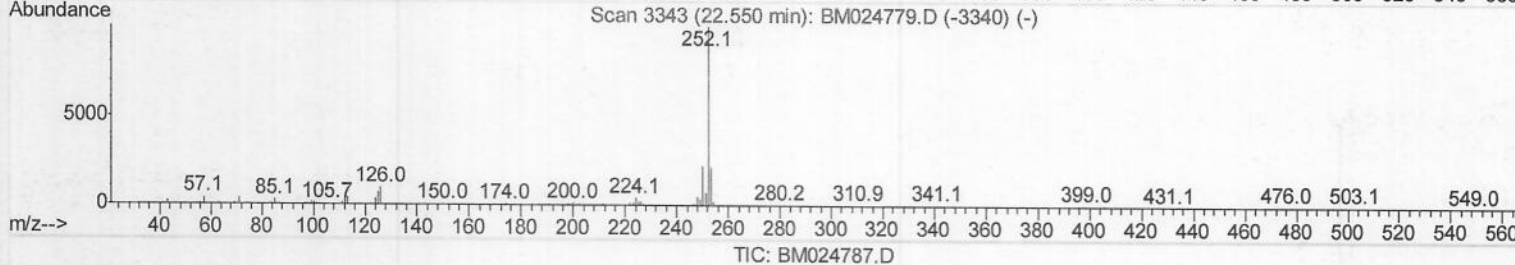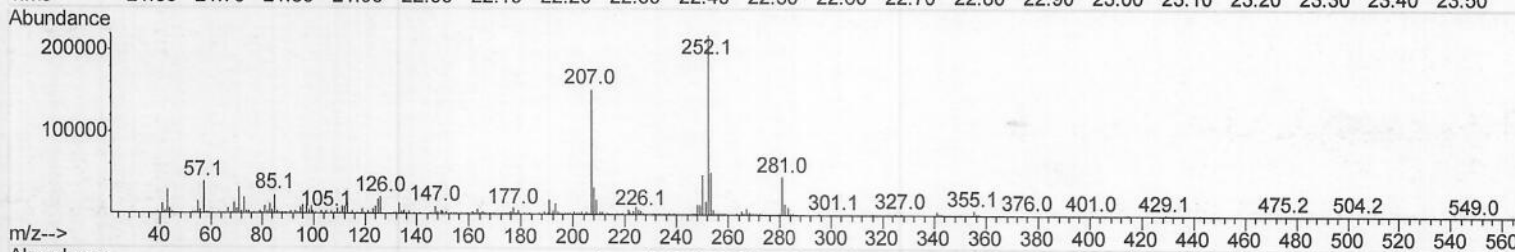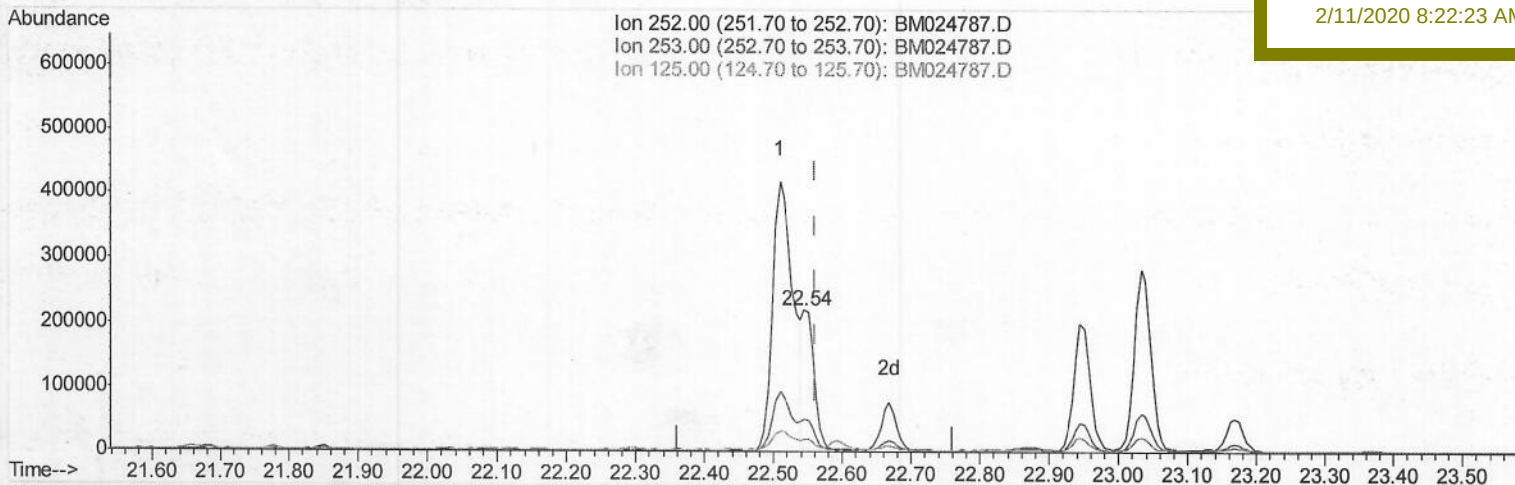

(89) Benzo(k)fluoranthene

22.545min (-0.017) 2.35ng/ul m>JU 02/12/20

response 251813

Ion	Exp%	Act%
252.00	100	100
253.00	21.70	23.22
125.00	6.40	8.36#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM020620\
 Data File : BM024787.D
 Acq On : 08 Feb 2020 07:16
 Operator : CG/JU
 Sample : L1400-07
 Misc :
 ALS Vial : 66 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 CB6H3

Quant Time: Feb 15 06:07:38 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM020620MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Feb 07 07:38:13 2020
 Response via : Initial Calibration

Manual Integrations
 APPROVED

mohammad
 2/11/2020 8:22:23 AM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.40	152	313429	20.00	ng/ul	0.00
18) Naphthalene-d8	10.16	136	1217820	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.06	164	806295	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.81	188	1726945	20.00	ng/ul	0.00
78) Chrysene-d12	21.02	240	1688851	20.00	ng/ul	-0.01
86) Perylene-d12	23.13	264	1750372	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.02	96	21895	3.36	ng/uL	0.00
5) Phenol-d5	6.60	99	352934	16.95	ng/ul	-0.01
7) Bis-(2-Chloroethyl) ether-d	6.76	67	240211	20.43	ng/ul	0.00
9) 2-Chlorophenol-d4	6.95	132	335241	17.97	ng/ul	0.00
13) 4-Methylphenol-d8	8.12	113	311781	17.75	ng/ul	-0.01
19) Nitrobenzene-d5	8.54	128	178122	20.23	ng/ul	-0.01
22) 2-Nitrophenol-d4	9.26	143	208363	20.02	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.79	165	354375	16.88	ng/ul	-0.01
29) 4-Chloroaniline-d4	10.30	131	452485	23.04	ng/ul	0.00
44) Dimethylphthalate-d6	13.48	166	1275157	20.95	ng/ul	0.00
47) Acenaphthylene-d8	13.74	160	1267193	17.83	ng/ul	-0.01
52) 4-Nitrophenol-d4	14.28	143	155004	15.67	ng/ul	0.00
58) Fluorene-d10	15.06	176	1004997	18.65	ng/ul	-0.01
63) 4,6-Dinitro-2-methylphenol	15.19	200	178886	15.89	ng/ul	0.00
71) Anthracene-d10	16.91	188	1407697	17.86	ng/ul	0.00
79) Pyrene-d10	19.22	212	1455248	17.23	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.00	264	1444616	16.43	ng/ul	0.00

Target Compounds

					Ovalue	
70) Phenanthrene	16.85	178	622559	6.612	ng/ul	99
72) Anthracene	16.95	178	136373	1.428	ng/ul	98
77) Fluoranthene	18.88	202	1357788	11.746	ng/ul	99
80) Pyrene	19.24	202	1021238	9.135	ng/ul	100
83) Benzo(a)anthracene	21.01	228	675177	5.935	ng/ul	99
85) Chrysene	21.06	228	607944	5.428	ng/ul	100
88) Benzo(b)fluoranthene	22.51	252	883207	7.935	ng/ul#	97
89) Benzo(k)fluoranthene	22.54	252	251813m>	2.351	ng/ul>ju	02/12/20
91) Benzo(a)pyrene	23.03	252	469252	4.703	ng/ul#	99
92) Indeno(1,2,3-cd)pyrene	25.17	276	369230	2.972	ng/ul	96
94) Benzo(a,h,i)perylene	25.79	276	255914	2.477	ng/ul	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed