

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM020620\
 Data File : BM024775.D
 Acq On : 07 Feb 2020 23:29
 Operator : CG/JU
 Sample : L1399-20
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 CB6X6

Quant Time: Feb 08 00:38:29 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM020620MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Feb 07 22:29:17 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.40	152	293336	20.00	ng/ul	0.00
18) Naphthalene-d8	10.16	136	1151878	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.06	164	785063	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.82	188	1775044	20.00	ng/ul	0.00
78) Chrysene-d12	21.02	240	1830129	20.00	ng/ul	-0.01
86) Perylene-d12	23.13	264	1863432	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.02	96	21279	3.49	ng/uL	0.00
5) Phenol-d5	6.60	99	353444	18.14	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.76	67	221202	20.10	ng/ul	0.00
9) 2-Chlorophenol-d4	6.95	132	324470	18.59	ng/ul	0.00
13) 4-Methylphenol-d8	8.12	113	305809	18.60	ng/ul	-0.01
19) Nitrobenzene-d5	8.55	128	163662	19.65	ng/ul	0.00
22) 2-Nitrophenol-d4	9.26	143	195749	19.89	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.80	165	340631	17.16	ng/ul	0.00
29) 4-Chloroaniline-d4	10.30	131	435785	23.46	ng/ul	0.00
44) Dimethylphthalate-d6	13.48	166	1251344	21.12	ng/ul	0.00
47) Acenaphthylene-d8	13.75	160	1300230	18.79	ng/ul	0.00
52) 4-Nitrophenol-d4	14.28	143	177770	18.46	ng/ul	0.00
58) Fluorene-d10	15.06	176	1012152	19.29	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.19	200	204280	17.66	ng/ul	0.00
71) Anthracene-d10	16.91	188	1636009	20.19	ng/ul	0.00
79) Pyrene-d10	19.22	212	1971019	21.53	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.00	264	2014454	21.52	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	13.53	163	87304	1.412	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM020620\
Data File : BM024775.D
Acq On : 07 Feb 2020 23:29
Operator : CG/JU
Sample : L1399-20
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
CB6X6

Quant Time: Feb 08 00:38:29 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM020620MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Feb 07 22:29:17 2020
Response via : Initial Calibration

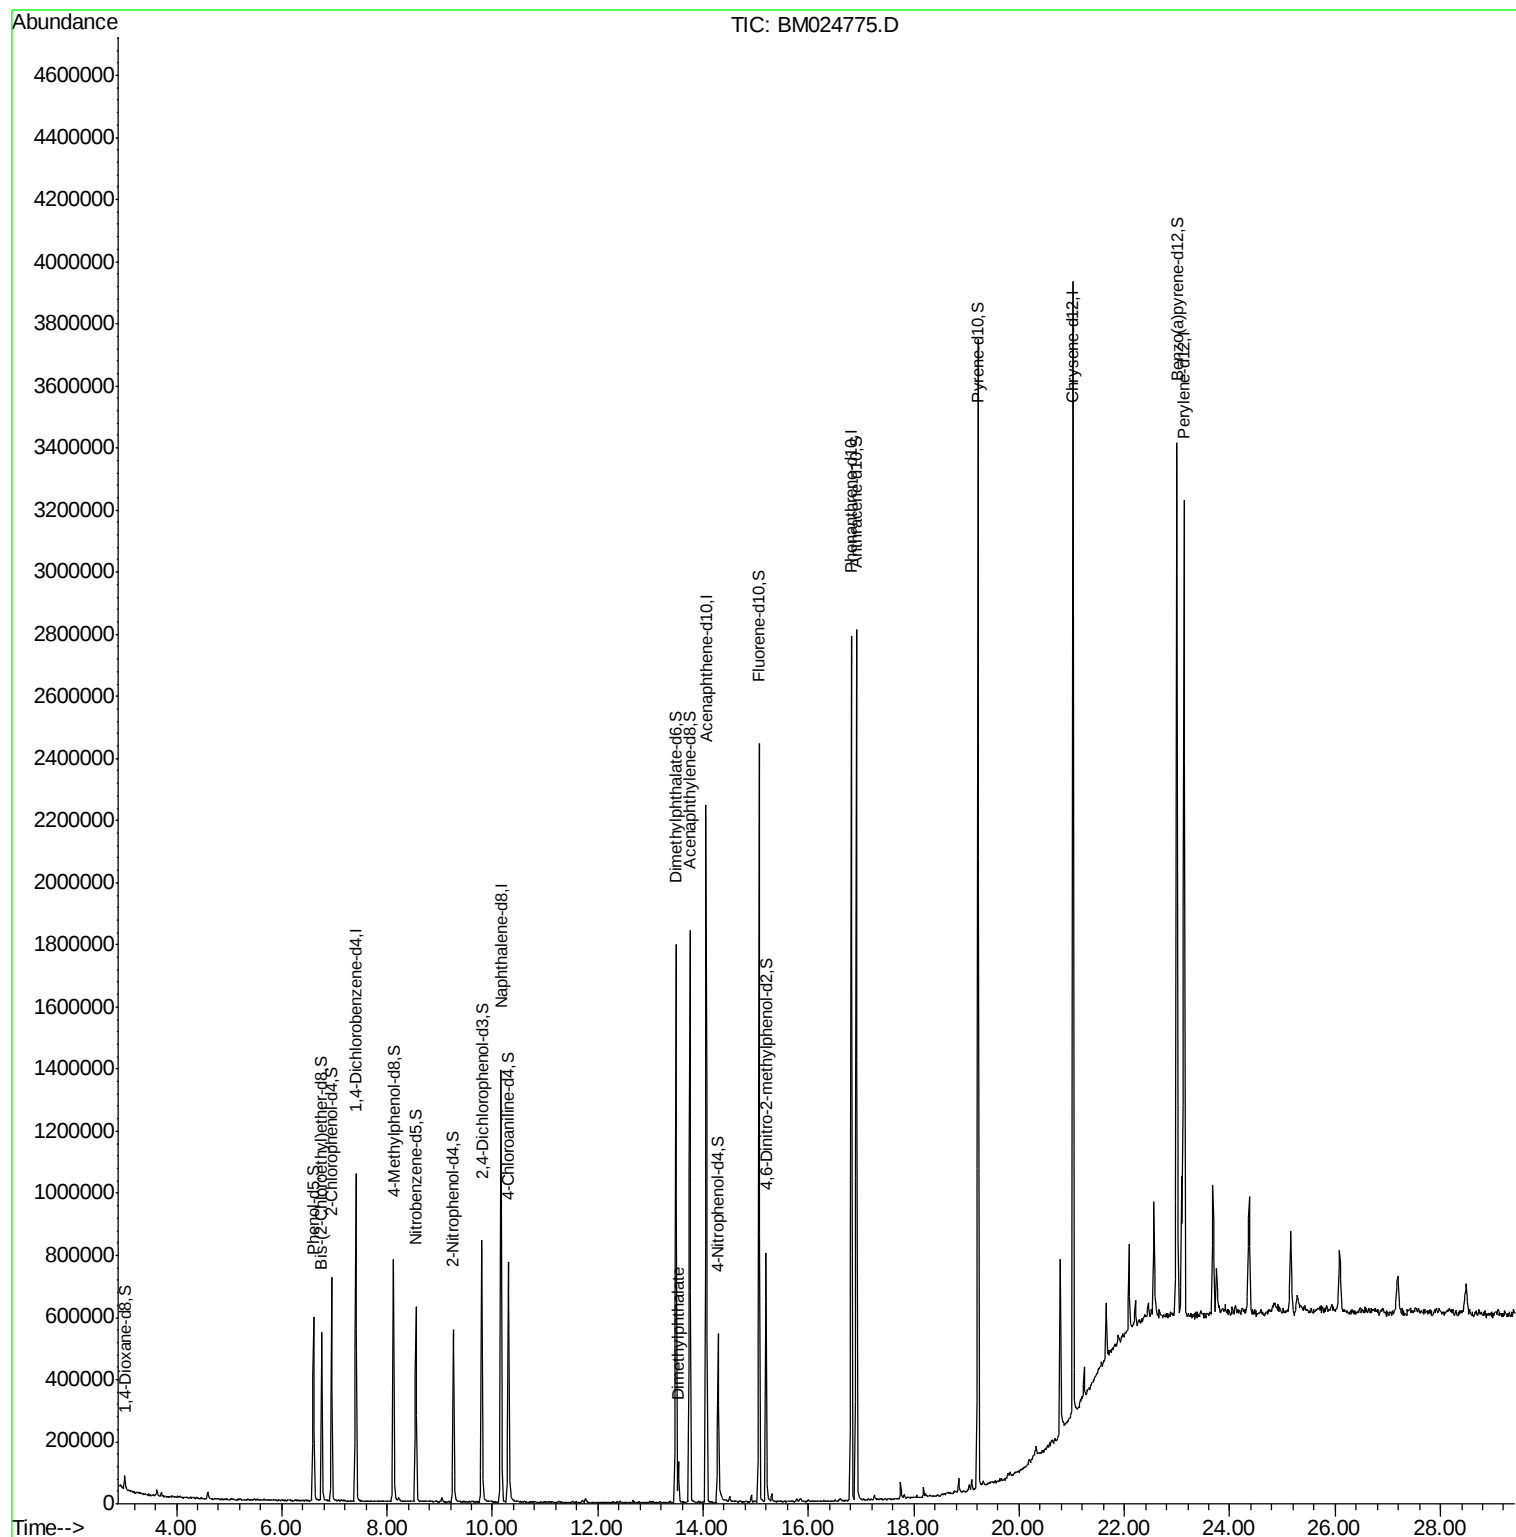

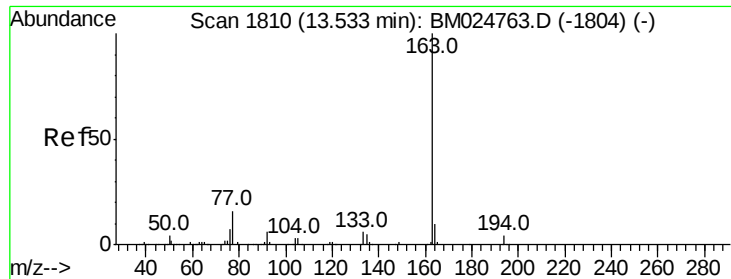

#45

Dimethylphthalate

Concen: 1.412 ng/ul

RT: 13.53 min Scan# 1809

Delta R.T. -0.01 min

Lab File: BM024775.D

Acq: 07 Feb 2020 23:29

Instrument :

BNA_M

ClientSampleId :

CB6X6



Tot Ion:163 Resp: 87304

Ion Ratio Lower Upper

163 100

194 4.4 3.5 5.3

164 10.8 8.2 12.2

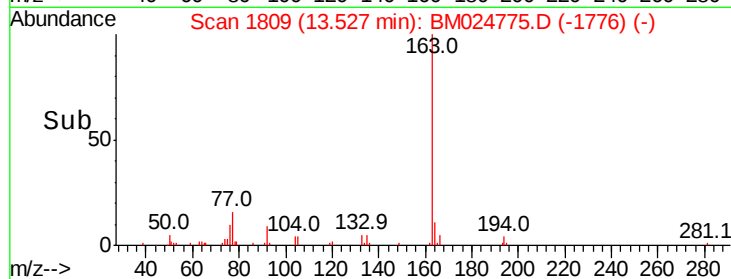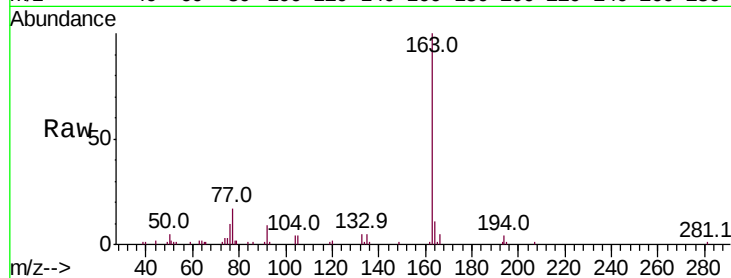

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

