

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM020620\
 Data File : BM024787.D
 Acq On : 08 Feb 2020 07:16
 Operator : CG/JU
 Sample : L1400-07
 Misc :
 ALS Vial : 66 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 CB6H3

Manual Integrations
 APPROVED

mohammad
 2/11/2020 8:22:23 AM

Quant Time: Feb 15 06:07:38 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM020620MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Feb 07 07:38:13 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.40	152	313429	20.00	ng/ul	0.00
18) Naphthalene-d8	10.16	136	1217820	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.06	164	806295	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.81	188	1726945	20.00	ng/ul	0.00
78) Chrysene-d12	21.02	240	1688851	20.00	ng/ul	-0.01
86) Perylene-d12	23.13	264	1750372	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.02	96	21895	3.36	ng/uL	0.00
5) Phenol-d5	6.60	99	352934	16.95	ng/ul	-0.01
7) Bis-(2-Chloroethyl)ether-d	6.76	67	240211	20.43	ng/ul	0.00
9) 2-Chlorophenol-d4	6.95	132	335241	17.97	ng/ul	0.00
13) 4-Methylphenol-d8	8.12	113	311781	17.75	ng/ul	-0.01
19) Nitrobenzene-d5	8.54	128	178122	20.23	ng/ul	-0.01
22) 2-Nitrophenol-d4	9.26	143	208363	20.02	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.79	165	354375	16.88	ng/ul	-0.01
29) 4-Chloroaniline-d4	10.30	131	452485	23.04	ng/ul	0.00
44) Dimethylphthalate-d6	13.48	166	1275157	20.95	ng/ul	0.00
47) Acenaphthylene-d8	13.74	160	1267193	17.83	ng/ul	-0.01
52) 4-Nitrophenol-d4	14.28	143	155004	15.67	ng/ul	0.00
58) Fluorene-d10	15.06	176	1004997	18.65	ng/ul	-0.01
63) 4,6-Dinitro-2-methylphenol	15.19	200	178886	15.89	ng/ul	0.00
71) Anthracene-d10	16.91	188	1407697	17.86	ng/ul	0.00
79) Pyrene-d10	19.22	212	1455248	17.23	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.00	264	1444616	16.43	ng/ul	0.00

Target Compounds

					Ovalue	
70) Phenanthrene	16.85	178	622559	6.612	ng/ul	99
72) Anthracene	16.95	178	136373	1.428	ng/ul	98
77) Fluoranthene	18.88	202	1357788	11.746	ng/ul	99
80) Pyrene	19.24	202	1021238	9.135	ng/ul	100
83) Benzo(a)anthracene	21.01	228	675177	5.935	ng/ul	99
85) Chrysene	21.06	228	607944	5.428	ng/ul	100
88) Benzo(b)fluoranthene	22.51	252	883207	7.935	ng/ul#	97
89) Benzo(k)fluoranthene	22.54	252	251813m	2.351	ng/ul	
91) Benzo(a)pyrene	23.03	252	469252	4.703	ng/ul#	99
92) Indeno(1,2,3-cd)pyrene	25.17	276	369230	2.972	ng/ul	96
94) Benzo(g,h,i)perylene	25.79	276	255914	2.477	ng/ul	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM020620\
Data File : BM024787.D
Acq On : 08 Feb 2020 07:16
Operator : CG/JU
Sample : L1400-07
Misc :
ALS Vial : 66 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
CB6H3

Quant Time: Feb 15 06:07:38 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM020620MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Feb 07 07:38:13 2020
Response via : Initial Calibration

Manual Integrations
APPROVED

mohammad
2/11/2020 8:22:23 AM

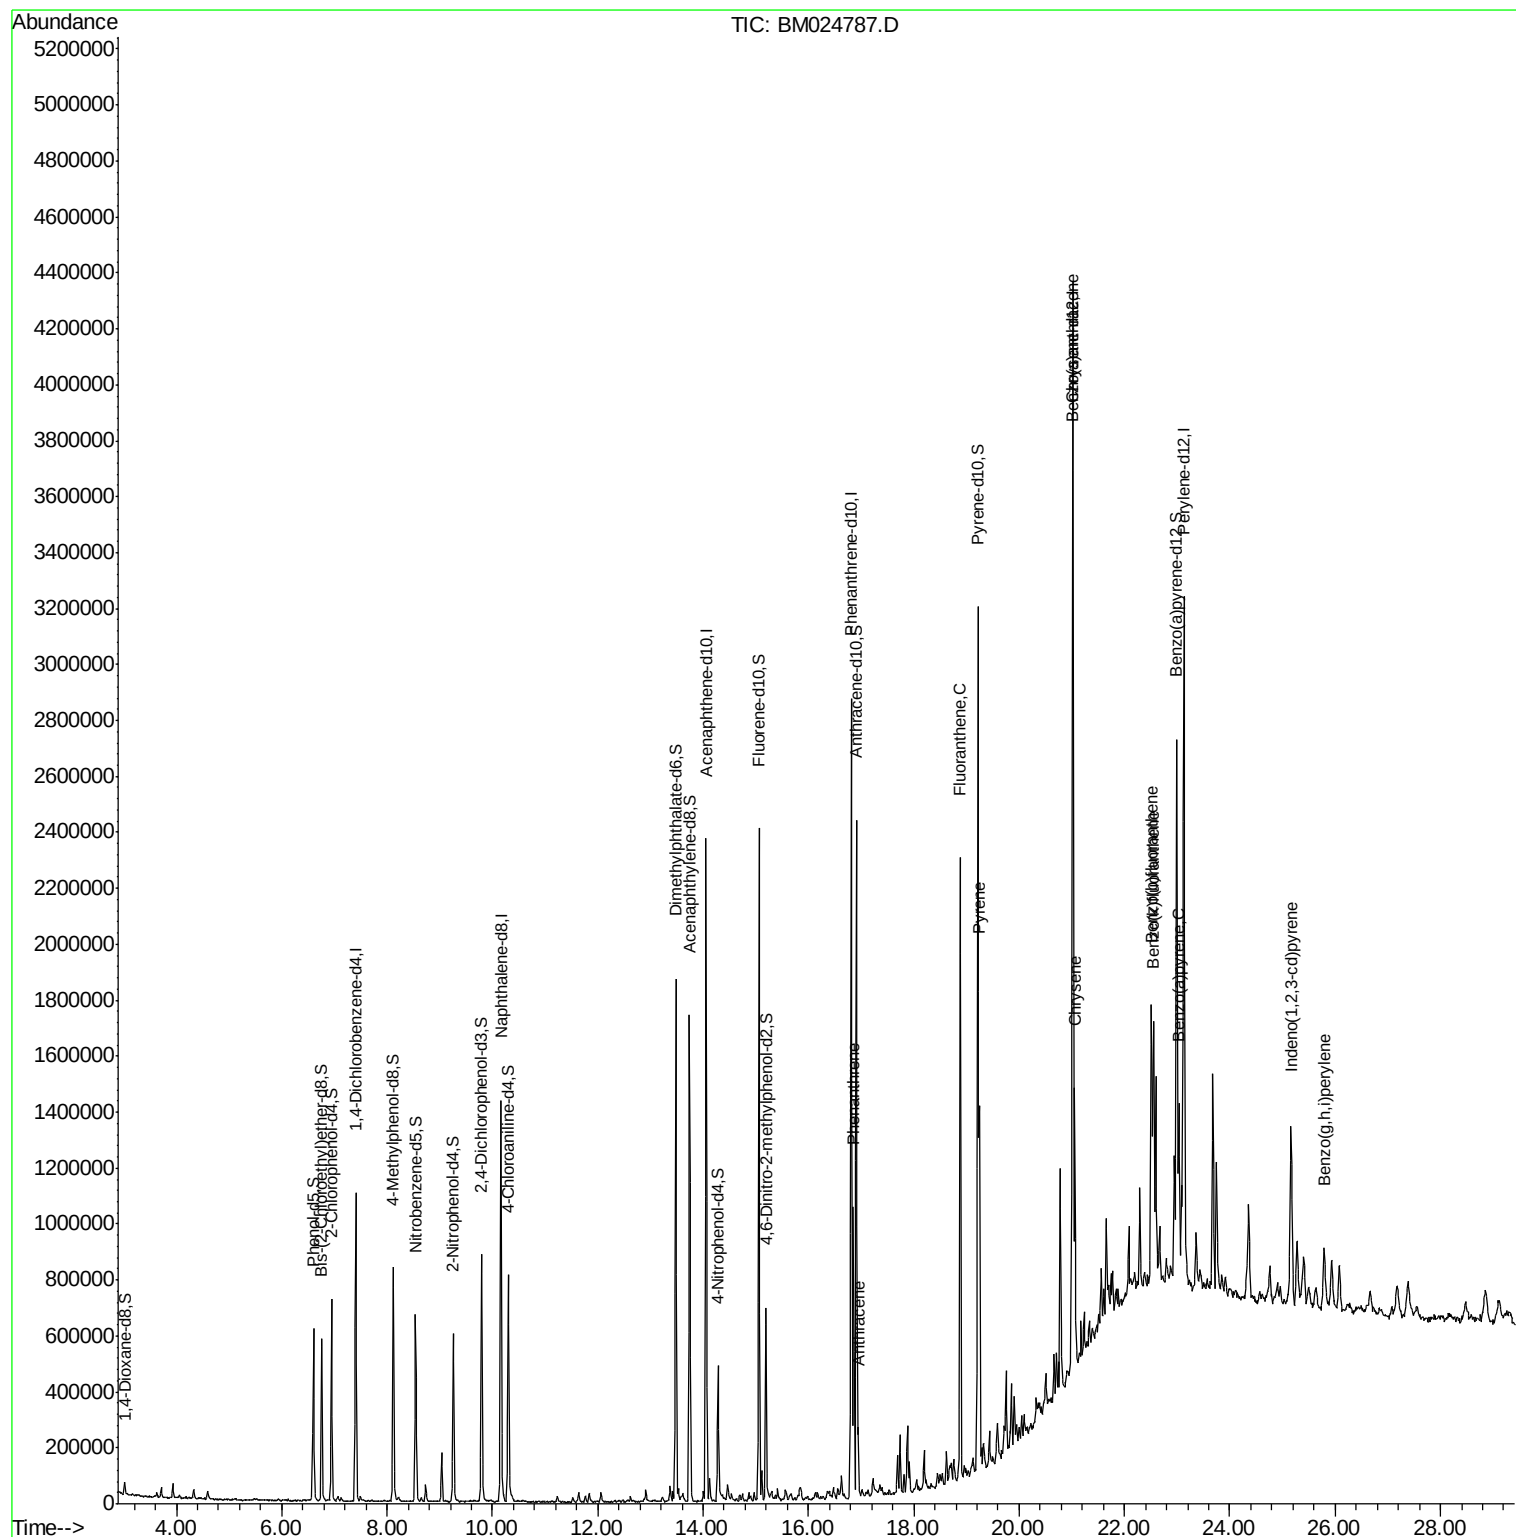

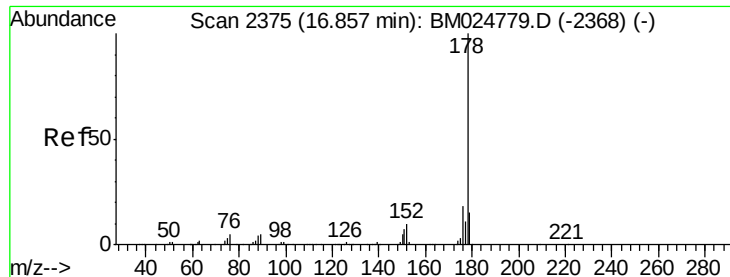





#70
Phenanthrene
Concen: 6.612 ng/ul
RT: 16.85 min Scan# 2374
Delta R.T. -0.01 min
Lab File: BM024787.D
Acq: 08 Feb 2020 07:16

Instrument :
BNA_M
ClientSampleId :
CB6H3

Tot Ion	Ratio	Lower	Upper
178	100		
179	15.6	12.2	18.2
176	18.5	14.5	21.7




Manual Integrations
APPROVED


mohammad
2/11/2020 8:22:23 AM

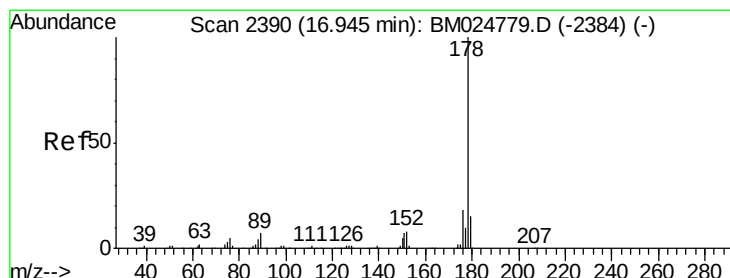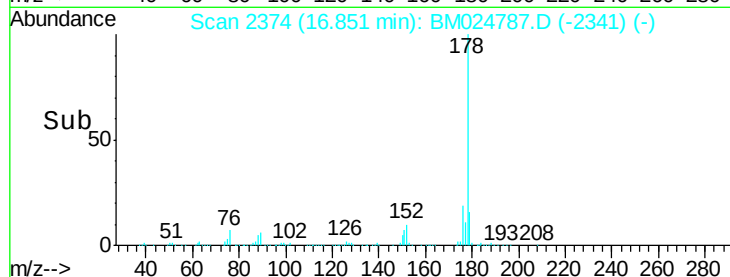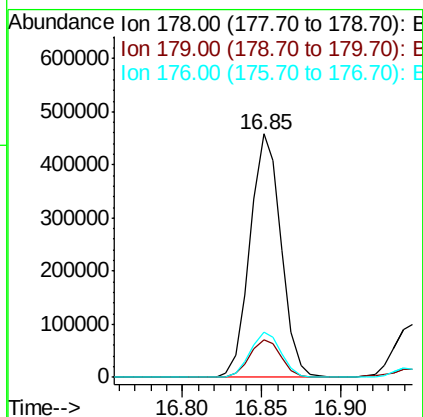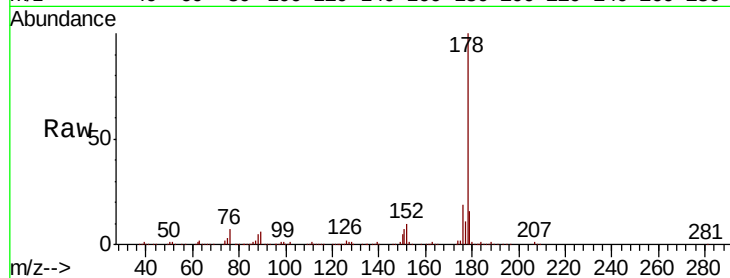

#72
Anthracene
Concen: 1.428 ng/ul
RT: 16.95 min Scan# 2390
Delta R.T. -0.01 min
Lab File: BM024787.D
Acq: 08 Feb 2020 07:16

Tgt Ion	Ratio	Lower	Upper
178	100		
179	15.6	12.3	18.5
176	16.5	14.1	21.1

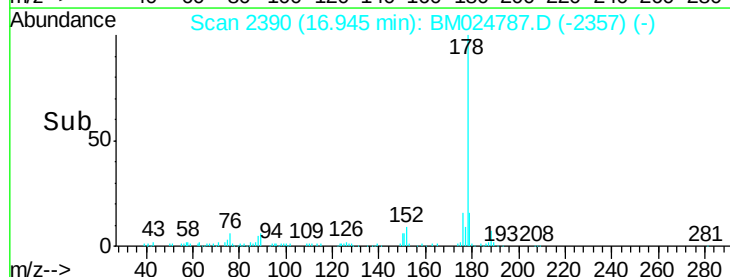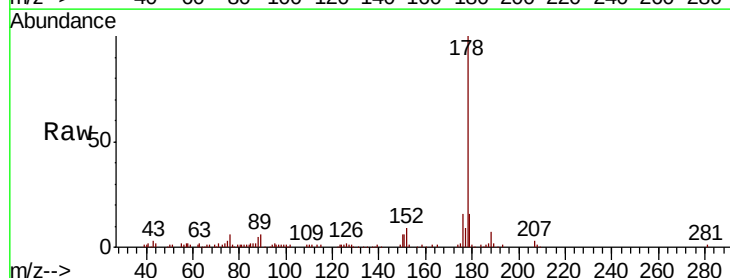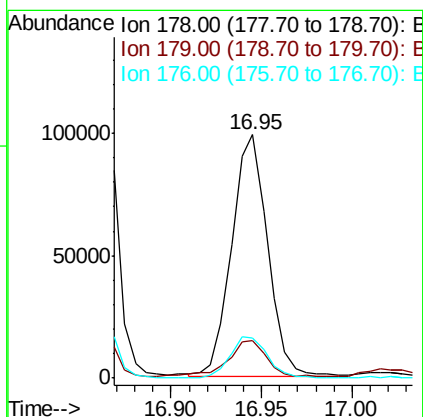

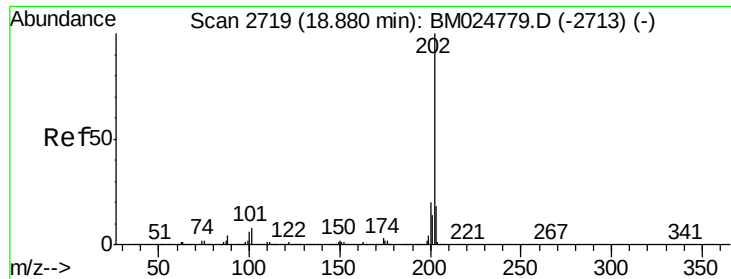





#77
 Fluoranthene
 Concen: 11.746 ng/ul
 RT: 18.88 min Scan# 2719
 Delta R.T. -0.01 min
 Lab File: BM024787.D
 Acq: 08 Feb 2020 07:16

Instrument :
 BNA_M
 ClientSampleId :
 CB6H3

Tot Ion	Ratio	Lower	Upper
202	100		
101	8.0	6.1	9.1
100	6.4	4.8	7.2




Manual Integrations
 APPROVED


mohammad
 2/11/2020 8:22:23 AM

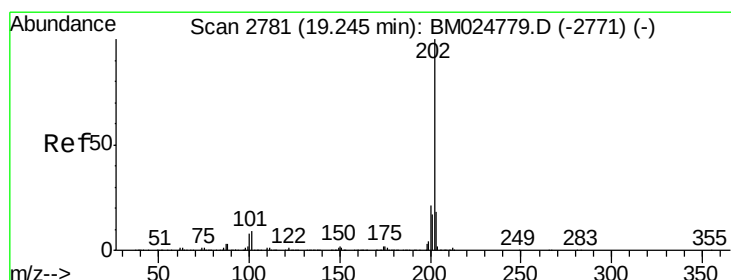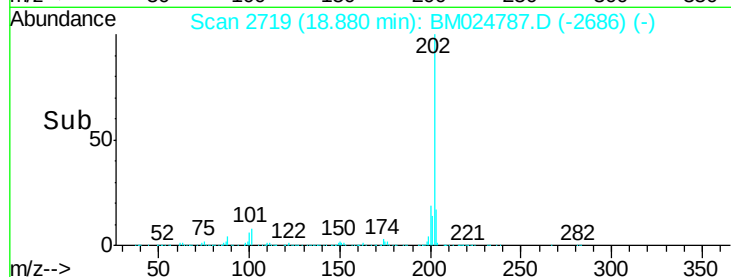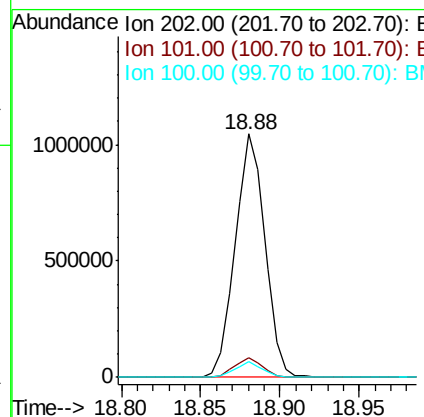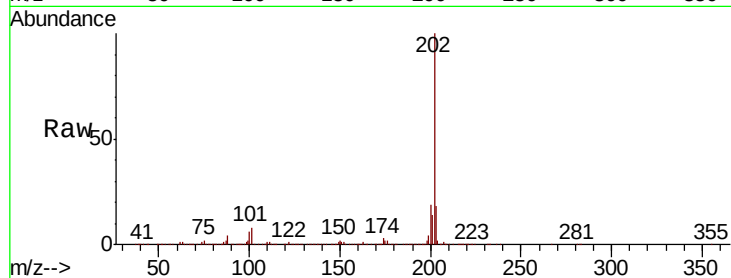

#80
 Pyrene
 Concen: 9.135 ng/ul
 RT: 19.24 min Scan# 2781
 Delta R.T. -0.01 min
 Lab File: BM024787.D
 Acq: 08 Feb 2020 07:16

Tgt Ion	Ratio	Lower	Upper
202	100		
101	8.7	7.0	10.4
100	7.4	5.8	8.8

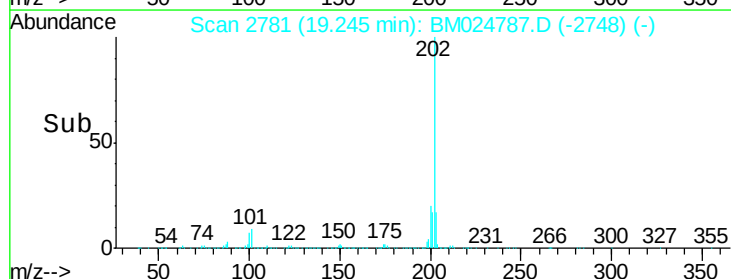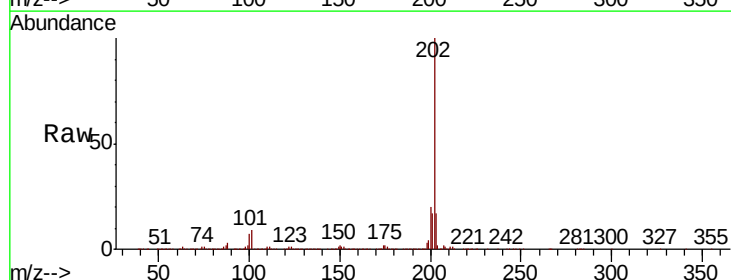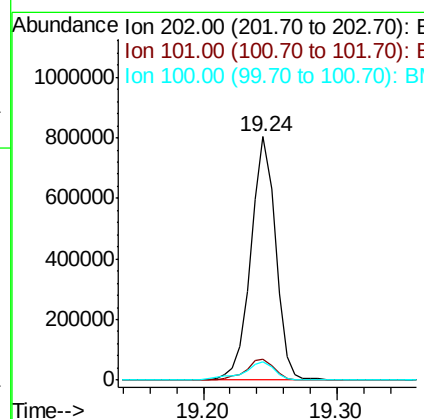

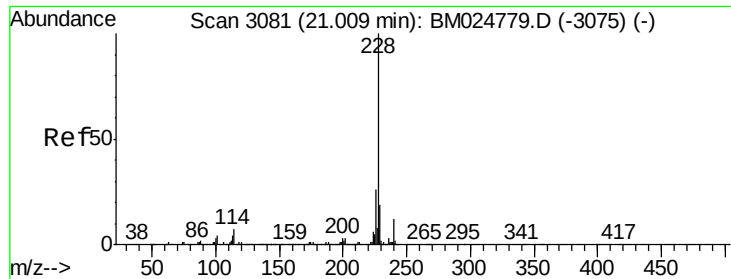





#83
Benzo(a)anthracene
Concen: 5.935 ng/ul
RT: 21.01 min Scan# 3081
Delta R.T. -0.01 min
Lab File: BM024787.D
Acq: 08 Feb 2020 07:16

Instrument :
BNA_M
ClientSampleId :
CB6H3

Tot Ion	Ratio	Lower	Upper
228	100		
229	20.1	15.9	23.9
226	26.4	20.8	31.2




Manual Integrations
APPROVED


mohammad
2/11/2020 8:22:23 AM

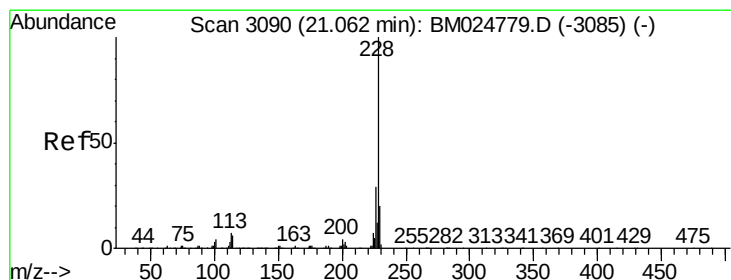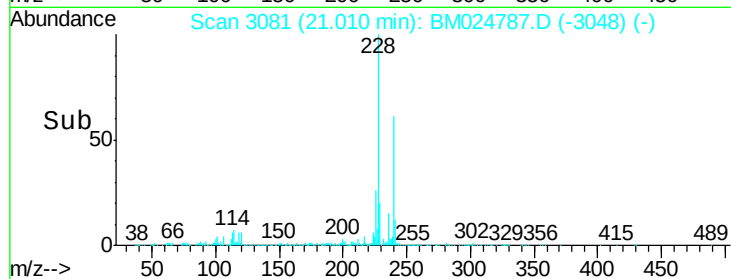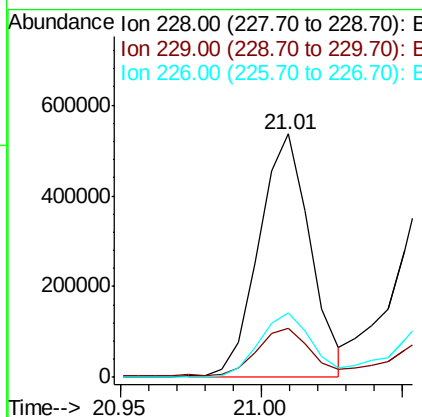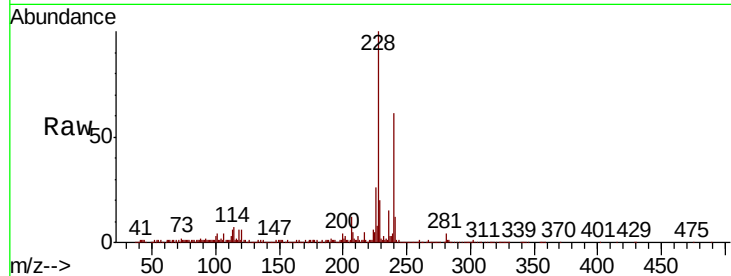

#85
Chrysene
Concen: 5.428 ng/ul
RT: 21.06 min Scan# 3089
Delta R.T. -0.01 min
Lab File: BM024787.D
Acq: 08 Feb 2020 07:16

Tgt Ion	Ratio	Lower	Upper
228	100		
226	28.8	23.0	34.4
229	20.1	15.8	23.8

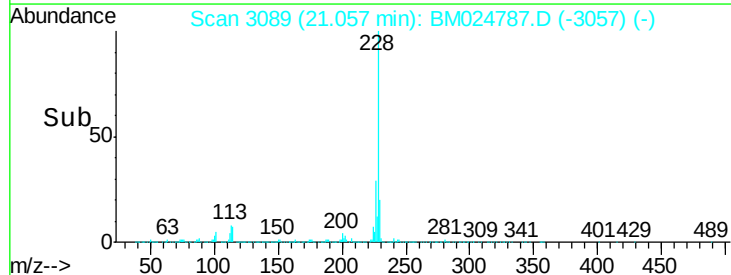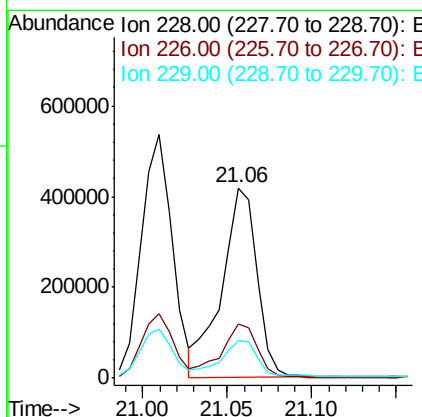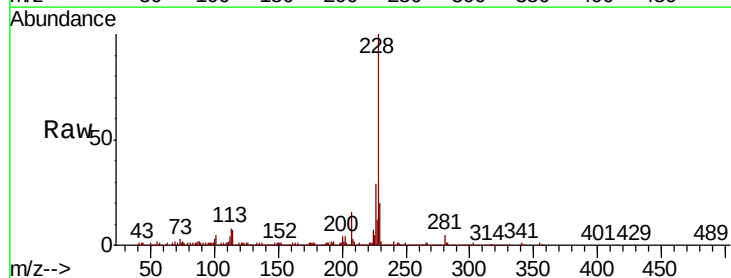

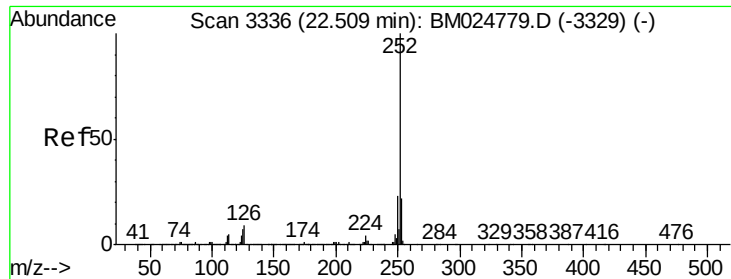





#88
 Benzo(b)fluoranthene
 Concen: 7.935 ng/ul
 RT: 22.51 min Scan# 3336
 Delta R.T. -0.01 min
 Lab File: BM024787.D
 Acq: 08 Feb 2020 07:16

Instrument :
 BNA_M
 ClientSampleID :
 CB6H3

Tot Ion	Ratio	Lower	Upper
252	100		
253	22.6	17.3	25.9
125	7.8	5.1	7.7#




Manual Integrations
 APPROVED


mohammad
 2/11/2020 8:22:23 AM

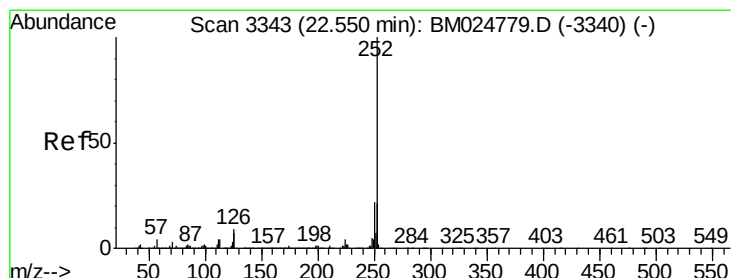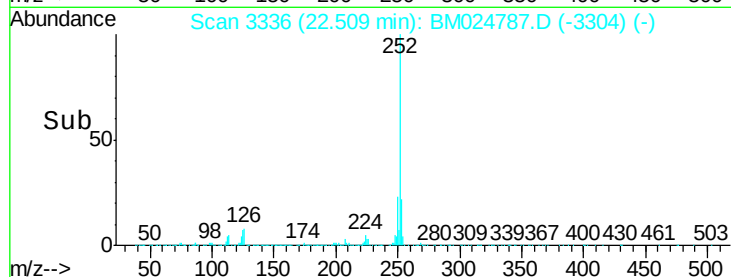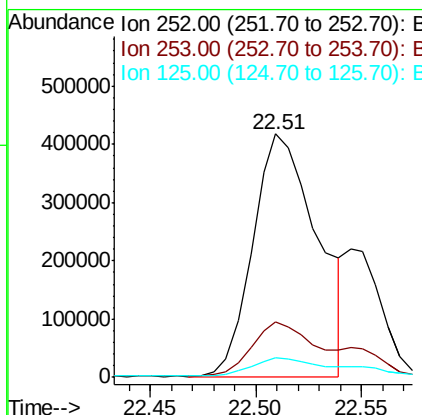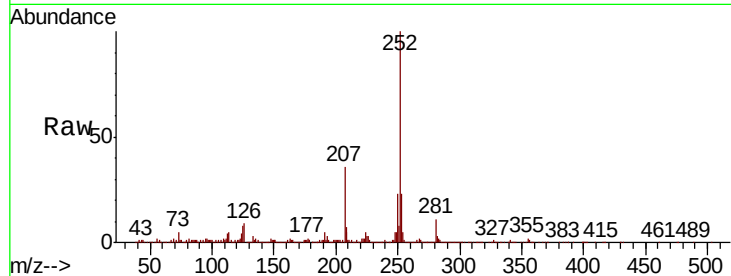

#89
 Benzo(k)fluoranthene
 Concen: 2.351 ng/ul m
 RT: 22.54 min Scan# 3342
 Delta R.T. -0.02 min
 Lab File: BM024787.D
 Acq: 08 Feb 2020 07:16

Tgt Ion	Ratio	Lower	Upper
252	100		
253	23.2	17.4	26.0
125	8.4	5.1	7.7#

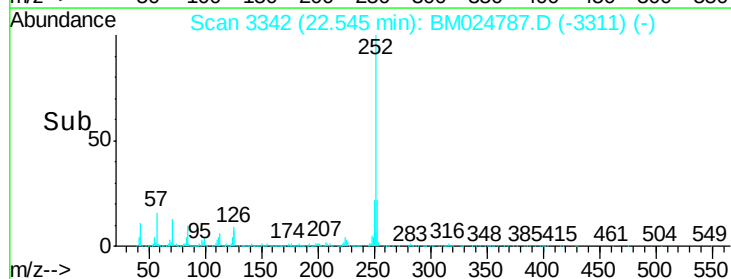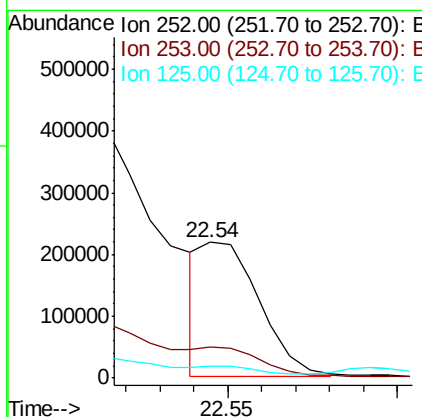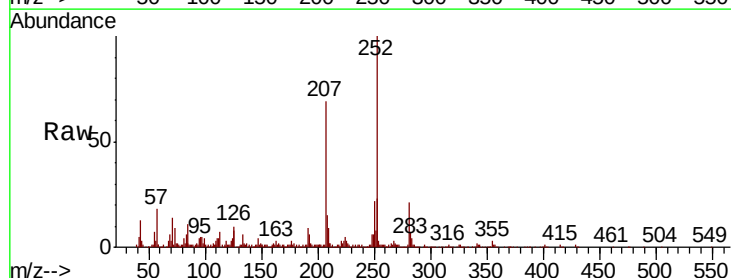

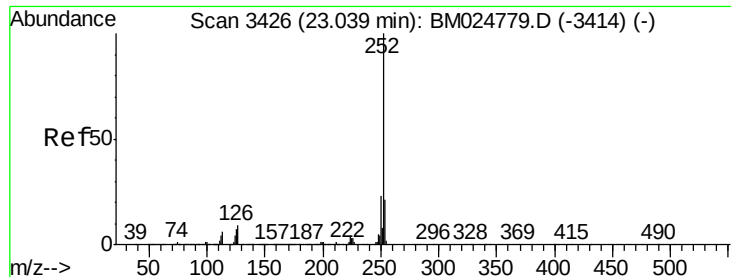





#91
Benzo(a)pyrene
Concen: 4.703 ng/ul
RT: 23.03 min Scan# 3425
Delta R.T. -0.01 min
Lab File: BM024787.D
Acq: 08 Feb 2020 07:16

Instrument :
BNA_M
ClientSampleId :
CB6H3

Tot Ion	Ratio	Lower	Upper
252	100		
253	21.8	17.5	26.3
125	8.4	5.6	8.4#




Manual Integrations
APPROVED


mohammad
2/11/2020 8:22:23 AM

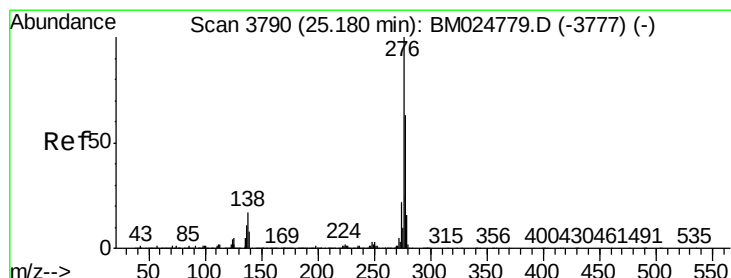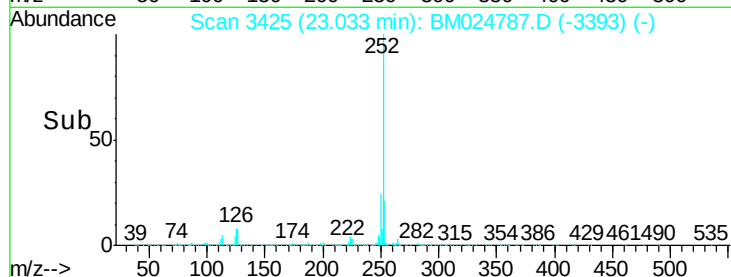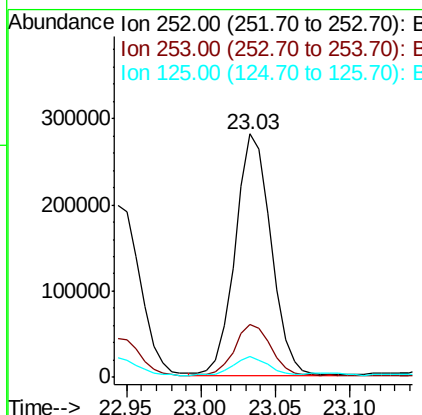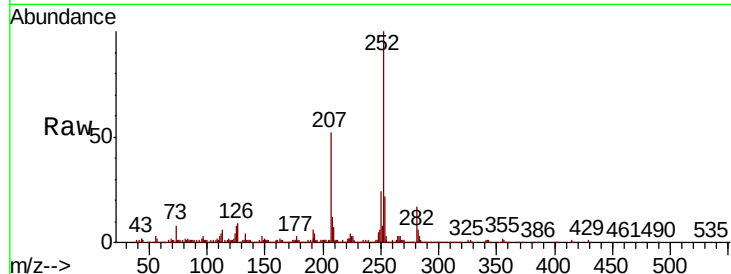

#92
Indeno(1,2,3-cd)pyrene
Concen: 2.972 ng/ul
RT: 25.17 min Scan# 3789
Delta R.T. -0.02 min
Lab File: BM024787.D
Acq: 08 Feb 2020 07:16

Tgt Ion	Ratio	Lower	Upper
276	100		
138	13.9	12.8	19.2
277	25.7	19.3	28.9

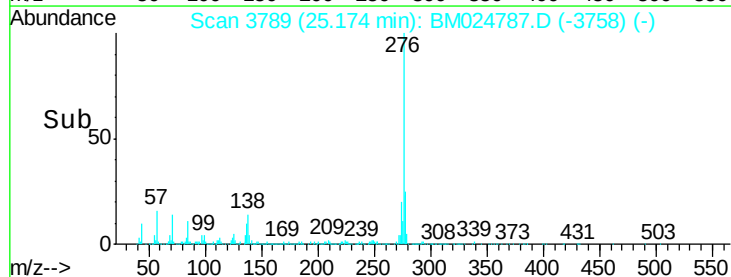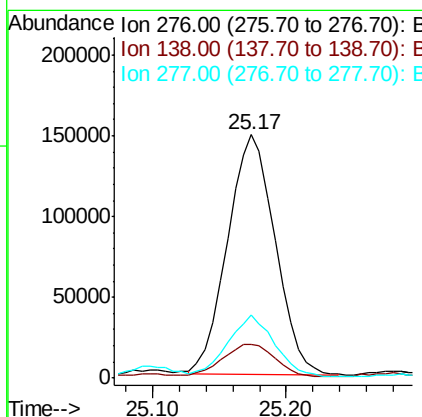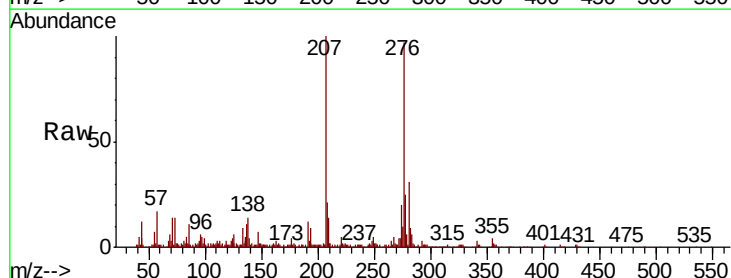

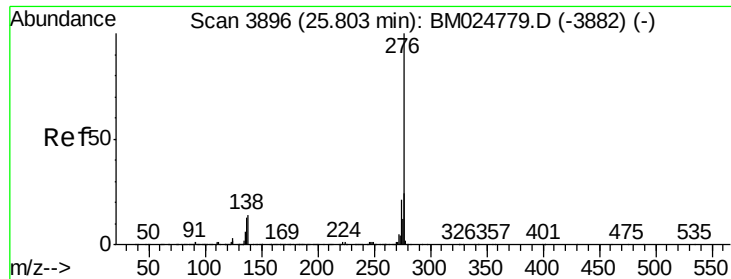

#94

Benzo(a,h,i)perylene

Concen: 2.477 ng/ul

RT: 25.79 min Scan# 3894

Delta R.T. -0.02 min

Lab File: BM024787.D

Acq: 08 Feb 2020 07:16

Instrument :

BNA_M

ClientSampleId :

CB6H3

Tot Ion:	276	Resp:	255914
Ion Ratio	Lower	Upper	
276	100		
138	14.5	11.8	17.6
277	23.0	19.0	28.6

Manual Integrations
APPROVED

mohammad
2/11/2020 8:22:23 AM

