

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM020620\
 Data File : BM024795.D
 Acq On : 08 Feb 2020 12:39
 Operator : CG/JU
 Sample : L1400-14
 Misc :
 ALS Vial : 74 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 CB6J0

Manual Integrations
 APPROVED

mohammad
 2/11/2020 8:22:42 AM

Quant Time: Feb 10 01:18:41 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM020620MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Feb 07 07:38:13 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.40	152	312556	20.00	ng/ul	0.00
18) Naphthalene-d8	10.16	136	1227497	20.00	ng/ul	-0.01
36) Acenaphthene-d10	14.06	164	802059	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.81	188	1706672	20.00	ng/ul	0.00
78) Chrysene-d12	21.02	240	1642660	20.00	ng/ul	-0.01
86) Perylene-d12	23.13	264	1708824	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.02	96	26329	4.05	ng/uL	0.00
5) Phenol-d5	6.60	99	439440	21.16	ng/ul	-0.01
7) Bis-(2-Chloroethyl)ether-d	6.75	67	291421	24.85	ng/ul	-0.01
9) 2-Chlorophenol-d4	6.95	132	410992	22.09	ng/ul	0.00
13) 4-Methylphenol-d8	8.12	113	343242	19.59	ng/ul	-0.01
19) Nitrobenzene-d5	8.54	128	214342	24.15	ng/ul	-0.01
22) 2-Nitrophenol-d4	9.26	143	255022	24.32	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.79	165	436294	20.62	ng/ul	-0.01
29) 4-Chloroaniline-d4	10.30	131	533799	26.97	ng/ul	0.00
44) Dimethylphthalate-d6	13.48	166	1521186	25.13	ng/ul	0.00
47) Acenaphthylene-d8	13.74	160	1578929	22.33	ng/ul	-0.01
52) 4-Nitrophenol-d4	14.28	143	191764	19.49	ng/ul	0.00
58) Fluorene-d10	15.06	176	1234893	23.03	ng/ul	-0.01
63) 4,6-Dinitro-2-methylphenol	15.19	200	224890	20.22	ng/ul	0.00
71) Anthracene-d10	16.91	188	1747098	22.42	ng/ul	0.00
79) Pyrene-d10	19.22	212	1842449	22.42	ng/ul	0.00
90) Benzo(a)pyrene-d12	22.99	264	1833842	21.37	ng/ul	-0.01

Target Compounds

					Ovalue	
70) Phenanthrene	16.85	178	441439	4.744	ng/ul	100
77) Fluoranthene	18.88	202	963374	8.433	ng/ul	99
80) Pyrene	19.24	202	796777	7.328	ng/ul	99
83) Benzo(a)anthracene	21.01	228	488969	4.419	ng/ul	97
85) Chrysene	21.06	228	466614	4.283	ng/ul	98
88) Benzo(b)fluoranthene	22.51	252	692355	6.372	ng/ul#	98
89) Benzo(k)fluoranthene	22.54	252	190421m	1.821	ng/ul	
91) Benzo(a)pyrene	23.03	252	381365	3.915	ng/ul#	98
92) Indeno(1,2,3-cd)pyrene	25.17	276	299243	2.467	ng/ul	95
94) Benzo(g,h,i)perylene	25.80	276	233679	2.317	ng/ul	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM020620\
Data File : BM024795.D
Acq On : 08 Feb 2020 12:39
Operator : CG/JU
Sample : L1400-14
Misc :
ALS Vial : 74 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampled :
CB6J0

Manual Integrations
APPROVED

mohammad
2/11/2020 8:22:42 AM

Quant Time: Feb 10 01:18:41 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM020620MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Feb 07 07:38:13 2020
Response via : Initial Calibration

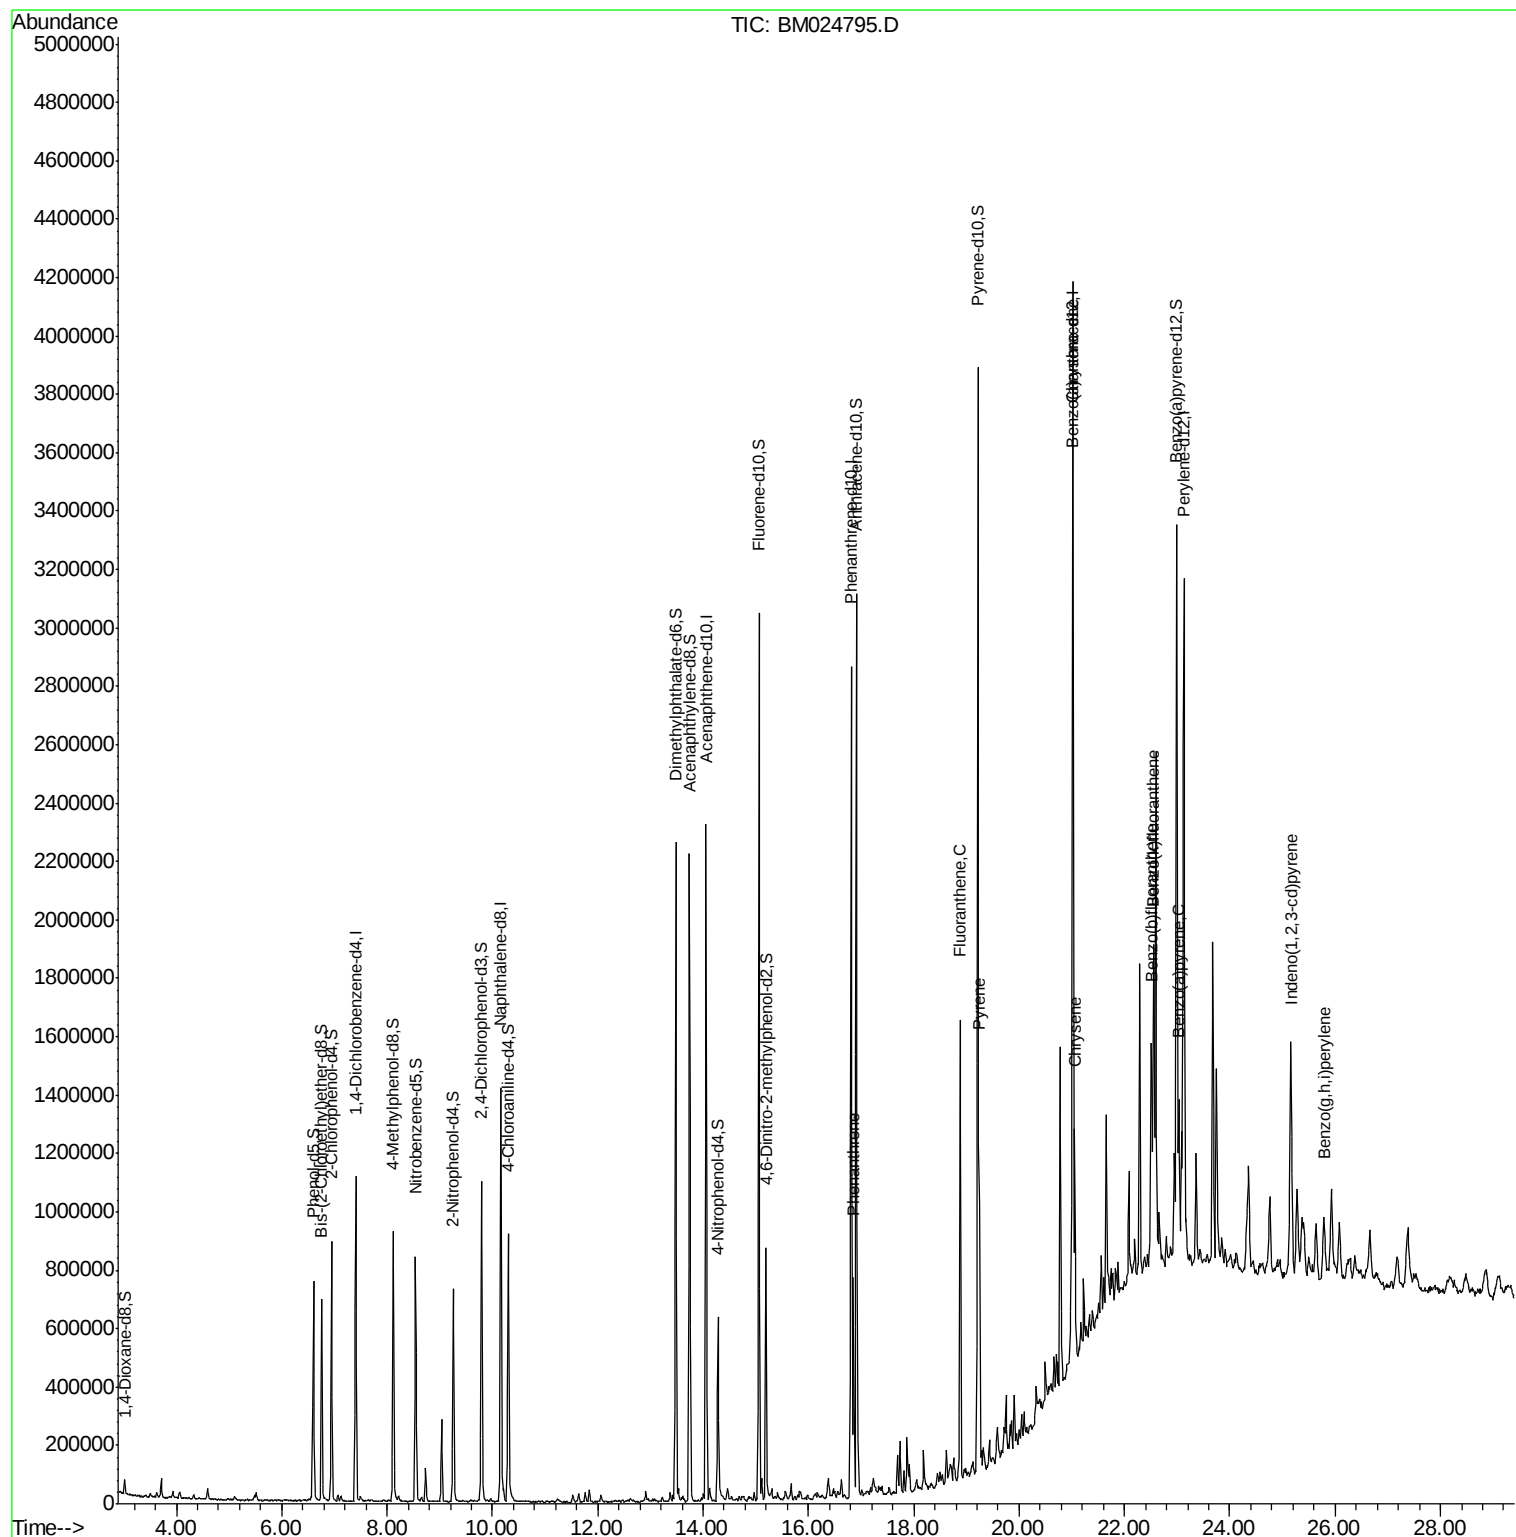

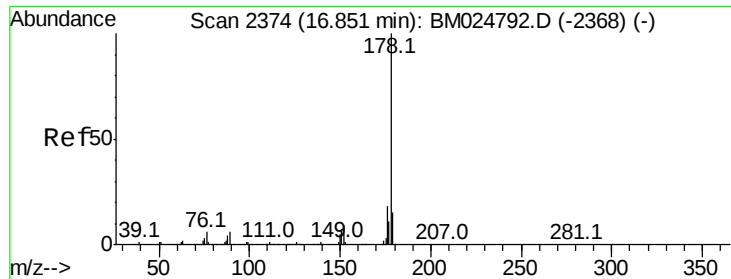





#70
Phenanthrene
Concen: 4.744 ng/ul
RT: 16.85 min Scan# 2374
Delta R.T. -0.01 min
Lab File: BM024795.D
Acq: 08 Feb 2020 12:39

Instrument :
BNA_M
ClientSampleId :
CB6J0

Tot Ion	Ratio	Lower	Upper
178	100		
179	15.3	12.2	18.2
176	17.8	14.5	21.7




Manual Integrations
APPROVED


mohammad
2/11/2020 8:22:42 AM

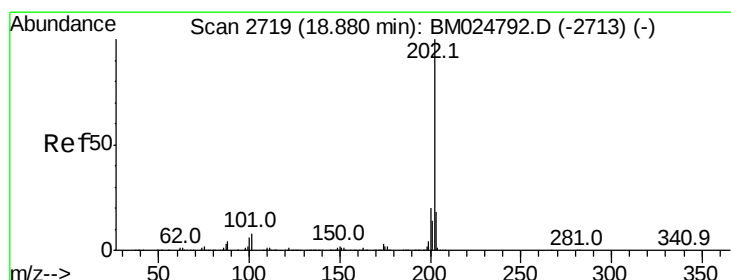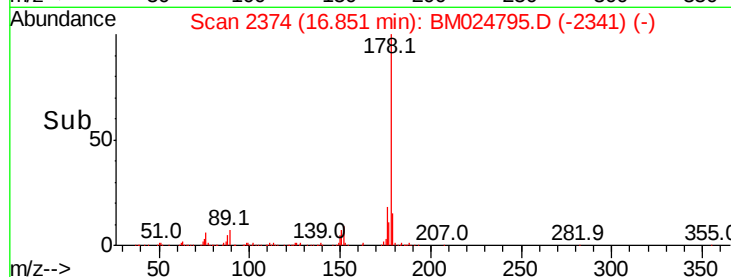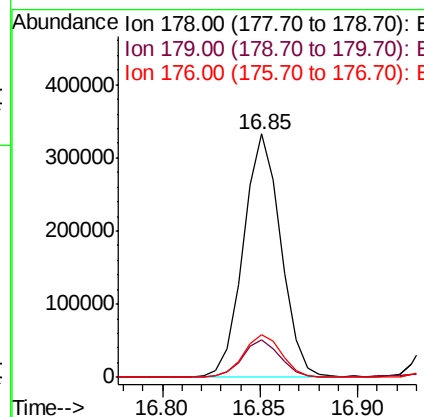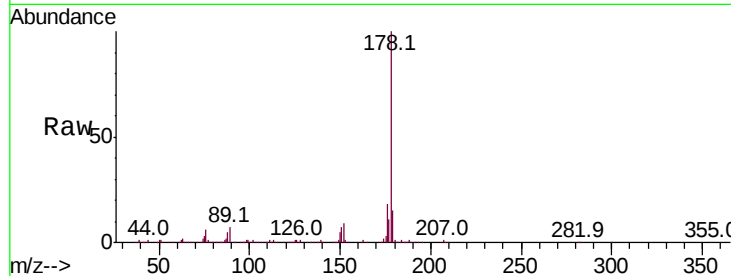

#77
Fluoranthene
Concen: 8.433 ng/ul
RT: 18.88 min Scan# 2719
Delta R.T. -0.01 min
Lab File: BM024795.D
Acq: 08 Feb 2020 12:39

Tgt Ion	Ratio	Lower	Upper
202	100		
101	8.0	6.1	9.1
100	6.0	4.8	7.2

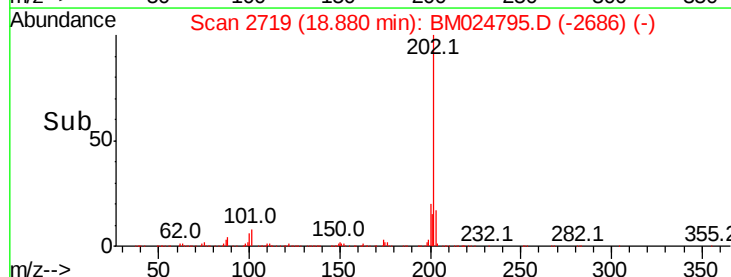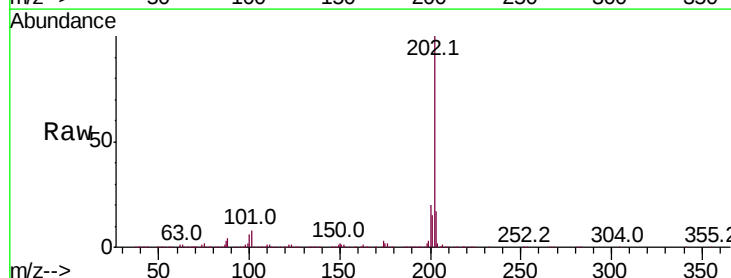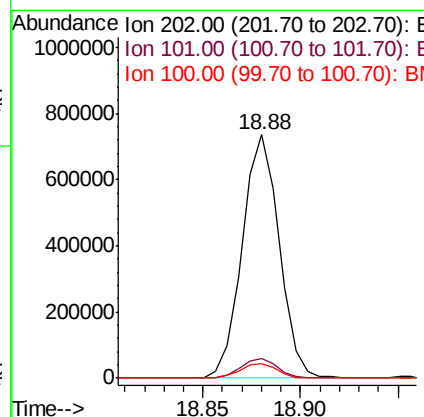

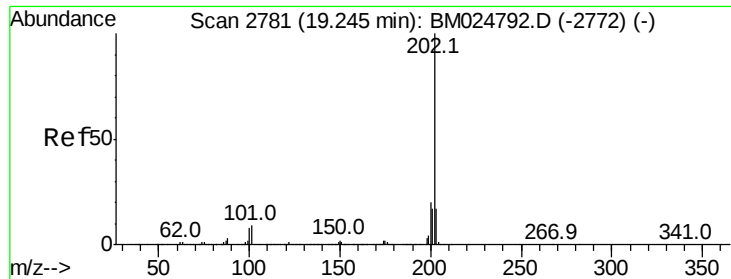


#80
Pvrene
Concen: 7.328 ng/ul
RT: 19.24 min Scan# 2781
Delta R.T. -0.01 min
Lab File: BM024795.D
Acq: 08 Feb 2020 12:39

Instrument :
BNA_M
ClientSampleId :
CB6J0

Tot Ion	Ratio	Resp Lower	Upper
202	100		
101	9.0	7.0	10.4
100	7.8	5.8	8.8

Manual Integrations
APPROVED

mohammad
2/11/2020 8:22:42 AM



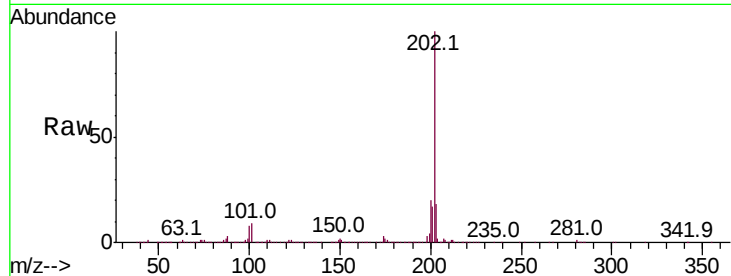


Abundance

Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): E

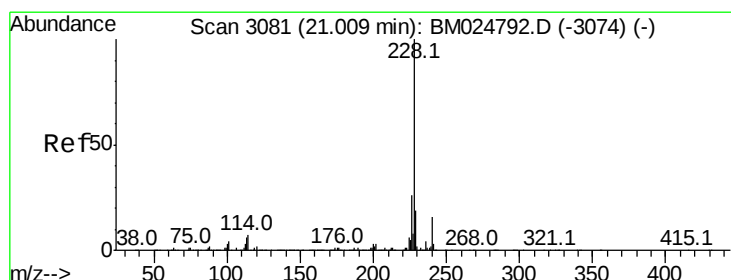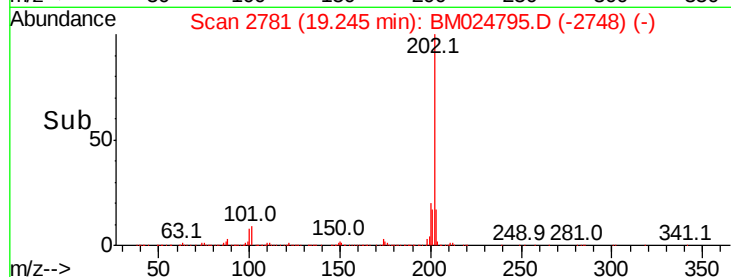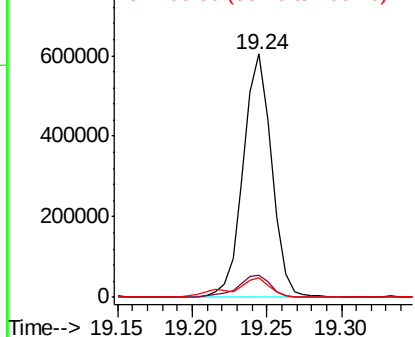

#83
Benzo(a)anthracene
Concen: 4.419 ng/ul
RT: 21.01 min Scan# 3081
Delta R.T. -0.01 min
Lab File: BM024795.D
Acq: 08 Feb 2020 12:39




Tgt Ion	Ratio	Resp Lower	Upper
228	100		
229	20.3	15.9	23.9
226	28.7	20.8	31.2


Abundance

Ion 228.00 (227.70 to 228.70): E

Ion 229.00 (228.70 to 229.70): E

Ion 226.00 (225.70 to 226.70): E

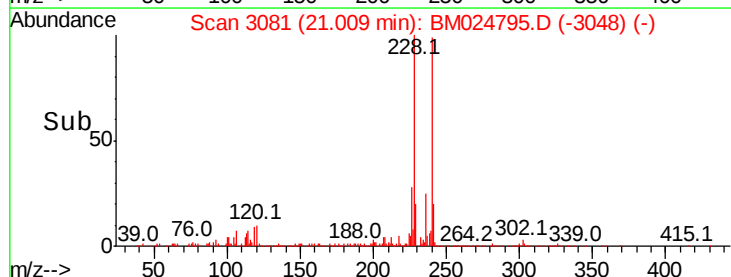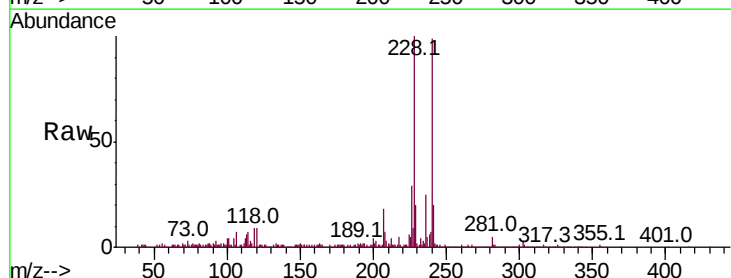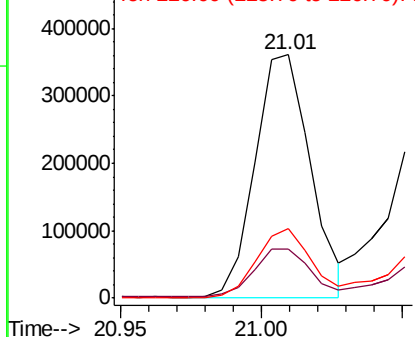

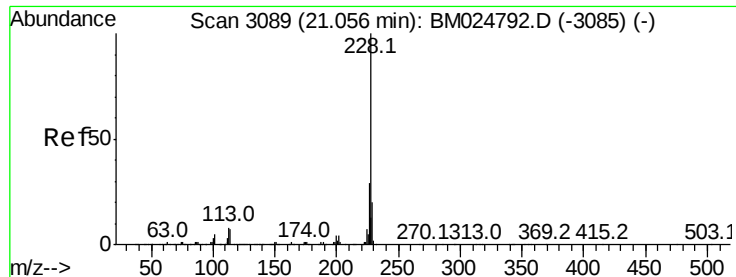





#85
Chrysene
Concen: 4.283 ng/ul
RT: 21.06 min Scan# 3089
Delta R.T. -0.01 min
Lab File: BM024795.D
Acq: 08 Feb 2020 12:39

Instrument :
BNA_M
ClientSampled :
CB6J0

Tot Ion	Ratio	Lower	Upper
228	100		
226	30.0	23.0	34.4
229	20.7	15.8	23.8




Manual Integrations
APPROVED


mohammad
2/11/2020 8:22:42 AM

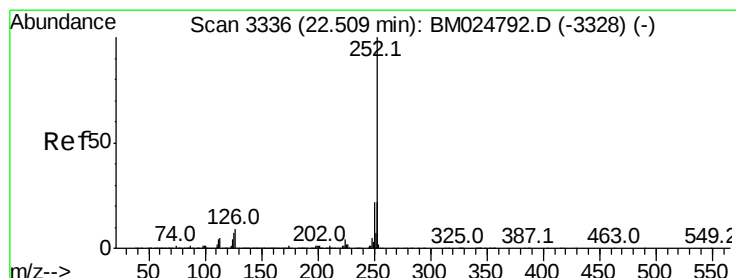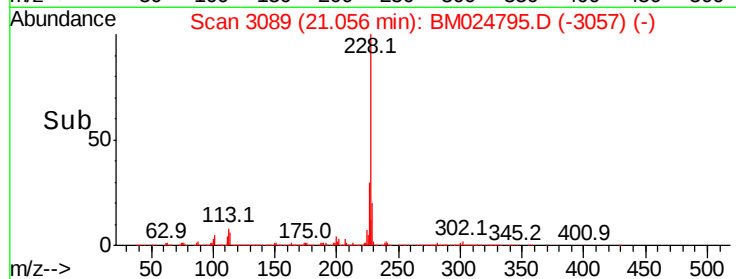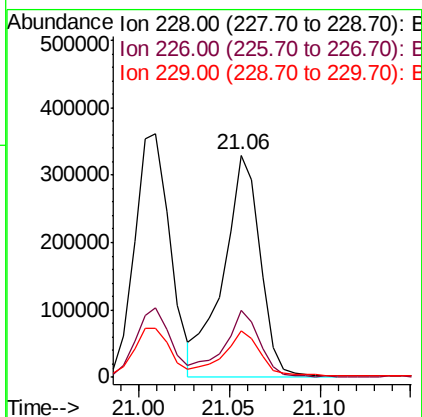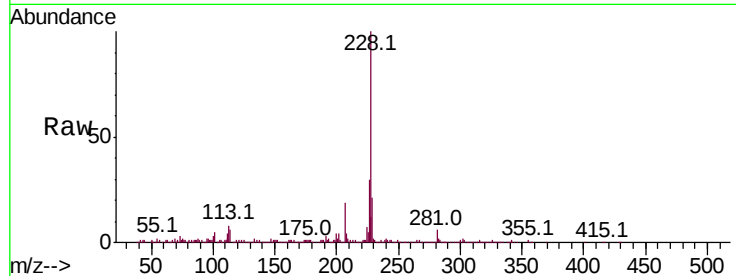

#88
Benzo(b)fluoranthene
Concen: 6.372 ng/ul
RT: 22.51 min Scan# 3336
Delta R.T. -0.01 min
Lab File: BM024795.D
Acq: 08 Feb 2020 12:39

Tgt Ion	Ratio	Lower	Upper
252	100		
253	22.3	17.3	25.9
125	7.9	5.1	7.7#

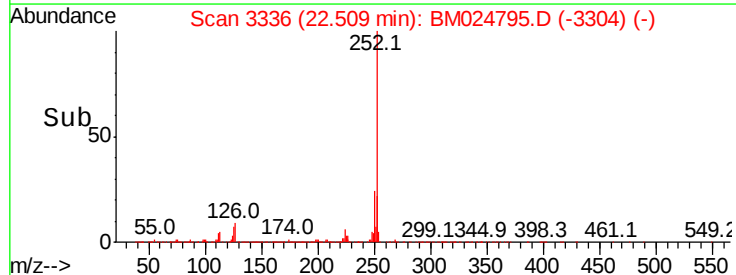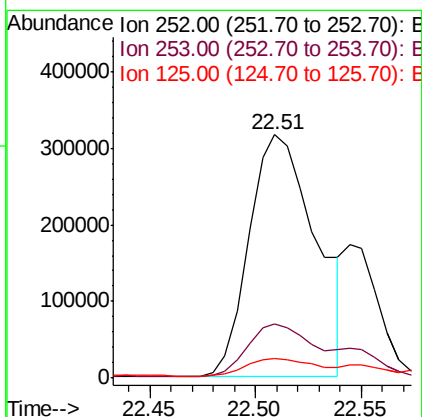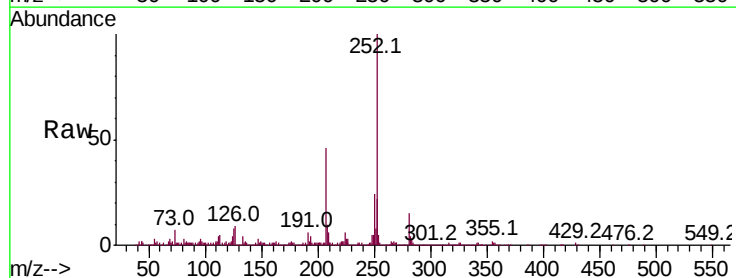

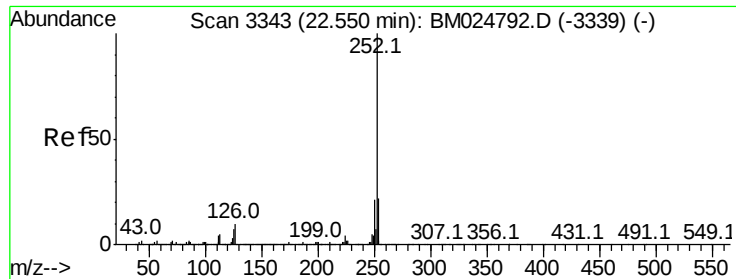





#89
Benzo(k)fluoranthene
Concen: 1.821 ng/ul m
RT: 22.54 min Scan# 3342
Delta R.T. -0.02 min
Lab File: BM024795.D
Acq: 08 Feb 2020 12:39

Instrument :
BNA_M
ClientSampled :
CB6J0

Tot Ion	Ratio	Resp Lower	Upper
252	100		
253	22.6	17.4	26.0
125	9.6	5.1	7.7#




Manual Integrations
APPROVED


mohammad
2/11/2020 8:22:42 AM

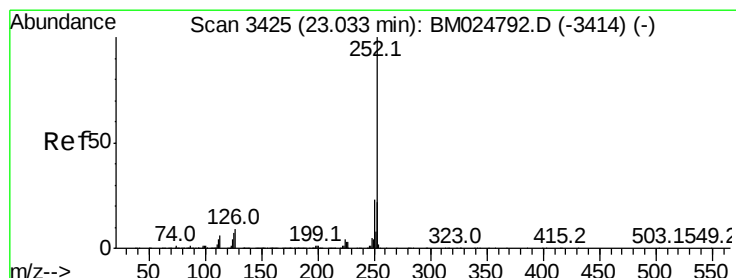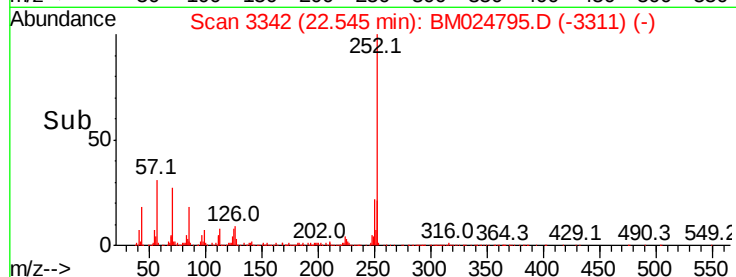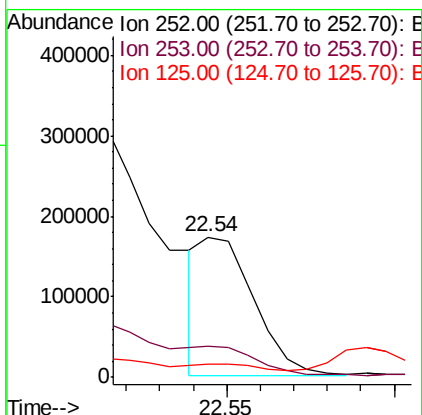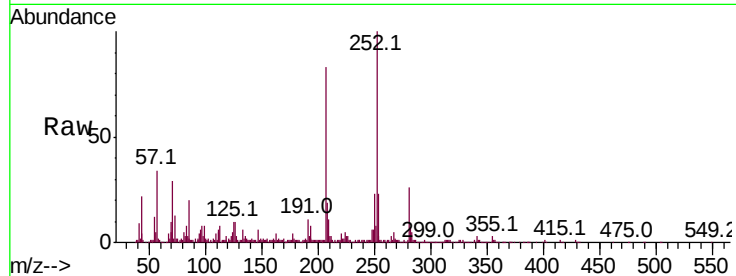

#91
Benzo(a)pyrene
Concen: 3.915 ng/ul
RT: 23.03 min Scan# 3425
Delta R.T. -0.01 min
Lab File: BM024795.D
Acq: 08 Feb 2020 12:39

Tgt Ion	Ratio	Resp Lower	Upper
252	100		
253	22.3	17.5	26.3
125	8.5	5.6	8.4#

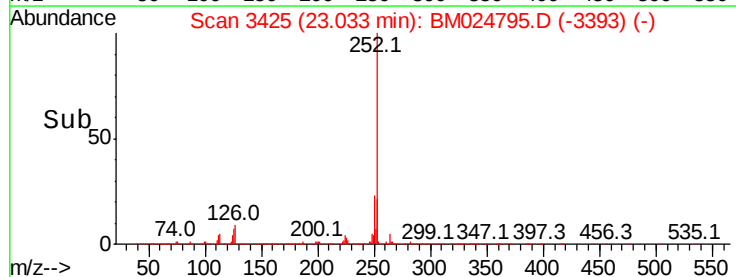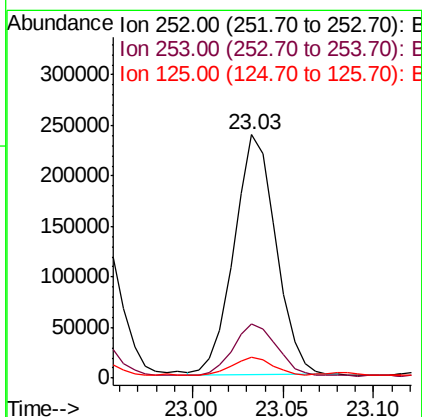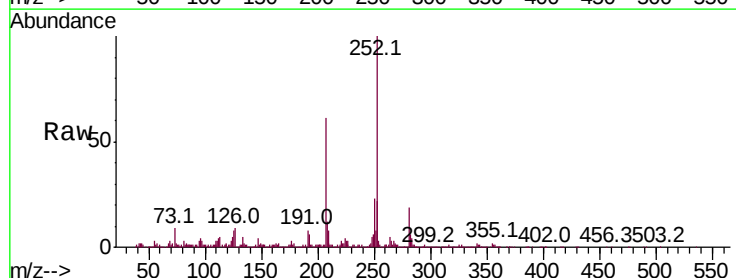

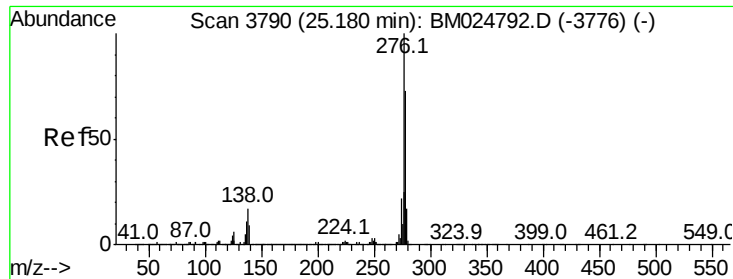

#92





Indeno(1,2,3-cd)pyrene
Concen: 2.467 ng/ul
RT: 25.17 min Scan# 3789
Delta R.T. -0.02 min
Lab File: BM024795.D
Acq: 08 Feb 2020 12:39

Instrument :
BNA_M
ClientSampleId :
CB6J0

Tot Ion	Ratio	Lower	Upper
276	100		
138	13.7	12.8	19.2
277	26.2	19.3	28.9

Manual Integrations
APPROVED

mohammad
2/11/2020 8:22:42 AM

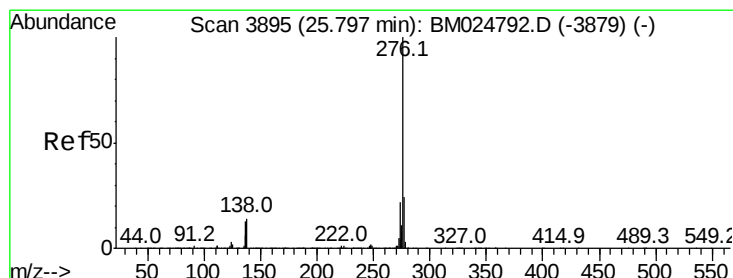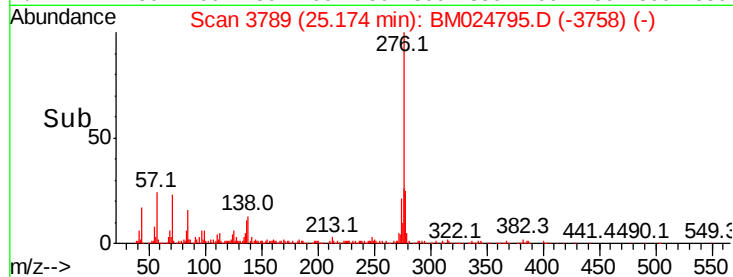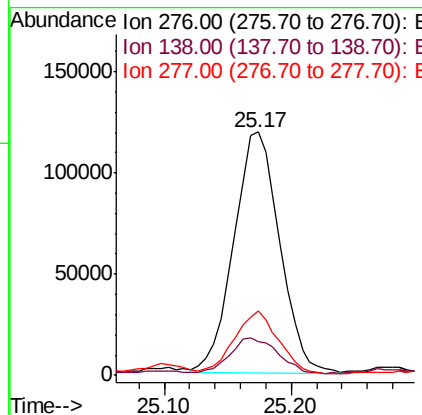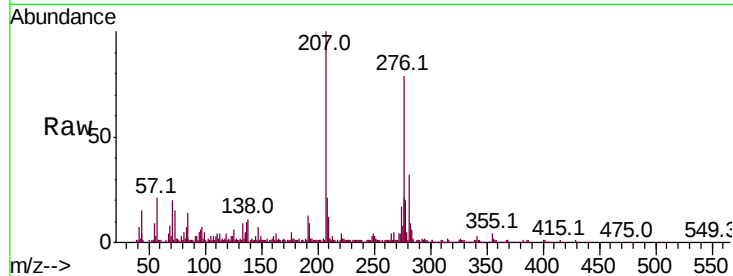

#94

Benzo(g,h,i)perylene
Concen: 2.317 ng/ul
RT: 25.80 min Scan# 3895
Delta R.T. -0.02 min
Lab File: BM024795.D
Acq: 08 Feb 2020 12:39

Tgt Ion	Ratio	Lower	Upper
276	100		
138	15.4	11.8	17.6
277	25.3	19.0	28.6

