

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM020620\
 Data File : BM024777.D
 Acq On : 08 Feb 2020 00:41
 Operator : CG/JU
 Sample : L1398-14
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 CB6E8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM020620MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.016	19	22	26	rBV	28245	30061	0.67%	0.058%
2	3.281	64	67	68	rBV3	4284	5092	0.11%	0.010%
3	3.634	119	127	132	rBV	16985	30243	0.67%	0.058%
4	3.716	136	141	144	rBV2	12126	18017	0.40%	0.035%
5	3.881	165	169	173	rVB5	3898	7072	0.16%	0.014%
6	3.934	173	178	185	rBV5	10369	15659	0.35%	0.030%
7	4.187	218	221	222	rBV3	5043	5345	0.12%	0.010%
8	4.316	239	243	244	rBV4	5797	7361	0.16%	0.014%
9	4.593	285	290	298	rBV	31634	58457	1.30%	0.112%
10	5.004	357	360	363	rBV5	2648	4657	0.10%	0.009%
11	5.287	405	408	411	rBV4	3978	5192	0.12%	0.010%
12	6.604	626	632	644	rBV	650215	1022503	22.69%	1.960%
13	6.757	650	658	670	rBV	555954	834853	18.53%	1.600%
14	6.945	684	690	698	rBV	756030	1142832	25.37%	2.191%
15	7.404	761	768	778	rBV	992322	1526392	33.88%	2.926%
16	8.122	883	890	900	rBV	871097	1416898	31.45%	2.716%
17	8.228	903	908	915	rVB	14444	25420	0.56%	0.049%
18	8.545	955	962	975	rBV	668055	1087020	24.13%	2.084%
19	9.033	1039	1045	1050	rBV5	3178	6459	0.14%	0.012%
20	9.257	1077	1083	1093	rBV	615537	983137	21.82%	1.885%
21	9.798	1166	1175	1188	rBV	966458	1645289	36.52%	3.154%
22	10.163	1229	1237	1249	rBV	1329852	2132254	47.33%	4.087%
23	10.304	1253	1261	1272	rBV	878841	1514911	33.62%	2.904%
24	13.480	1795	1801	1813	rBV	1789689	2464209	54.69%	4.724%
25	13.745	1839	1846	1860	rBV	2074874	3013363	66.88%	5.776%
26	14.057	1892	1899	1909	rBV	2078157	3038714	67.45%	5.825%
27	14.280	1931	1937	1956	rBV	486330	890529	19.77%	1.707%
28	14.510	1970	1976	1979	rVB6	5335	7753	0.17%	0.015%
29	14.910	2041	2044	2048	rBV3	4673	7877	0.17%	0.015%
30	15.062	2063	2070	2079	rBV	2649267	3678753	81.65%	7.052%
31	15.192	2086	2092	2106	rBV	710499	977033	21.69%	1.873%
32	15.304	2106	2111	2116	rVB2	27430	38349	0.85%	0.074%
33	15.851	2201	2204	2208	rVB3	9328	11833	0.26%	0.023%
34	16.604	2327	2332	2336	rBV2	8932	14625	0.32%	0.028%

LSC Area Percent Report

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM020620\
Data File : BM024777.D
Acq On : 08 Feb 2020 00:41
Operator : CG/JU
Sample : L1398-14
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
CB6E8

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 0.1 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM020620MA.M
Title : SVOA CALIBRATION

35	16.809	2361	2367	2378	rBV	2535356	3559182	79.00%	6.822%
36	16.909	2378	2384	2396	rVV2	2855771	3848357	85.42%	7.377%
37	17.133	2419	2422	2427	rVB	12611	13613	0.30%	0.026%
38	17.750	2523	2527	2532	rBV6	7605	11256	0.25%	0.022%
39	17.815	2534	2538	2543	rVB	23988	27790	0.62%	0.053%
40	18.198	2599	2603	2604	rVB3	6042	6077	0.13%	0.012%
41	18.921	2722	2726	2730	rVB	38763	49707	1.10%	0.095%
42	19.103	2752	2757	2761	rBV3	26764	38119	0.85%	0.073%
43	19.215	2770	2776	2785	rBV	3264059	4505414	100.00%	8.636%
44	21.021	3078	3083	3092	rBV	3046472	3961277	87.92%	7.593%
45	22.086	3261	3264	3269	rVB4	124722	163621	3.63%	0.314%
46	22.997	3412	3419	3429	rVB2	2399634	4186158	92.91%	8.024%
47	23.085	3430	3434	3435	rVV2	229720	313756	6.96%	0.601%
48	23.127	3435	3441	3450	rVB	2139873	3816354	84.71%	7.315%


Sum of corrected areas: 52168843

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM020620\
Data File : BM024777.D
Acq On : 08 Feb 2020 00:41
Operator : CG/JU
Sample : L1398-14
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
CB6E8

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM020620MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

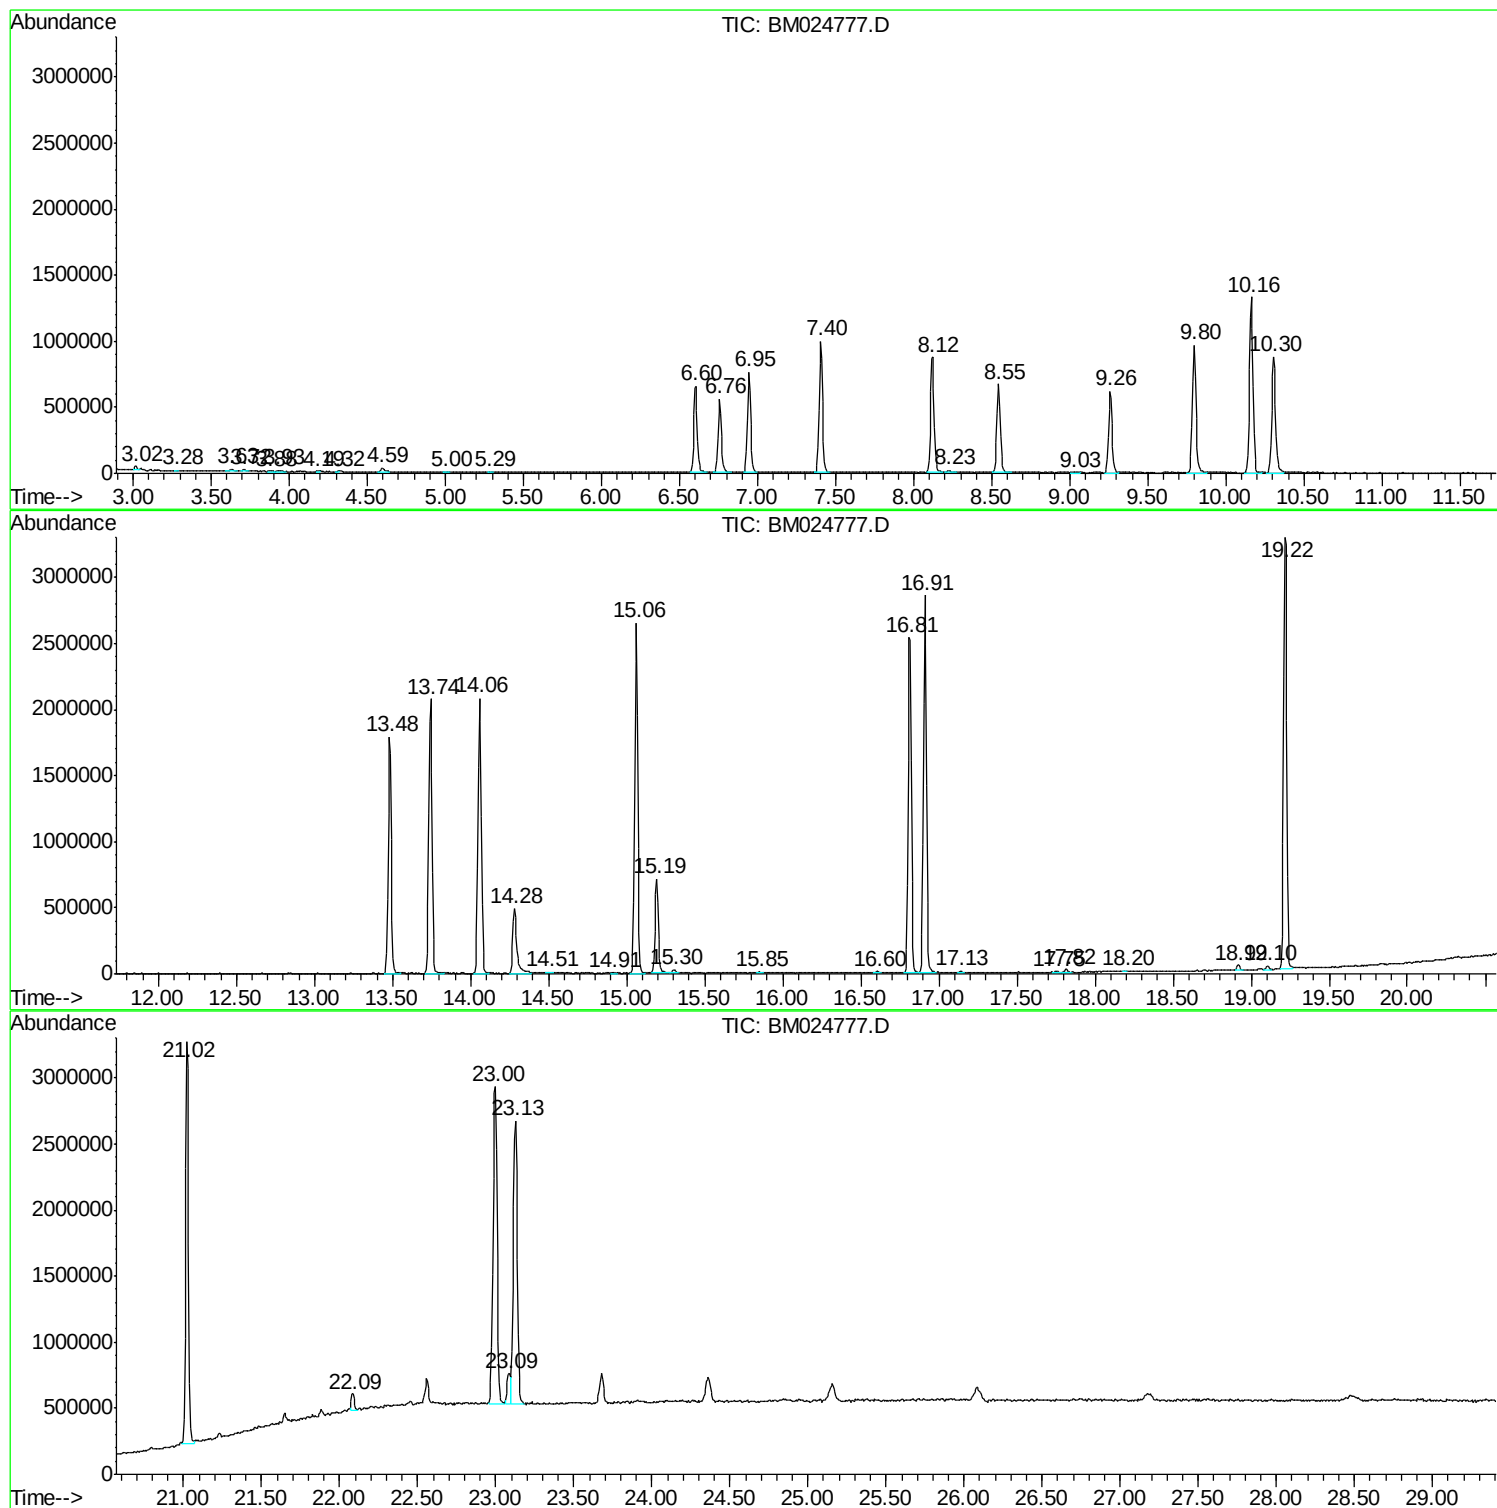

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM020620\
Data File : BM024777.D
Acq On : 08 Feb 2020 00:41
Operator : CG/JU
Sample : L1398-14
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
CB6E8

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM020620MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM020620\
Data File : BM024777.D
Acq On : 08 Feb 2020 00:41
Operator : CG/JU
Sample : L1398-14
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
CB6E8

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM020620MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc