


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM020821\
Data File : BM028675.D
Acq On : 08 Feb 2021 15:34
Operator : CG/JU
Sample : M1311-04
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0A60

Manual Integrations
APPROVED

mohammad
2/9/2021 2:11:50 PM

Quant Time: Feb 08 16:10:00 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM020521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 08 13:26:08 2021
Response via : Initial Calibration

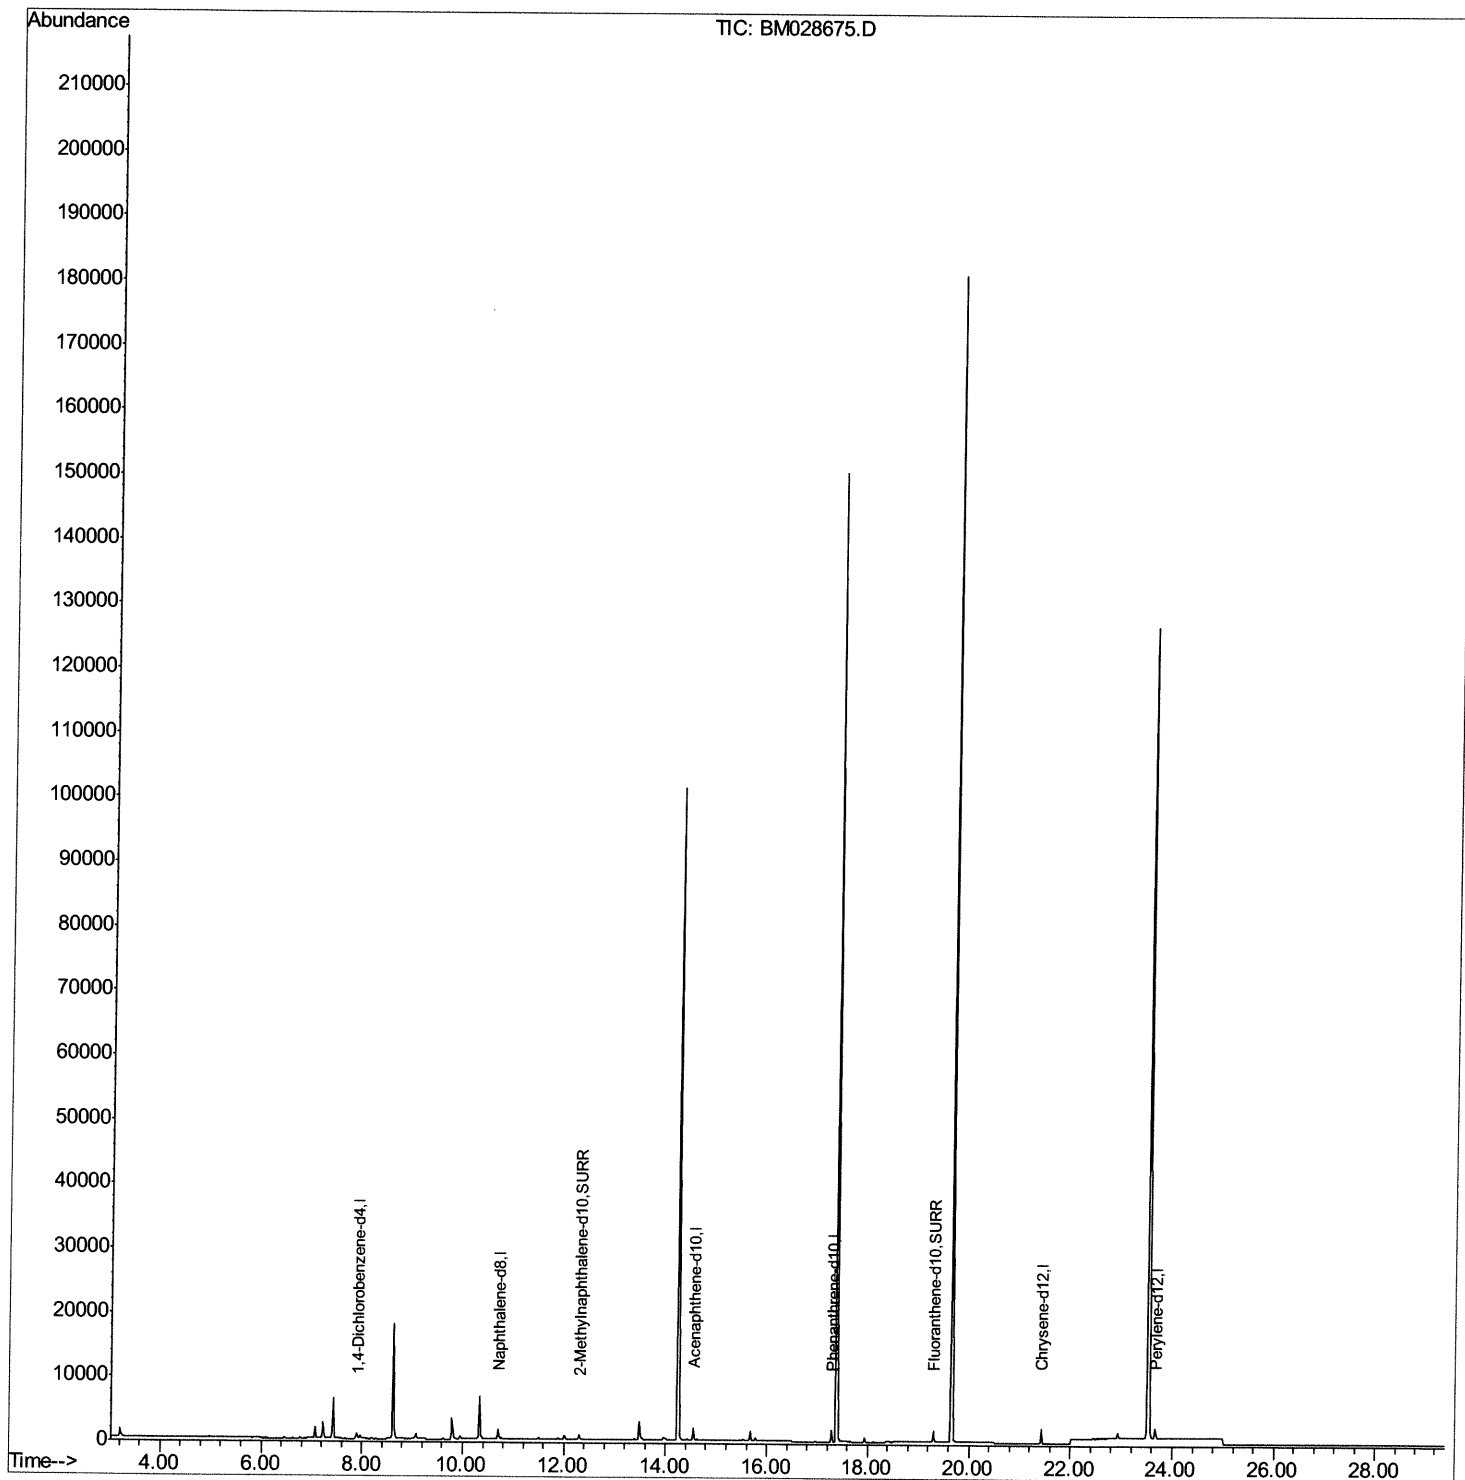

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM020821\
 Data File : BM028675.D
 Acq On : 08 Feb 2021 15:34
 Operator : CG/JU
 Sample : M1311-04
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
ClientSampleId :
 C0A60

Manual Integrations
APPROVED

mohammad
 2/9/2021 2:11:50 PM

Quant Time: Feb 08 16:08:57 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM020521.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Feb 08 13:26:08 2021
 Response via : Initial Calibration

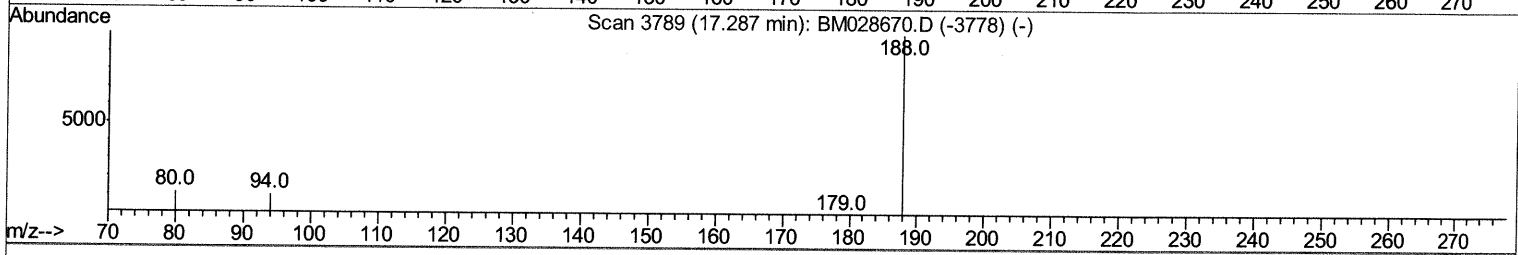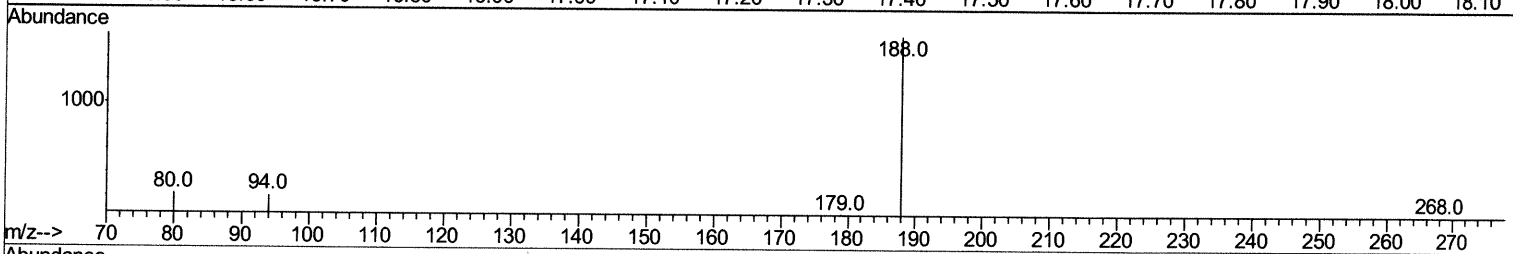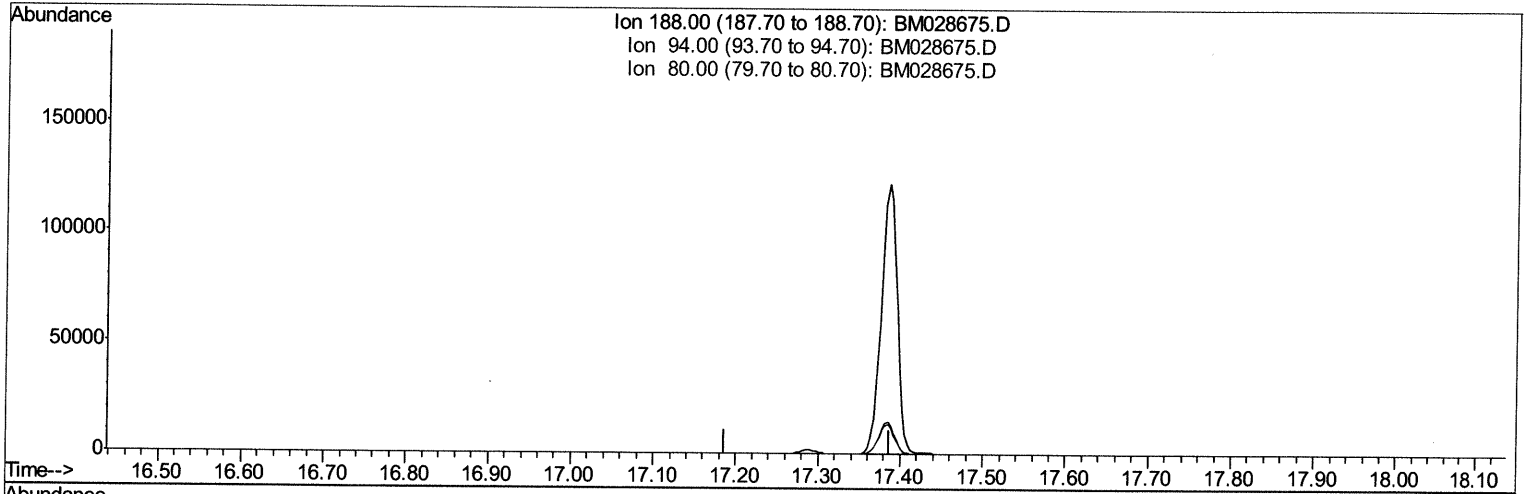

TIC: BM028675.D

(10) Phenanthrene-d10 (I)

17.287min (-17.287) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	13.50	0.00#
80.00	14.00	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM020821\
 Data File : BM028675.D
 Acq On : 08 Feb 2021 15:34
 Operator : CG/JU
 Sample : M1311-04
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
ClientSampleId :
 C0A60

Manual Integrations
APPROVED

mohammad
 2/9/2021 2:11:50 PM

Quant Time: Feb 08 16:08:57 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM020521.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Feb 08 13:26:08 2021
 Response via : Initial Calibration

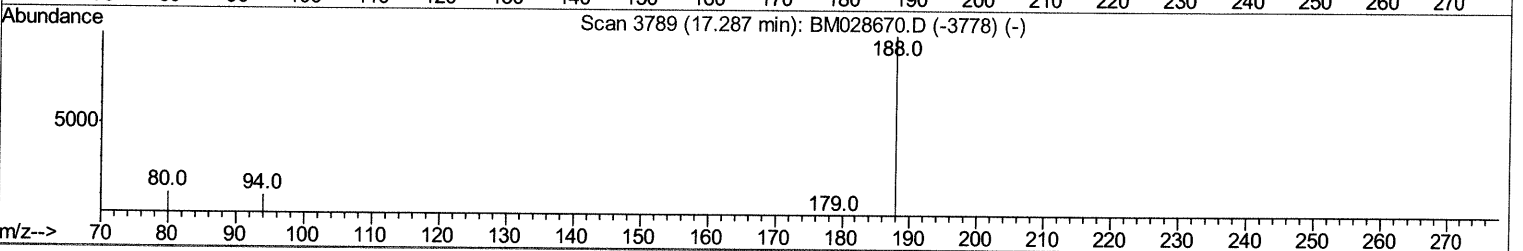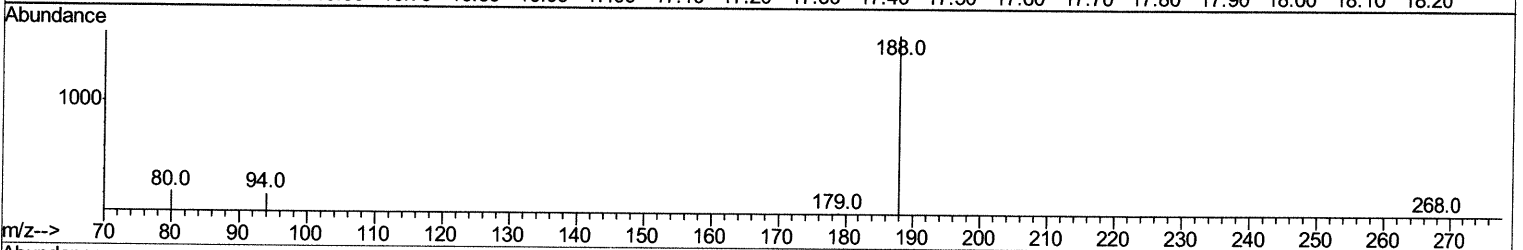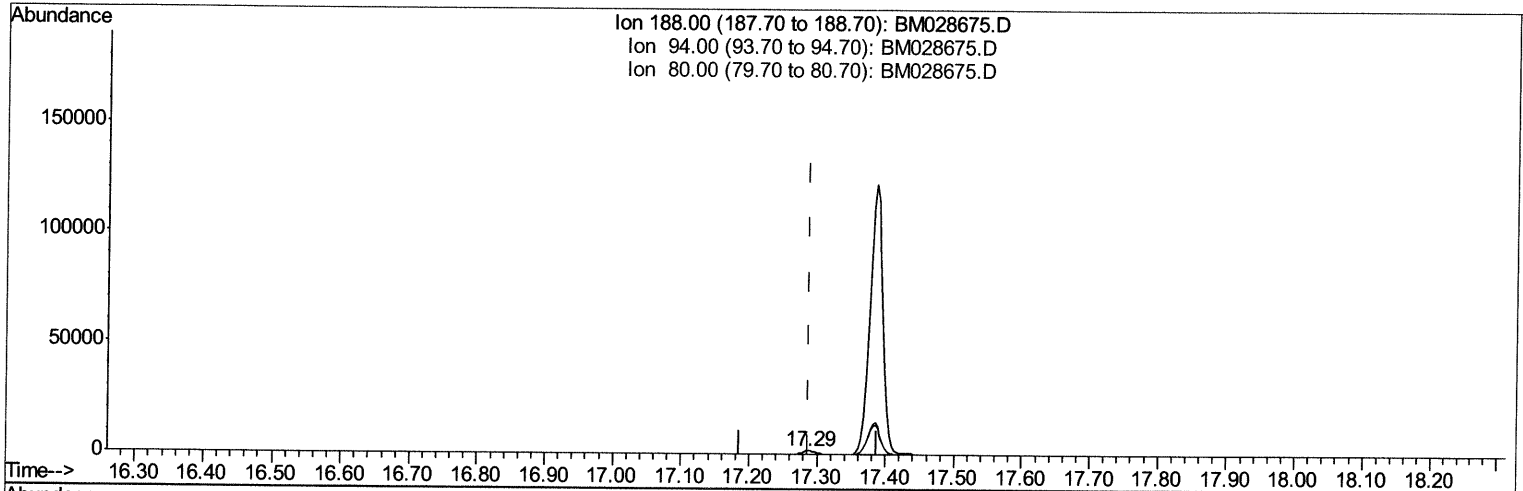

TIC: BM028675.D

(10) Phenanthrene-d10 (I)

17.287min (+0.000) 0.40ng/ul m 02/10/21 JU

response 2248

Ion	Exp%	Act%
188.00	100	100
94.00	13.50	12.52
80.00	14.00	13.46
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM020821\
 Data File : BM028675.D
 Acq On : 08 Feb 2021 15:34
 Operator : CG/JU
 Sample : M1311-04
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0A60

Manual Integrations
 APPROVED

mohammad
 2/9/2021 2:11:50 PM

Quant Time: Feb 08 16:10:00 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM020521.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Feb 08 13:26:08 2021
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.91	152	470	0.40	ng/ul	0.00
2) Naphthalene-d8	10.71	136	1930	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.55	164	1124	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.29	188	2248m>	0.40	ng/ul>	0.00002/0.02134
16) Chrysene-d12	21.43	240	1911	0.40	ng/ul	0.00
20) Perylene-d12	23.67	264	1955	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.30	152	985	0.36	ng/ul	0.00
14) Fluoranthene-d10	19.30	212	1981	0.34	ng/ul	0.00

Target Compounds Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed