


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM020821\
 Data File : BM028669.D
 Acq On : 08 Feb 2021 11:55
 Operator : CG/JU
 Sample : DFTPP24
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP24

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM020521.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Feb 08 13:26:08 2021

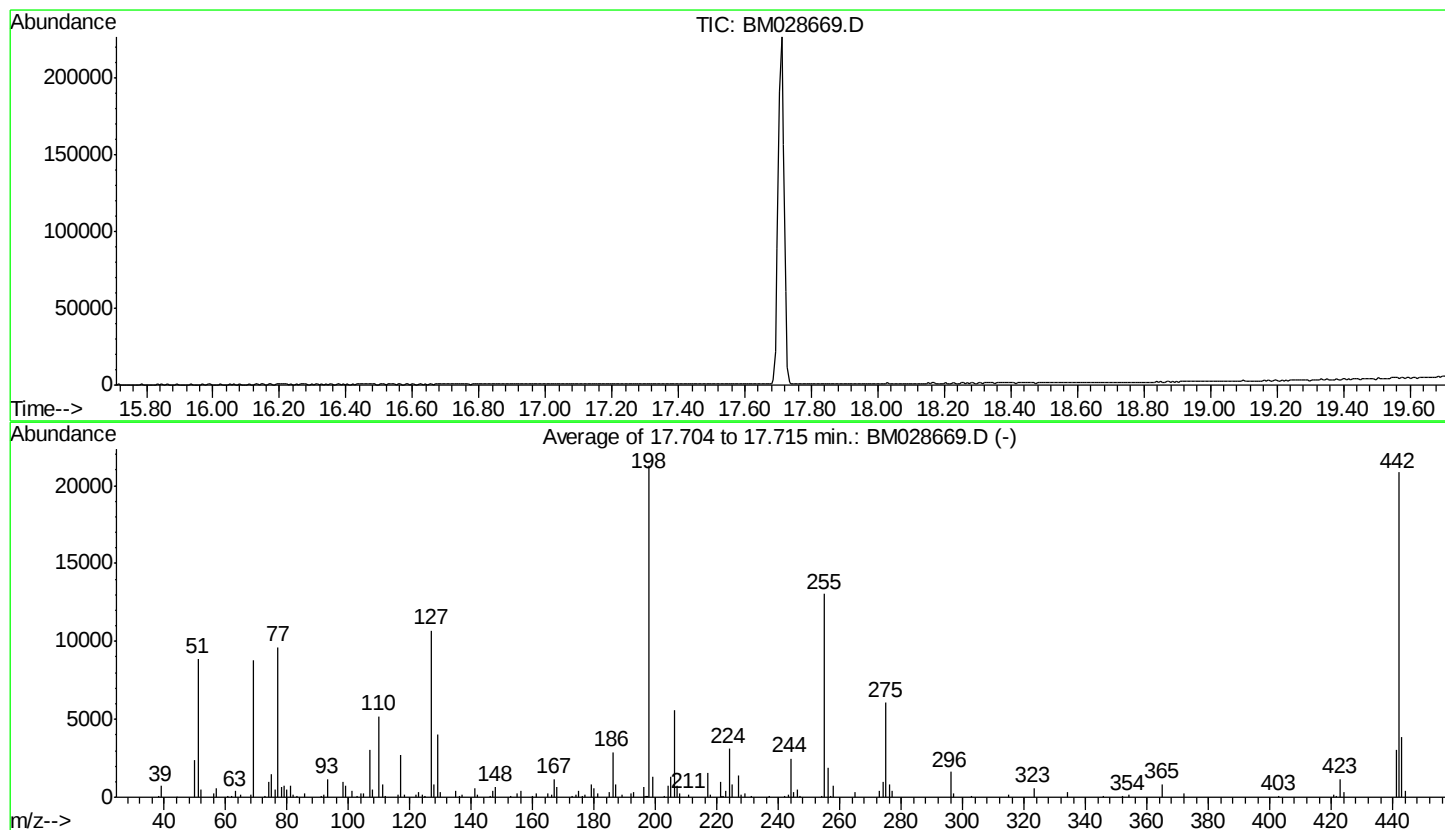

AutoFind: Scans 2468, 2469, 2470; Background Corrected with Scan 2462

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.9	8912	PASS
68	69	0.00	2	1.5	136	PASS
69	198	0.00	100	41.5	8824	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	50.3	10702	PASS
197	198	0.00	2	0.5	98	PASS
198	198	100	100	100.0	21285	PASS
199	198	5	9	6.4	1356	PASS
275	198	10	60	28.4	6043	PASS
365	198	1	100	3.9	825	PASS
441	198	0.01	100	14.3	3035	PASS
442	198	50	100	97.9	20845	PASS
443	442	15	24	18.5	3851	PASS

Scan 2462 (17.668 min): BM028669.D
DFTPP24

m/z	Abundance
43.90	484.0
73.00	155.0
207.00	328.0

Instrument :
BNA_M
ClientSampleId :
DFTPP24

m/z	Abundance
39.00	806.0
43.90	497.0
50.00	2685.0
51.10	10310.0
52.00	505.0
55.90	304.0
57.00	674.0
60.90	167.0
62.00	170.0
63.00	409.0
65.00	209.0
68.00	186.0
69.00	9764.0
73.00	196.0
74.10	1040.0
75.00	1670.0
76.00	540.0
77.10	10546.0
78.00	736.0
79.00	774.0
80.00	552.0
81.00	908.0
82.00	209.0
83.00	180.0
85.90	229.0
91.00	156.0
91.90	178.0
93.00	1207.0
98.00	982.0
99.00	790.0
101.00	400.0
103.00	155.0
104.00	312.0
105.00	296.0
107.00	3402.0
108.00	596.0
110.00	5621.0
111.00	902.0
116.00	156.0
117.00	2870.0
118.00	197.0
121.90	208.0
123.00	330.0
123.90	154.0
127.00	11286.0
128.00	849.0
129.00	4364.0
130.00	411.0
134.90	382.0
137.00	198.0
141.00	647.0
141.90	227.0
147.00	451.0
147.90	713.0
152.90	161.0
155.00	282.0
156.00	470.0
159.90	161.0
161.00	251.0
165.00	212.0
166.00	177.0
167.00	1256.0
168.00	719.0
174.00	255.0
175.00	436.0
177.00	232.0
178.90	786.0
180.00	628.0
180.90	253.0
185.00	376.0
186.00	2836.0
187.00	782.0
188.90	201.0
191.90	314.0
193.00	302.0
196.00	650.0
197.00	251.0
198.00	21608.0
199.00	1317.0
204.00	874.0
205.00	1285.0
206.10	5649.0
207.00	1128.0
208.00	278.0
211.00	211.0
217.00	1563.0
218.00	210.0
220.90	927.0
222.90	375.0
224.00	3265.0
225.00	942.0
227.00	1340.0

Instrument :
BNA_M
ClientSampleId :
DFTPP24

228.00	166.0
229.00	251.0
241.90	173.0
243.00	209.0
244.00	2361.0
245.00	305.0
246.00	516.0
254.10	153.0
255.00	12424.0
256.00	1857.0
257.00	161.0
258.00	734.0
264.90	321.0
272.90	348.0
274.00	970.0
275.00	5523.0
276.00	846.0
276.90	380.0
296.00	1608.0
296.90	213.0
314.90	266.0
323.00	520.0
334.00	311.0
365.00	743.0
372.00	210.0
423.00	895.0
424.00	287.0
441.00	2332.0
442.00	16081.0
443.00	3172.0
444.00	344.0

Instrument :
BNA_M
ClientSampleId :
DFTPP24

m/z	Abundance
38.00	161.0
39.00	810.0
44.00	484.0
50.00	2867.0
51.10	10164.0
52.00	531.0
55.90	263.0
57.00	697.0
60.90	187.0
62.00	167.0
63.00	441.0
65.00	182.0
68.00	223.0
69.00	10527.0
73.00	326.0
74.00	1018.0
75.00	1755.0
76.10	560.0
77.10	11311.0
78.00	772.0
79.00	844.0
79.90	608.0
81.00	776.0
82.00	195.0
83.00	169.0
85.90	295.0
91.00	198.0
92.00	230.0
93.00	1450.0
98.00	1245.0
99.00	837.0
100.90	420.0
102.90	156.0
104.00	293.0
105.00	364.0
107.00	3447.0
107.90	571.0
110.00	6014.0
111.00	1086.0
111.90	151.0
116.00	228.0
117.00	3224.0
118.00	230.0
121.90	216.0
123.00	345.0
123.90	209.0
124.90	166.0
127.00	12491.0
127.90	1000.0
129.00	4592.0
130.00	419.0
135.00	449.0
136.00	170.0
136.90	256.0
141.00	683.0
142.00	210.0
146.00	195.0
147.00	386.0
148.00	853.0
153.00	193.0
155.00	353.0
156.00	532.0
160.00	177.0
161.00	283.0
165.00	253.0
166.00	252.0
167.00	1357.0
168.00	635.0
173.00	182.0
173.90	326.0
175.00	515.0
176.00	159.0
176.90	234.0
178.90	1061.0
180.00	719.0
180.90	323.0
185.00	440.0
186.00	3411.0
187.00	1044.0
188.90	319.0
192.00	295.0
193.00	447.0
196.00	771.0
197.20	296.0
198.00	25120.0
198.90	1618.0
202.90	205.0
204.00	918.0
205.00	1509.0
206.10	6589.0
207.00	1124.0
207.90	248.0

Instrument :
BNA_M
ClientSampleId :
DFTPP24

210.90	214.0
217.00	1876.0
218.00	224.0
221.00	1070.0
221.70	195.0
223.00	372.0
224.00	3557.0
225.00	969.0
227.00	1637.0
227.90	202.0
229.00	296.0
231.00	166.0
237.00	179.0
242.00	172.0
243.10	178.0
244.00	2918.0
245.00	466.0
246.00	563.0
246.90	164.0
255.00	15308.0
256.00	2205.0
256.90	201.0
258.00	886.0
264.90	343.0
273.00	529.0
274.00	1106.0
275.00	7051.0
276.00	897.0
276.90	569.0
296.00	1875.0
296.90	275.0
302.90	180.0
314.90	199.0
323.00	743.0
333.90	406.0
345.90	168.0
352.00	192.0
354.00	245.0
364.90	1035.0
372.00	344.0
403.00	187.0
420.90	245.0
421.80	191.0
423.00	1384.0
424.00	435.0
441.00	3459.0
442.00	24528.0
443.00	4401.0
443.90	373.0

Instrument :
BNA_M
ClientSampleId :
DFTPP24

m/z	Abundance
39.00	583.0
43.90	489.0
50.00	1680.0
51.00	6263.0
52.00	334.0
56.00	212.0
57.00	425.0
63.00	276.0
69.00	6182.0
72.90	207.0
74.00	831.0
75.00	1064.0
76.00	322.0
77.10	6988.0
78.10	441.0
79.00	544.0
80.00	360.0
81.00	516.0
86.00	173.0
91.90	155.0
93.00	898.0
98.00	637.0
98.90	515.0
101.00	308.0
103.90	166.0
104.90	193.0
107.00	2283.0
107.90	345.0
110.00	3908.0
111.00	579.0
116.00	159.0
117.00	2151.0
121.90	184.0
122.90	248.0
123.90	152.0
127.00	8330.0
128.00	590.0
129.00	3183.0
129.90	272.0
134.90	325.0
140.90	463.0
141.90	164.0
146.90	284.0
147.90	535.0
155.00	228.0
156.00	319.0
161.00	203.0
164.90	182.0
167.00	870.0
168.00	536.0
175.00	389.0
178.90	623.0
180.00	457.0
181.00	216.0
185.00	287.0
186.00	2466.0
187.00	584.0
192.00	230.0
193.00	300.0
196.00	584.0
196.70	156.0
198.00	17128.0
199.00	1133.0
204.00	539.0
205.00	1120.0
206.10	4523.0
207.00	992.0
207.90	298.0
210.80	167.0
217.00	1259.0
221.00	847.0
222.00	183.0
222.90	378.0
224.00	2519.0
225.00	572.0
227.00	1119.0
227.90	183.0
228.90	199.0
243.10	203.0
244.00	2137.0
245.00	272.0
246.00	462.0
255.00	11396.0
256.00	1549.0
258.00	687.0
264.90	276.0
273.00	333.0
274.00	823.0
275.00	5556.0
276.00	644.0
277.00	397.0
296.00	1384.0

Instrument :
BNA_M
ClientSampleId :
DFTPP24

297.00	166.0
303.00	164.0
323.10	500.0
334.00	345.0
354.00	219.0
365.00	699.0
372.00	217.0
402.90	153.0
420.80	206.0
423.00	1230.0
424.00	344.0
441.00	3316.0
442.00	21928.0
443.00	3980.0
444.00	413.0

Instrument :
BNA_M
ClientSampleId :
DFTPP24