

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020823\
 Data File : BM038712.D
 Acq On : 08 Feb 2023 09:51
 Operator : CG/JU
 Sample : PB150699BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK699

Quant Time: Feb 08 23:55:20 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM020723.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Feb 07 14:57:50 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.908	152	1726	0.400	ng/ul	0.00
4) Naphthalene-d8	10.713	136	4851	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.546	164	3828	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.291	188	7682	0.400	ng/ul	0.00
17) Chrysene-d12	21.469	240	5179	0.400	ng/ul	0.00
23) Perylene-d12	23.848	264	6789	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.284	96	9498	5.212	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.308	152	2215	0.263	ng/ul	0.00
18) Fluoranthene-d10	19.315	212	4460	0.295	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.536	166	1006	0.068	ng/ul#	16
20) Pyrene	19.678	202	963	0.044	ng/ul#	1
26) Benzo(a)pyrene	23.690	252	1948	0.089	ng/ul#	46


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020823\
Data File : BM038712.D
Acq On : 08 Feb 2023 09:51
Operator : CG/JU
Sample : PB150699BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK699

Quant Time: Feb 08 23:55:20 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM020723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 07 14:57:50 2023
Response via : Initial Calibration




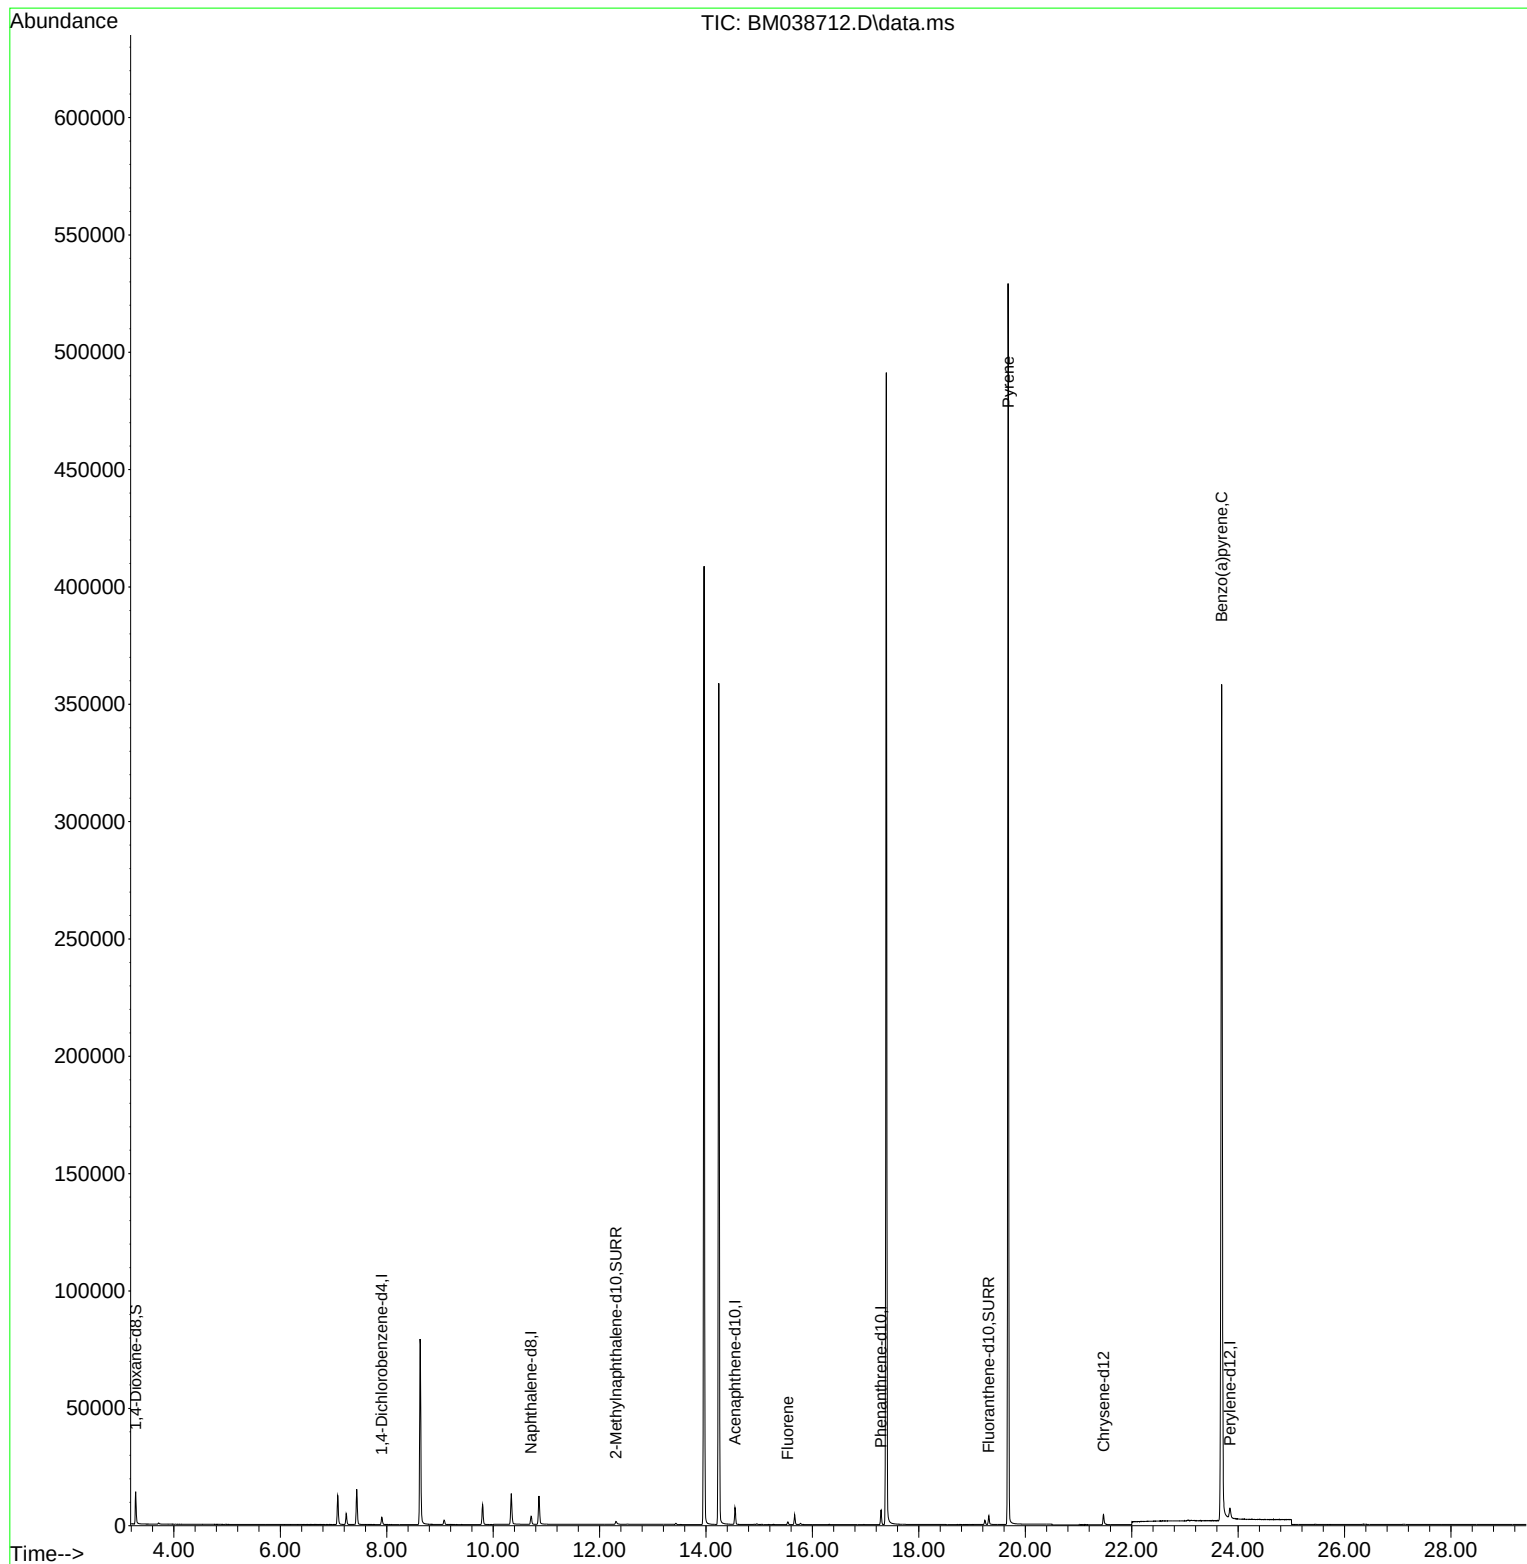


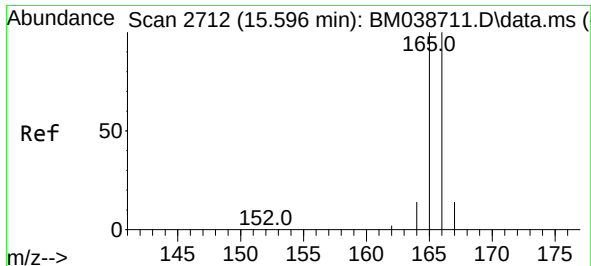

#12
Fluorene
Concen: 0.068 ng/ul
RT: 15.536 min Scan# 20
Delta R.T. -0.060 min
Lab File: BM038712.D
Acq: 08 Feb 2023 09:51




Instrument :
BNA_M
ClientSampleId :
SBLK699


Tgt Ion:166 Resp: 1006
Ion Ratio Lower Upper
166 100
165 9.6 80.7 121.1#
167 31.5 11.8 17.6#

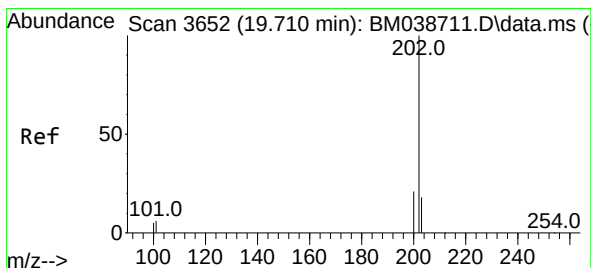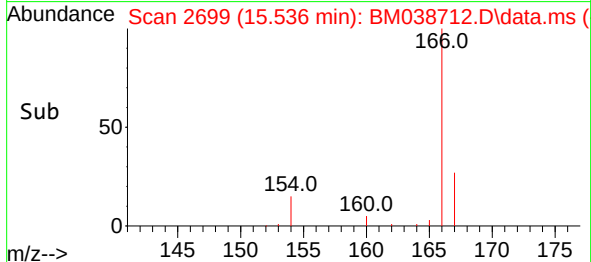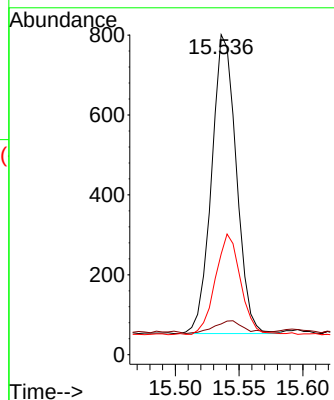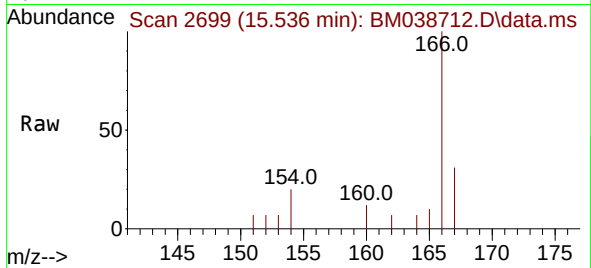

#20
Pyrene
Concen: 0.044 ng/ul
RT: 19.678 min Scan# 3645
Delta R.T. -0.032 min
Lab File: BM038712.D
Acq: 08 Feb 2023 09:51


Tgt Ion:202 Resp: 963
Ion Ratio Lower Upper
202 100
101 126.2 6.2 9.2#
100 982.4 5.2 7.8#

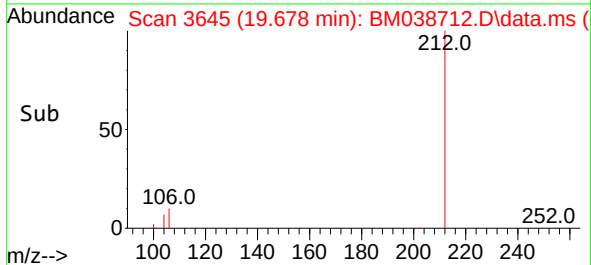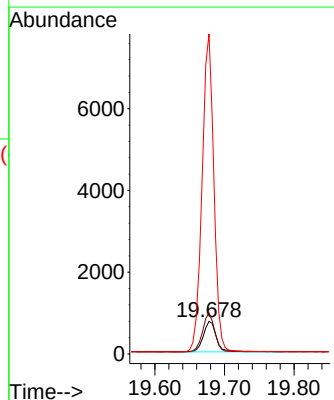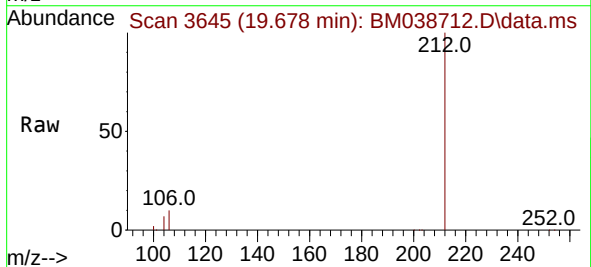

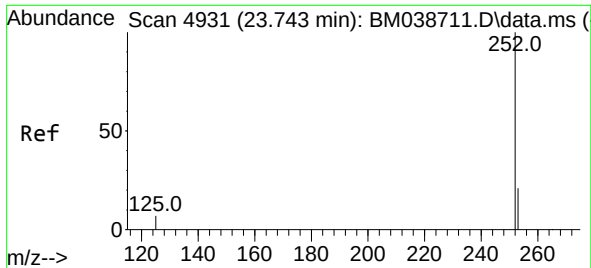

#26
Benzo(a)pyrene
Concen: 0.089 ng/ul
RT: 23.690 min Scan# 4931
Delta R.T. -0.055 min
Lab File: BM038712.D
Acq: 08 Feb 2023 09:51

Instrument :
BNA_M
ClientSampleId :
SBLK699

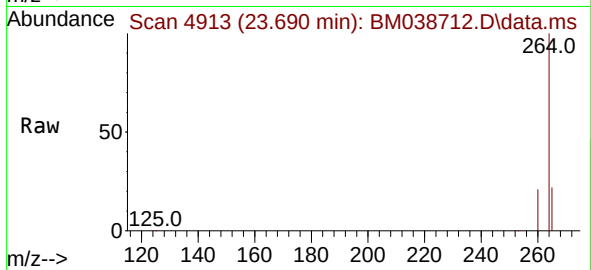

Tgt Ion:252 Resp: 1948
Ion Ratio Lower Upper
252 100
253 58.6 25.2 37.8#
125 40.5 11.4 17.0#

