

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020823\
 Data File : BM038717.D
 Acq On : 08 Feb 2023 12:56
 Operator : CG/JU
 Sample : 01422-11
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0B73

Quant Time: Feb 08 23:56:26 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM020723.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Feb 07 14:57:50 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.912	152	2132	0.400	ng/ul	0.00
4) Naphthalene-d8	10.713	136	6305	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.546	164	5124	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.291	188	10236	0.400	ng/ul	0.00
17) Chrysene-d12	21.472	240	6565	0.400	ng/ul	0.00
23) Perylene-d12	23.848	264	7570	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.284	96	7824	3.475	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.308	152	3434	0.314	ng/ul	0.00
18) Fluoranthene-d10	19.315	212	7288	0.380	ng/ul	0.00
Target Compounds						Qvalue
12) Fluorene	15.540	166	1429	0.072	ng/ul#	14
20) Pyrene	19.678	202	1270	0.046	ng/ul#	1
26) Benzo(a)pyrene	23.690	252	2155	0.088	ng/ul#	44


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020823\
Data File : BM038717.D
Acq On : 08 Feb 2023 12:56
Operator : CG/JU
Sample : 01422-11
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0B73

Quant Time: Feb 08 23:56:26 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM020723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 07 14:57:50 2023
Response via : Initial Calibration




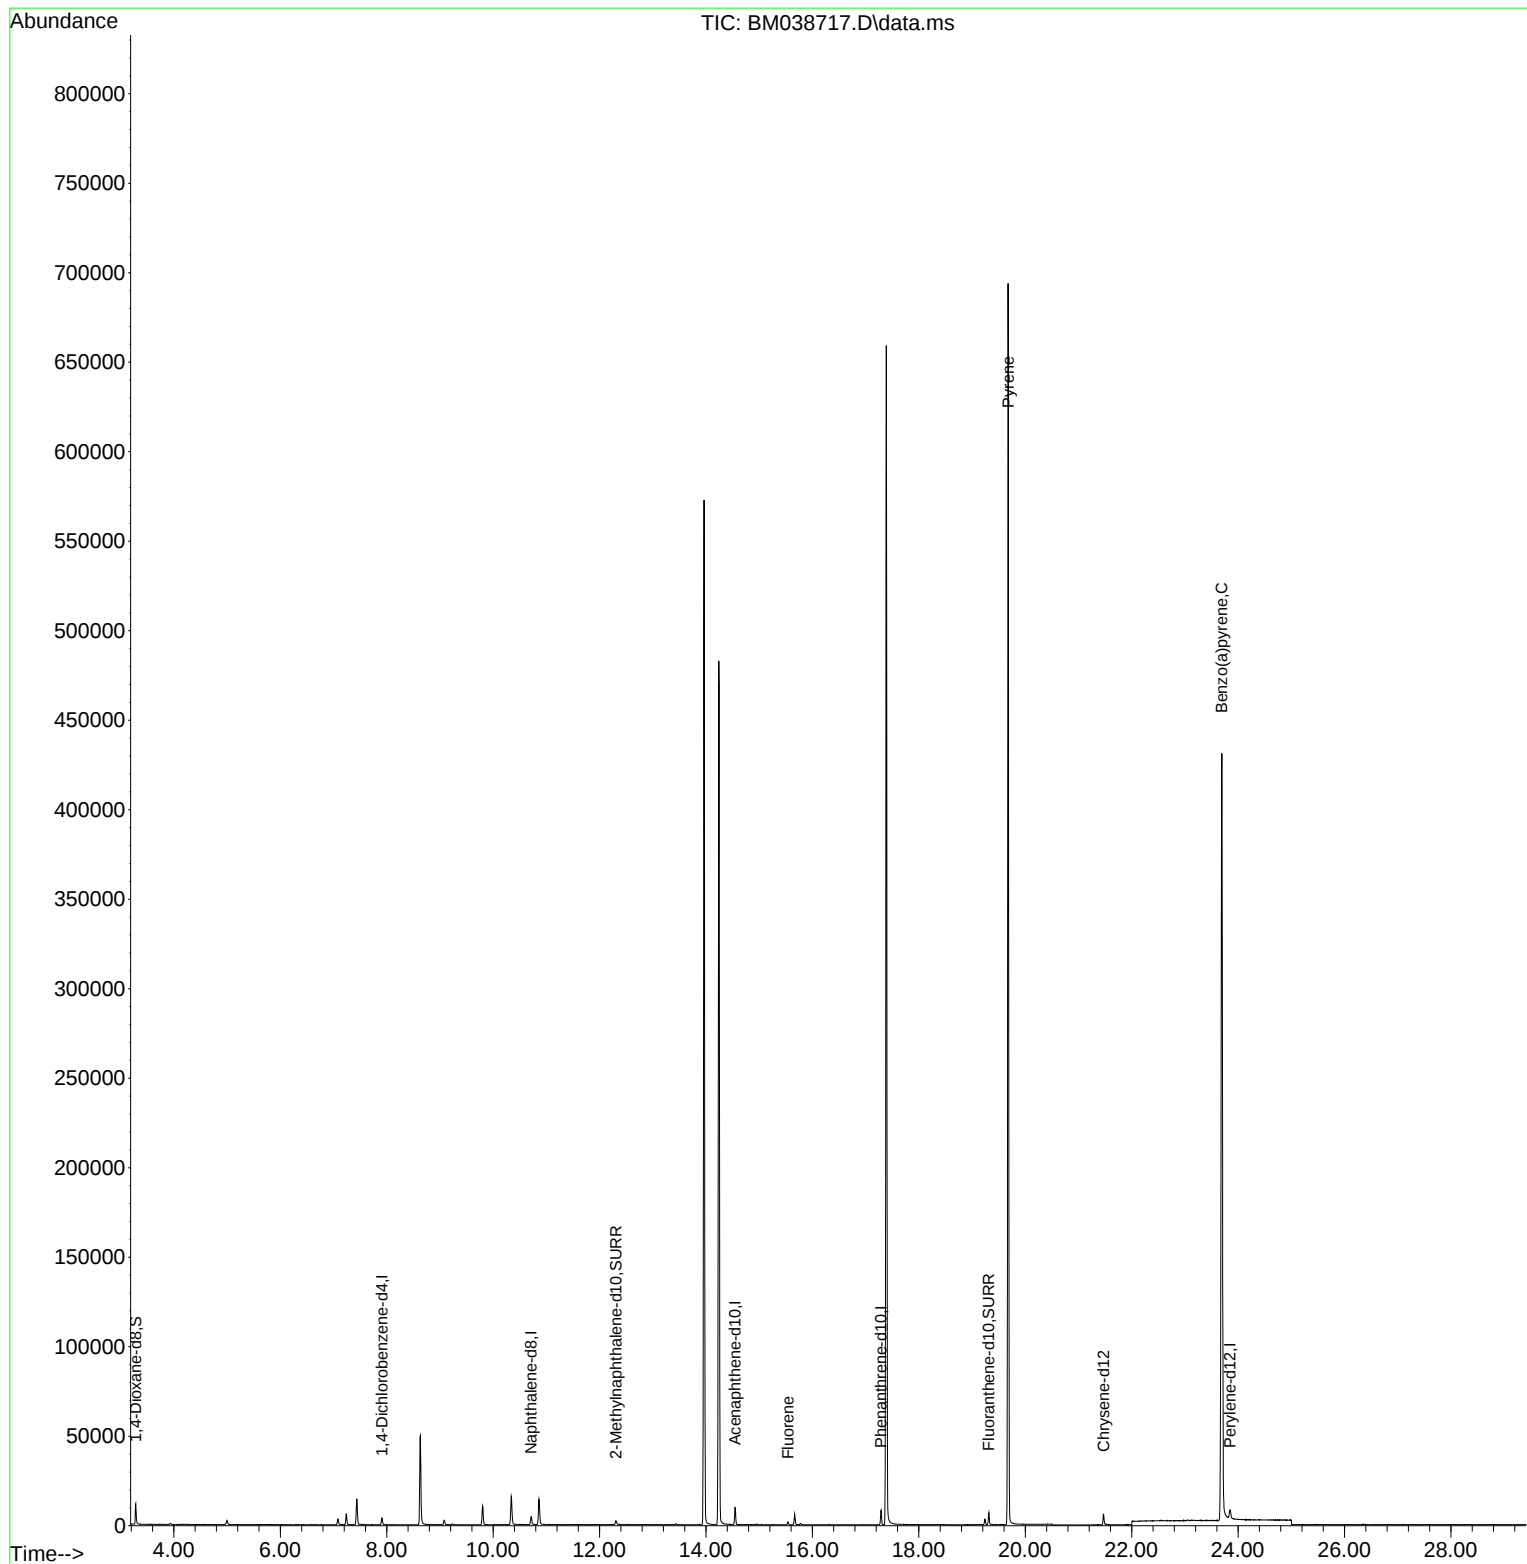


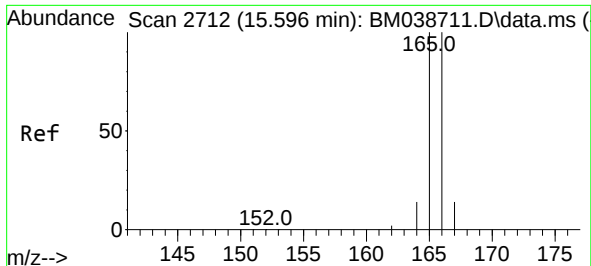

#12
 Fluorene
 Concen: 0.072 ng/ul
 RT: 15.540 min Scan# 21
 Delta R.T. -0.055 min
 Lab File: BM038717.D
 Acq: 08 Feb 2023 12:56




Instrument :
 BNA_M
 ClientSampleId :
 C0B73


Tgt Ion:166 Resp: 1429
 Ion Ratio Lower Upper
 166 100
 165 9.3 80.7 121.1#
 167 34.2 11.8 17.6#

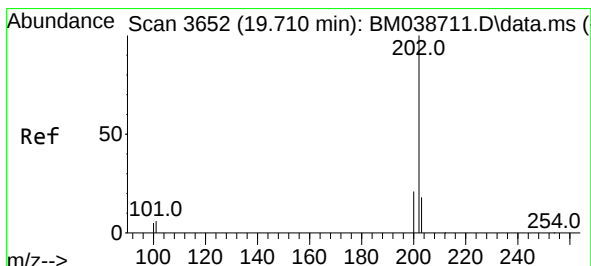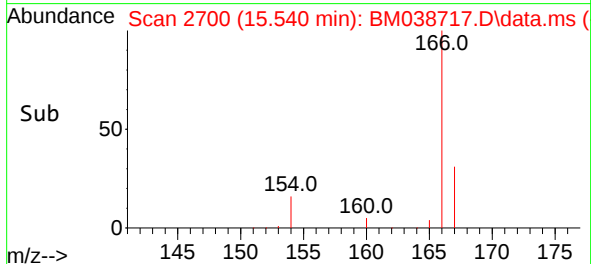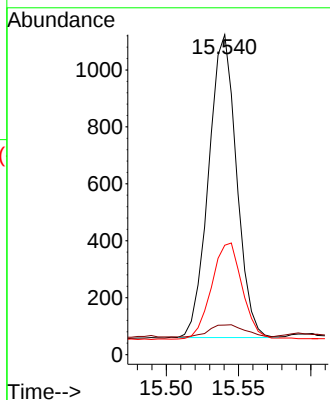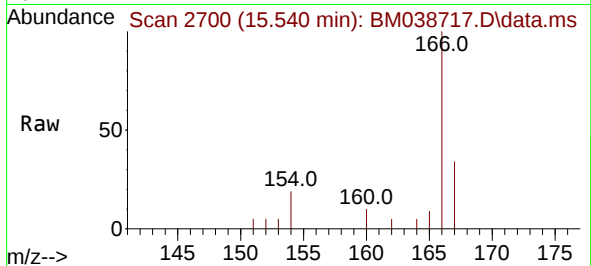

#20
 Pyrene
 Concen: 0.046 ng/ul
 RT: 19.678 min Scan# 3645
 Delta R.T. -0.032 min
 Lab File: BM038717.D
 Acq: 08 Feb 2023 12:56


Tgt Ion:202 Resp: 1270
 Ion Ratio Lower Upper
 202 100
 101 124.8 6.2 9.2#
 100 949.0 5.2 7.8#

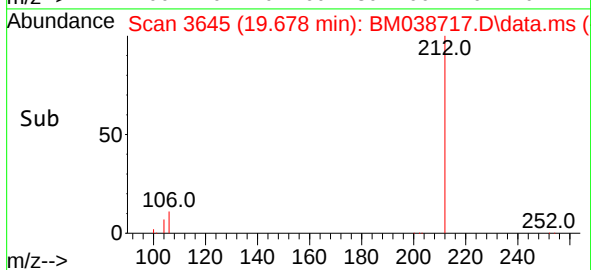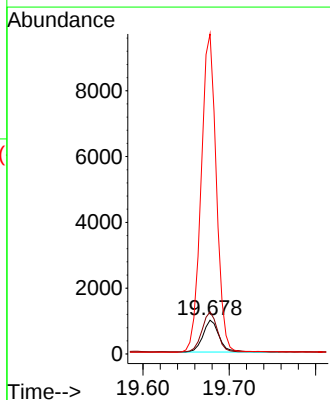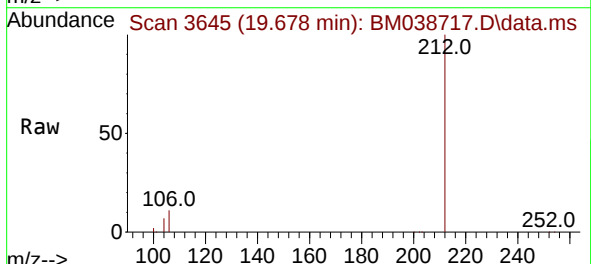

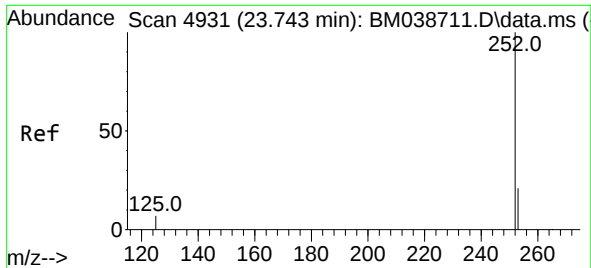

#26
Benzo(a)pyrene
Concen: 0.088 ng/ul
RT: 23.690 min Scan# 4913
Delta R.T. -0.055 min
Lab File: BM038717.D
Acq: 08 Feb 2023 12:56

Instrument :
BNA_M
ClientSampleId :
C0B73

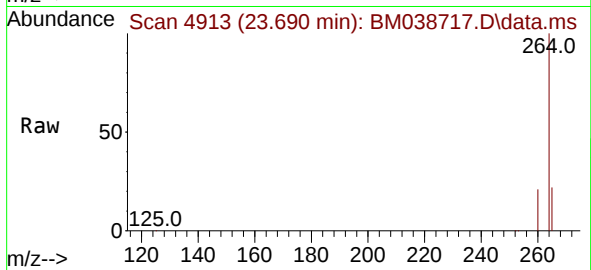

Tgt Ion:252 Resp: 2155
Ion Ratio Lower Upper
252 100
253 60.0 25.2 37.8#
125 41.7 11.4 17.0#

