

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020823\
 Data File : BM038713.D
 Acq On : 08 Feb 2023 10:28
 Operator : CG/JU
 Sample : 01422-01
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0B45

Quant Time: Feb 08 23:55:33 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM020723.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Feb 07 14:57:50 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.912	152	1583	0.400	ng/ul	0.00
4) Naphthalene-d8	10.713	136	4195	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.546	164	3013	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.291	188	5961	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.469	240	5804	0.400	ng/ul	0.00
23) Perylene-d12	23.845	264	8822	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.284	96	6400	3.829	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.308	152	1674	0.230	ng/ul	0.00
18) Fluoranthene-d10	19.315	212	4577	0.270	ng/ul	0.00
Target Compounds						
						Qvalue
5) Naphthalene	10.762	128	314	0.031	ng/ul#	55
15) Phenanthrene	17.333	178	516	0.029	ng/ul#	75


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020823\
Data File : BM038713.D
Acq On : 08 Feb 2023 10:28
Operator : CG/JU
Sample : 01422-01
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0B45

Quant Time: Feb 08 23:55:33 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM020723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 07 14:57:50 2023
Response via : Initial Calibration

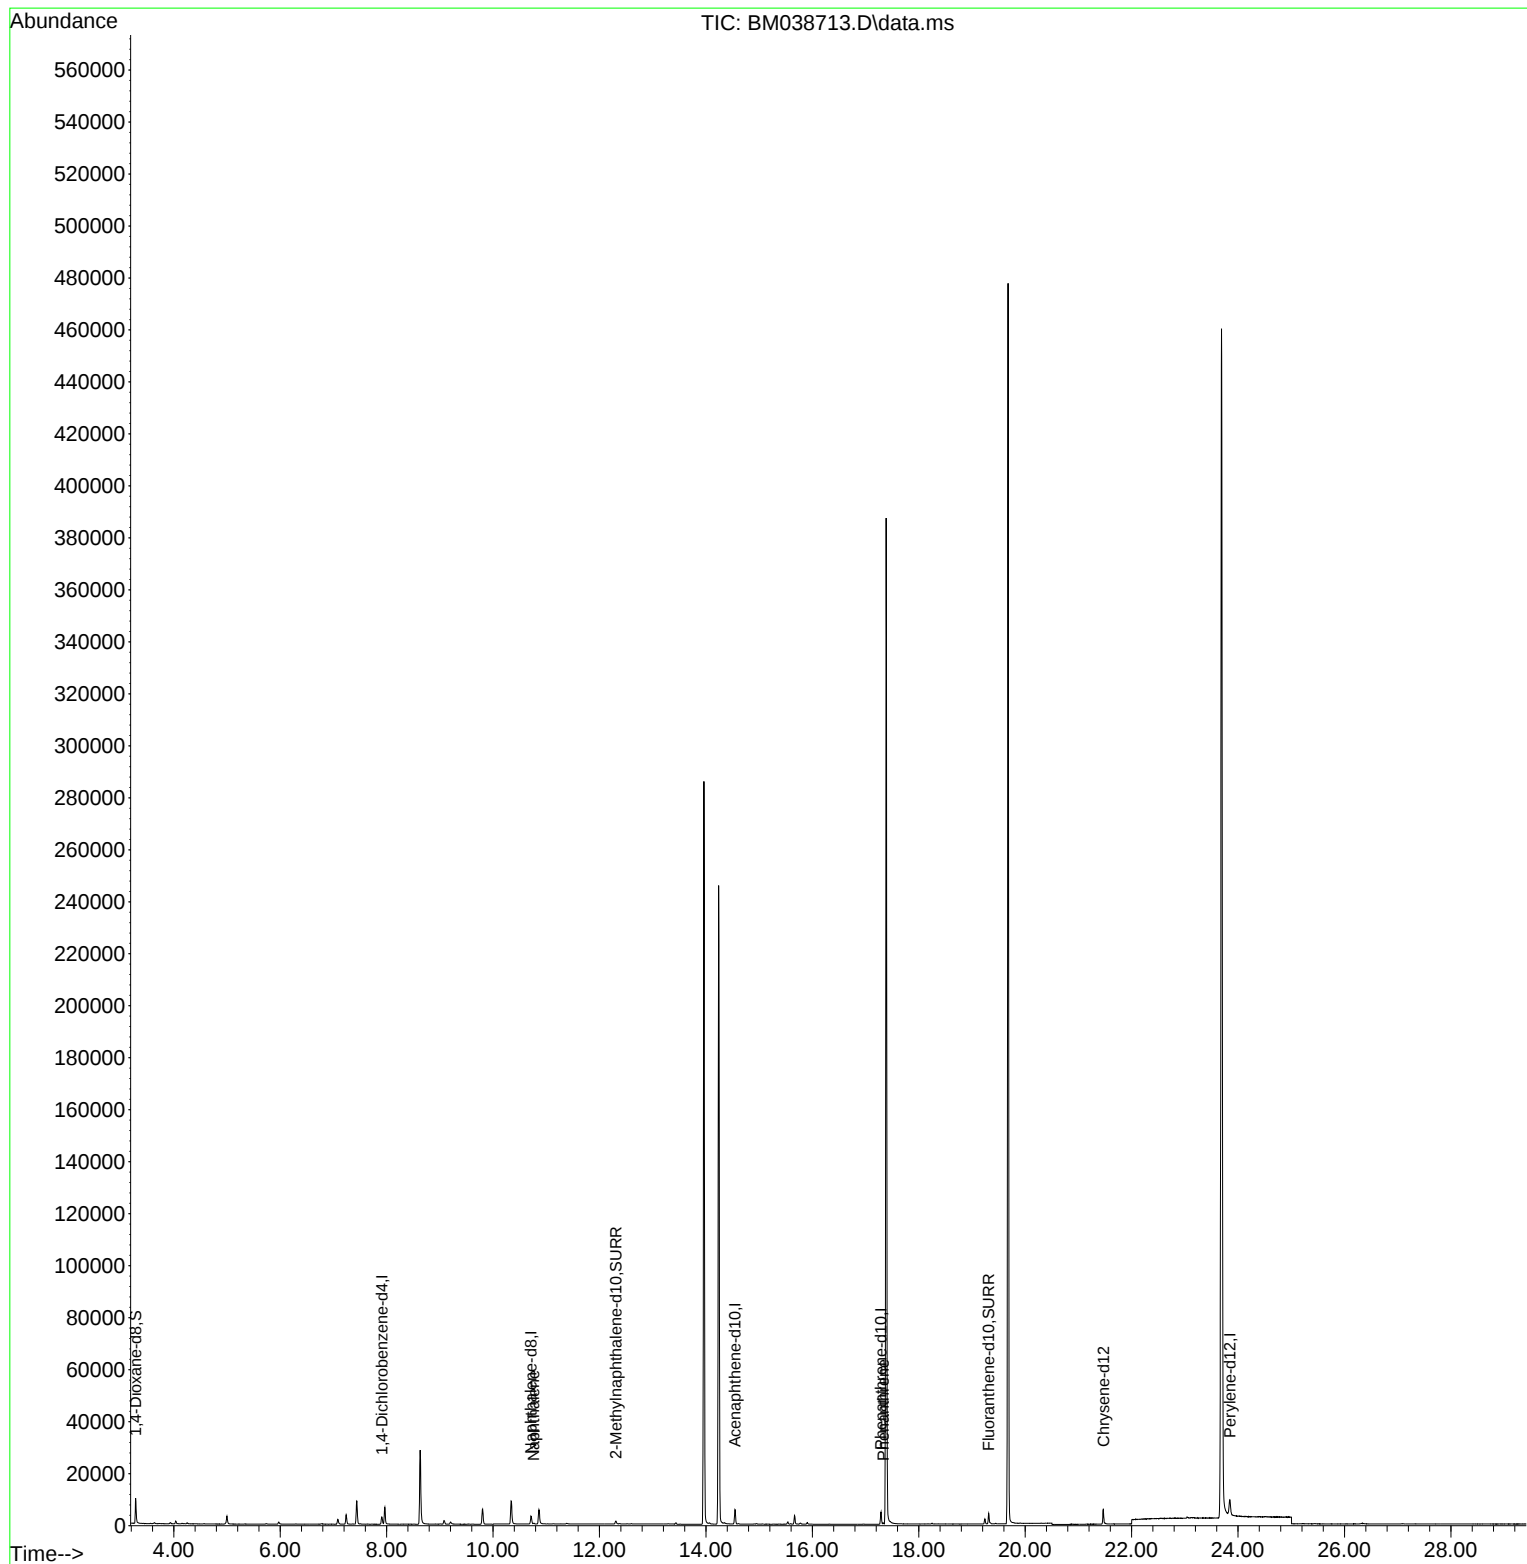

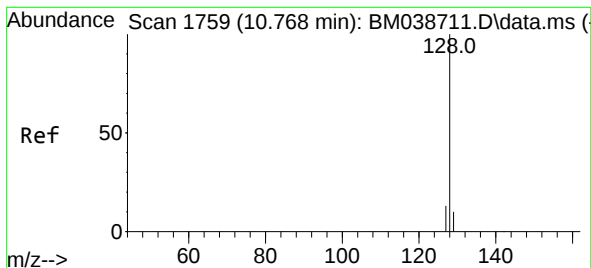

#5

Naphthalene

Concen: 0.031 ng/ul

RT: 10.762 min Scan# 1758

Delta R.T. -0.006 min

Lab File: BM038713.D

Acq: 08 Feb 2023 10:28

Instrument :

BNA_M

ClientSampleId :

C0B45





Tgt Ion:128 Resp: 314

Ion Ratio Lower Upper

128 100

129 31.2 10.2 15.4#

127 31.6 11.2 16.8#

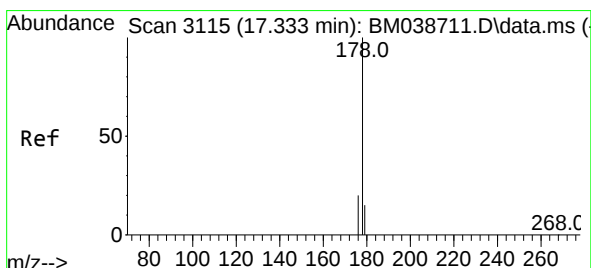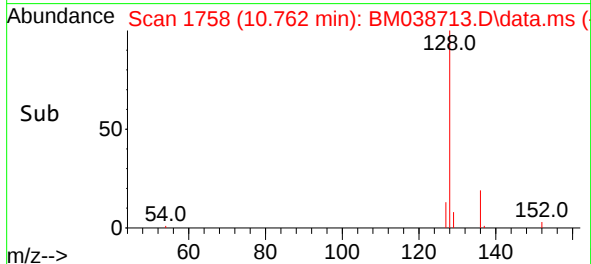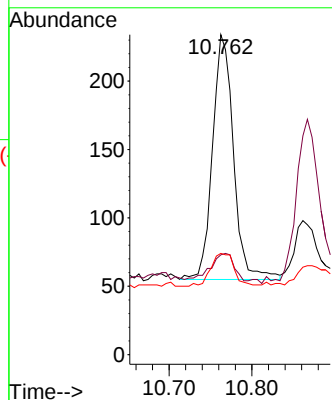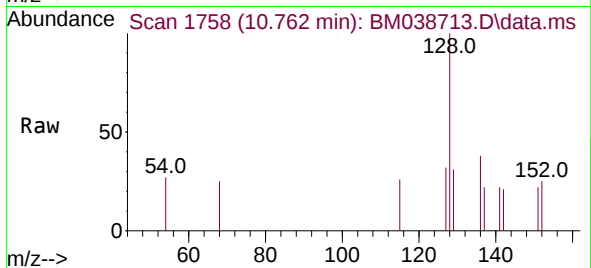

#15

Phenanthrene

Concen: 0.029 ng/ul

RT: 17.333 min Scan# 3115

Delta R.T. -0.000 min

Lab File: BM038713.D

Acq: 08 Feb 2023 10:28

Tgt Ion:178 Resp: 516

Ion Ratio Lower Upper

178 100

179 29.5 13.0 19.6#

176 30.4 16.5 24.7#

