

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM020921\
 Data File : BM028697.D
 Acq On : 09 Feb 2021 22:45
 Operator : CG/JU
 Sample : M1310-07
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0A41

Quant Time: Feb 10 01:27:32 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM011621MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Feb 09 23:51:34 2021
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.89	152	27700	20.00	ng/ul	0.00
18) Naphthalene-d8	10.70	136	109110	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.54	164	61344	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.28	188	125698	20.00	ng/ul	0.00
78) Chrysene-d12	21.43	240	126771	20.00	ng/ul	0.00
86) Perylene-d12	23.66	264	129291	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.20	96	3259	4.96	ng/uL	0.00
5) Phenol-d5	7.06	99	60356	25.52	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.23	67	34953	23.62	ng/ul	0.00
9) 2-Chlorophenol-d4	7.42	132	52780	25.74	ng/ul	0.00
13) 4-Methylphenol-d8	8.62	113	49141	25.73	ng/ul	0.00
19) Nitrobenzene-d5	9.07	128	24171	25.89	ng/ul	0.00
22) 2-Nitrophenol-d4	9.79	143	27313	26.79	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.33	165	47035	25.31	ng/ul	0.00
29) 4-Chloroaniline-d4	10.85	131	62895	29.08	ng/ul	0.00
44) Dimethylphthalate-d6	13.96	166	132384	27.18	ng/ul	0.00
47) Acenaphthylene-d8	14.24	160	174484	28.04	ng/ul	0.00
52) 4-Nitrophenol-d4	14.76	143	21677	23.75	ng/ul	0.00
58) Fluorene-d10	15.54	176	114013	27.08	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.67	200	18063	20.88	ng/ul	0.00
71) Anthracene-d10	17.38	188	175475	27.12	ng/ul	0.00
79) Pyrene-d10	19.66	212	189645	25.61	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.52	264	204399	27.86	ng/ul	0.00


Target Compounds					Ovalue	
6) Phenol	7.09	94	5365	2.280	ng/ul	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM020921\
Data File : BM028697.D
Acq On : 09 Feb 2021 22:45
Operator : CG/JU
Sample : M1310-07
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0A41

Quant Time: Feb 10 01:27:32 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM011621MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Feb 09 23:51:34 2021
Response via : Initial Calibration

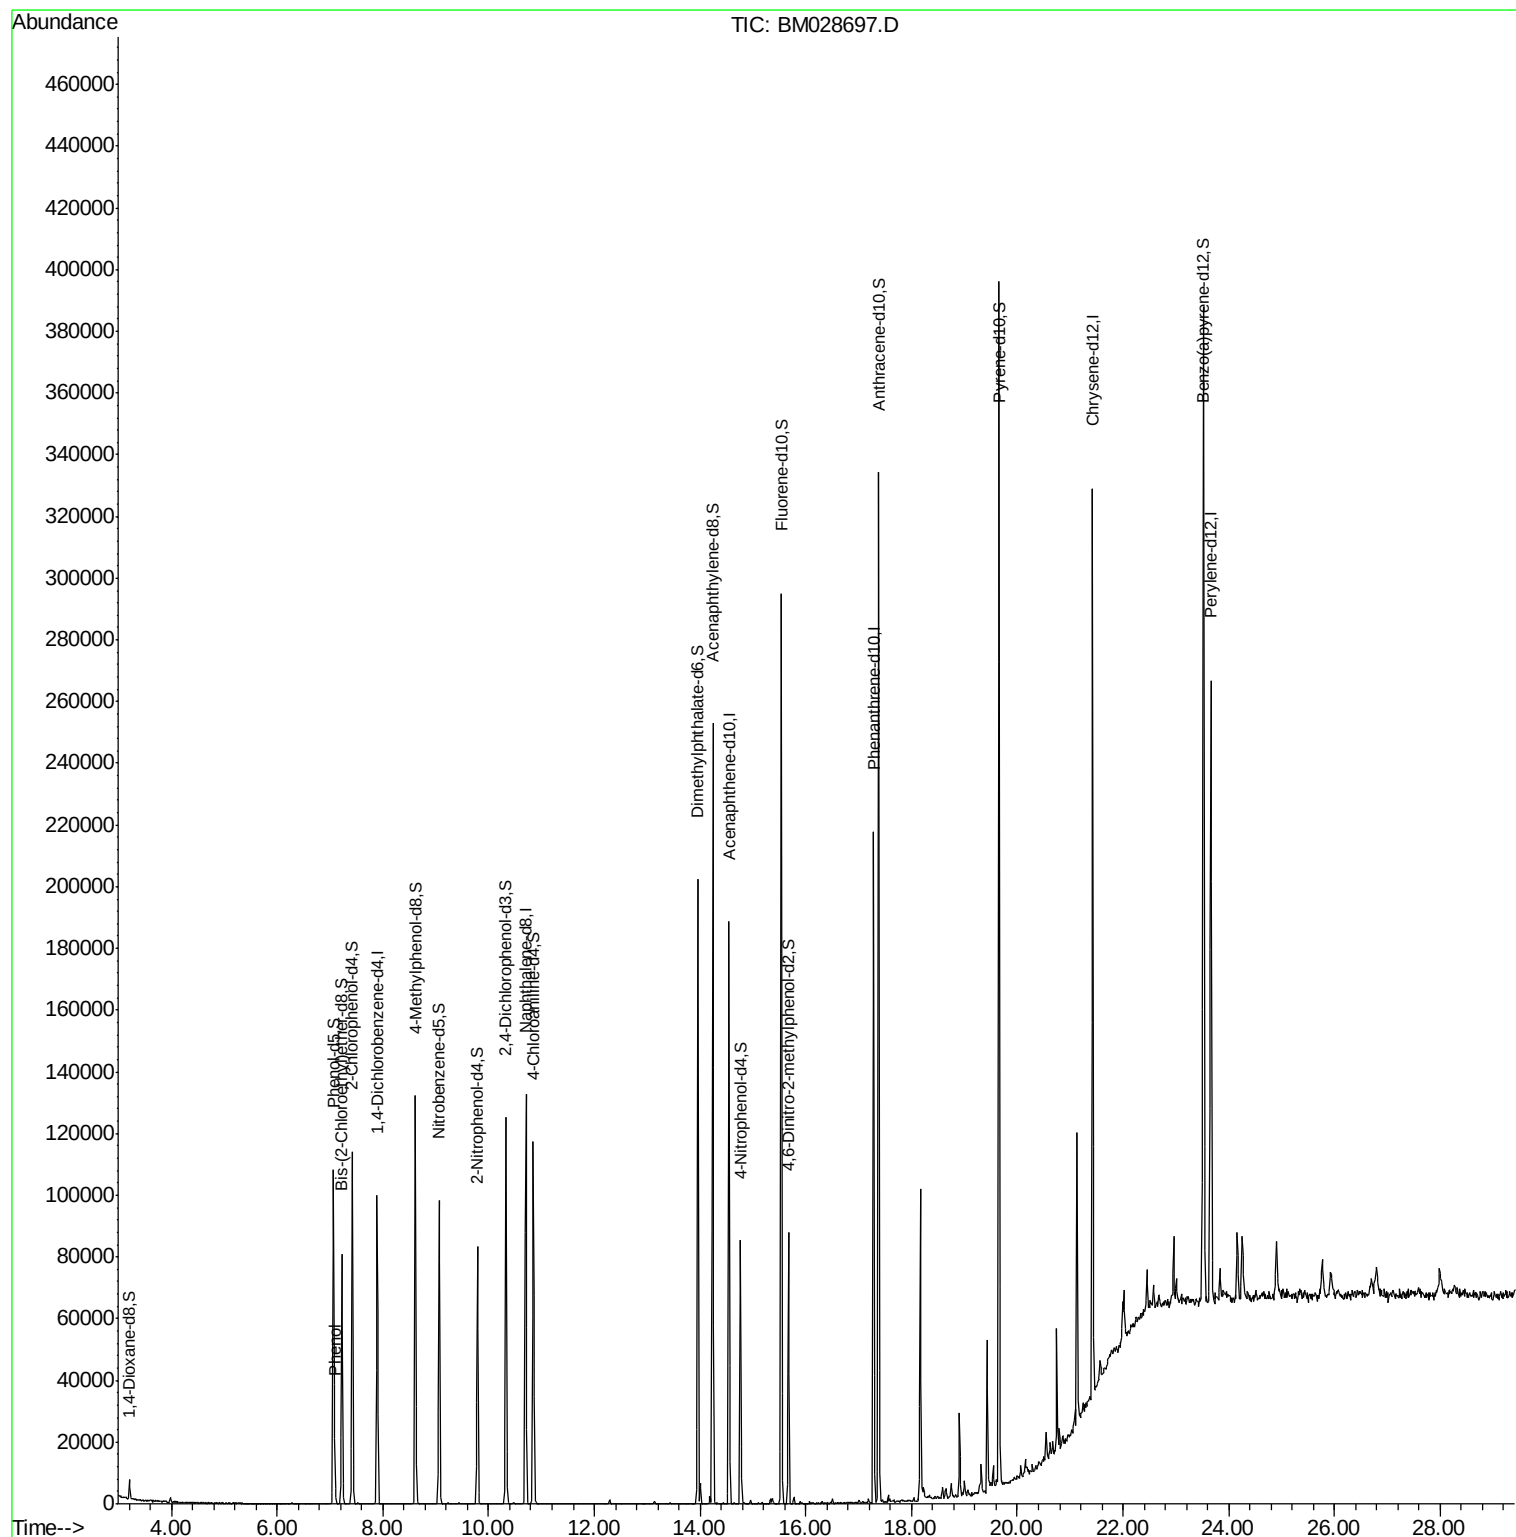

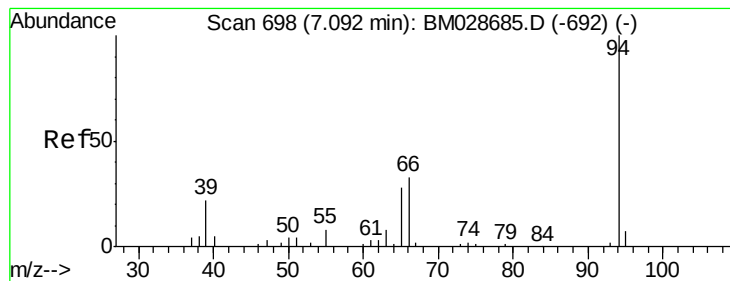

#6

Phenol

Concen: 2.280 ng/ul

RT: 7.09 min Scan# 698

Delta R.T. 0.00 min

Lab File: BM028697.D

Acq: 09 Feb 2021 22:45

Instrument :

BNA_M

ClientSampleId :

C0A41

Tot Ion: 94 Resp: 5365

Ion Ratio Lower Upper

94 100

65 27.8 25.6 38.4

66 39.8 33.0 49.4

