

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM020921\
 Data File : BM028680.D
 Acq On : 09 Feb 2021 10:33
 Operator : CG/JU
 Sample : PB134489BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK89

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM011621MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.204	33	37	44	rVB	7679	9445	1.58%	0.164%
2	3.981	167	169	172	rVB	904	921	0.15%	0.016%
3	7.063	688	693	706	rBB	113702	178585	29.93%	3.098%
4	7.228	715	721	731	rBB	89491	137362	23.02%	2.383%
5	7.422	749	754	764	rBB	119607	191075	32.02%	3.314%
6	7.892	828	834	842	rBB	73049	115238	19.31%	1.999%
7	8.616	951	957	969	rBB	139739	216295	36.25%	3.752%
8	9.069	1028	1034	1044	rBB	108059	169091	28.34%	2.933%
9	9.792	1151	1157	1164	rBV	89155	141611	23.73%	2.456%
10	10.333	1243	1249	1261	rBB	130950	216938	36.36%	3.763%
11	10.704	1305	1312	1320	rBB	101922	162047	27.16%	2.811%
12	10.845	1330	1336	1344	rBV	132967	218506	36.62%	3.790%
13	12.298	1579	1583	1586	rBB	1278	1767	0.30%	0.031%
14	13.957	1859	1865	1873	rVB	223421	302260	50.66%	5.243%
15	14.245	1907	1914	1920	rBV	267112	382150	64.05%	6.629%
16	14.545	1959	1965	1973	rVB2	136994	204955	34.35%	3.555%
17	14.762	1997	2002	2014	rBV	96794	140297	23.51%	2.434%
18	15.539	2128	2134	2141	rBV	327230	443386	74.31%	7.691%
19	15.668	2151	2156	2166	rBV	106279	135565	22.72%	2.351%
20	15.774	2170	2174	2179	rVB	2183	2336	0.39%	0.041%
21	17.280	2424	2430	2436	rBV	159403	226523	37.96%	3.929%
22	17.380	2441	2447	2456	rBV	344093	473608	79.37%	8.215%
23	18.856	2695	2698	2700	rBV2	426	623	0.10%	0.011%
24	19.297	2768	2773	2778	rBV2	3167	4482	0.75%	0.078%
25	19.421	2792	2794	2796	rBV2	821	742	0.12%	0.013%
26	19.550	2813	2816	2820	rVB	2742	2651	0.44%	0.046%
27	19.662	2828	2835	2843	rBV	406022	551649	92.45%	9.569%
28	21.427	3130	3135	3141	rBV	215005	267598	44.85%	4.642%
29	23.527	3485	3492	3500	rVB	336634	596672	100.00%	10.350%
30	23.668	3510	3516	3524	rVB2	148206	270834	45.39%	4.698%


Sum of corrected areas: 5765212

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM020921\
Data File : BM028680.D
Acq On : 09 Feb 2021 10:33
Operator : CG/JU
Sample : PB134489BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK89

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM011621MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

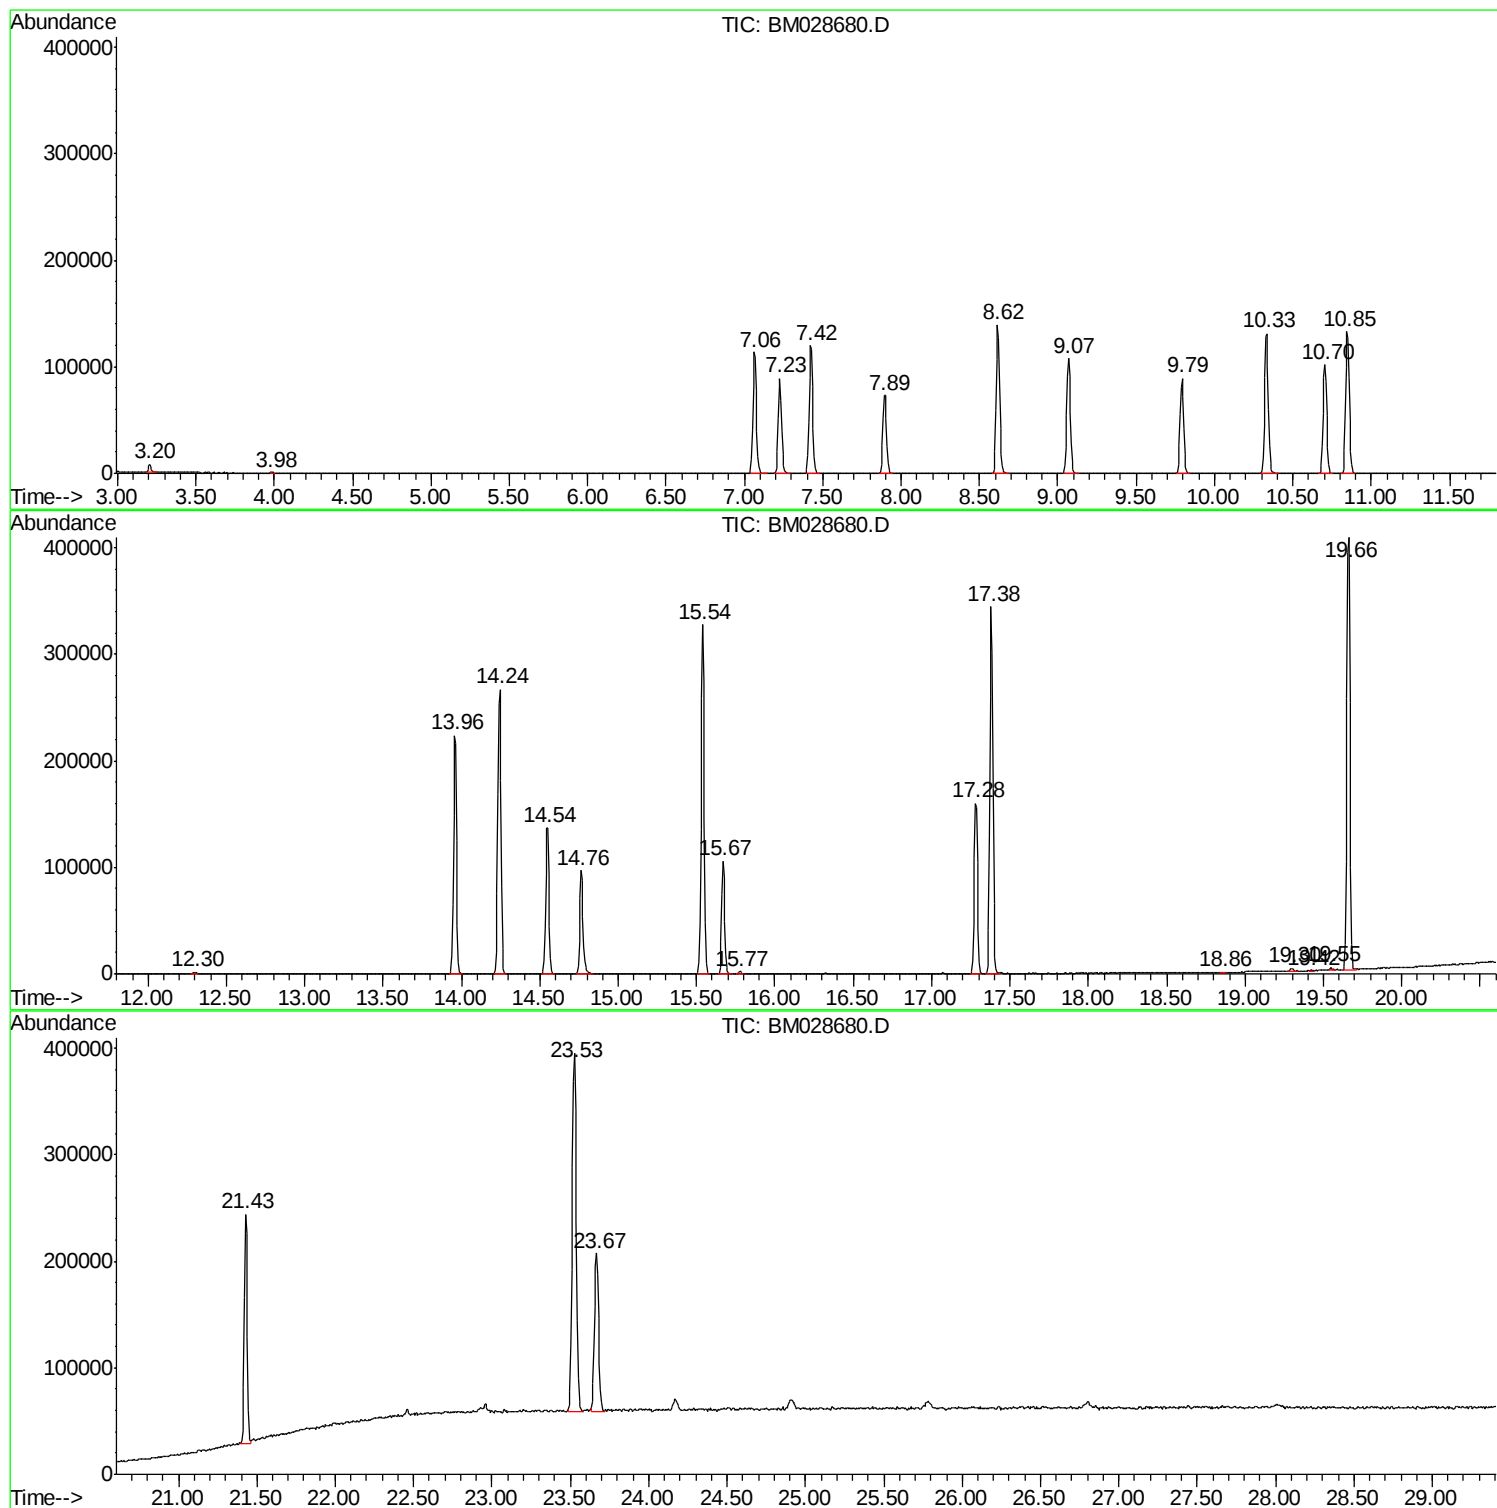

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM020921\
Data File : BM028680.D
Acq On : 09 Feb 2021 10:33
Operator : CG/JU
Sample : PB134489BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK89

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM011621MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM020921\
Data File : BM028680.D
Acq On : 09 Feb 2021 10:33
Operator : CG/JU
Sample : PB134489BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK89

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM011621MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc