


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM020921\
 Data File : BM028678.D
 Acq On : 09 Feb 2021 08:41
 Operator : CG/JU
 Sample : DFTPP25
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP25

Integration File: LSCINT.P

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM011621MA.M
 Title : SVOA CALIBRATION
 Last Update : Tue Feb 09 10:35:42 2021

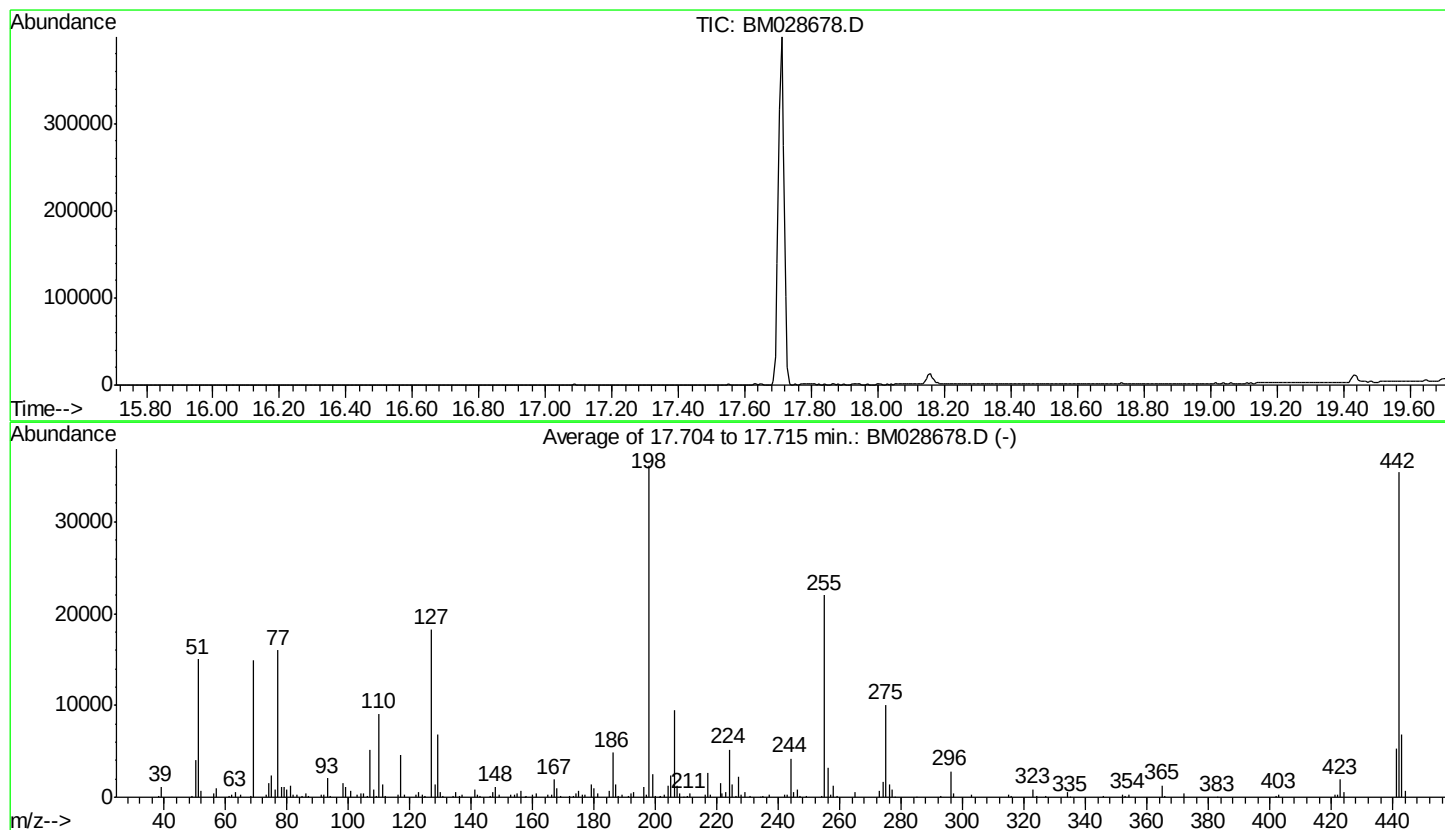

AutoFind: Scans 2468, 2469, 2470; Background Corrected with Scan 2463

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.7	15041	PASS
68	69	0.00	2	1.4	213	PASS
69	198	0.00	100	41.1	14854	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	50.4	18199	PASS
197	198	0.00	2	0.7	250	PASS
198	198	100	100	100.0	36112	PASS
199	198	5	9	6.8	2473	PASS
275	198	10	60	27.8	10051	PASS
365	198	1	100	3.6	1314	PASS
441	198	0.01	100	14.7	5301	PASS
442	198	50	100	97.9	35370	PASS
443	442	15	24	19.5	6905	PASS

Scan 2463 (17.674 min): BM028678.D
DFTPP25

m/z	Abundance
44.00	271.0
207.00	303.0

Instrument :
BNA_M
ClientSampleId :
DFTPP25

m/z	Abundance
38.00	248.0
39.00	1271.0
43.90	238.0
49.00	183.0
50.10	4447.0
51.10	17000.0
52.00	776.0
56.00	510.0
57.00	1022.0
61.00	169.0
62.00	306.0
63.00	550.0
65.00	198.0
68.10	300.0
69.00	16039.0
73.00	283.0
74.00	1529.0
75.00	2668.0
76.10	868.0
77.10	17432.0
78.00	1308.0
79.00	1281.0
80.00	876.0
81.00	1388.0
81.90	297.0
83.00	301.0
85.00	216.0
86.00	322.0
86.90	177.0
90.90	258.0
92.00	345.0
93.00	2132.0
94.00	187.0
98.00	1801.0
99.00	1253.0
100.90	716.0
103.00	250.0
104.00	454.0
105.00	453.0
105.90	172.0
107.00	5466.0
108.00	864.0
109.00	175.0
110.00	9541.0
111.00	1553.0
111.90	193.0
116.00	323.0
117.00	4854.0
118.00	379.0
122.00	335.0
122.90	536.0
124.00	287.0
125.00	205.0
127.00	18856.0
128.00	1468.0
129.00	7109.0
130.00	627.0
130.90	162.0
134.00	230.0
135.00	731.0
136.00	255.0
137.00	301.0
141.00	960.0
141.90	323.0
142.90	177.0
146.00	197.0
147.00	549.0
148.00	1197.0
149.00	308.0
153.00	300.0
154.00	226.0
155.00	470.0
156.00	584.0
158.00	179.0
159.90	285.0
161.00	432.0
164.90	383.0
166.00	316.0
167.00	1915.0
168.00	1090.0
169.00	163.0
171.90	159.0
173.10	203.0
173.90	387.0
175.00	706.0
175.90	254.0
177.00	302.0
179.00	1377.0
180.00	994.0
181.00	403.0
185.00	636.0
186.00	4728.0

Instrument :
BNA_M
ClientSampleId :
DFTPP25

187.00	1298.0
187.90	154.0
189.00	312.0
190.90	199.0
192.00	435.0
193.00	467.0
195.90	898.0
196.90	184.0
197.10	188.0
198.00	34600.0
199.00	2511.0
200.00	157.0
201.20	179.0
202.90	249.0
204.00	1229.0
205.00	2291.0
206.00	9093.0
207.00	1559.0
208.00	362.0
209.00	167.0
210.30	154.0
210.90	379.0
216.00	206.0
217.00	2442.0
217.90	307.0
221.00	1493.0
221.70	350.0
222.90	629.0
224.00	5013.0
225.00	1280.0
226.00	157.0
227.00	2112.0
228.00	321.0
228.90	390.0
235.00	150.0
237.00	222.0
242.00	294.0
242.90	272.0
244.00	3803.0
245.00	551.0
246.00	739.0
254.20	178.0
255.00	19792.0
256.00	2889.0
256.90	247.0
258.00	1229.0
258.90	188.0
265.00	526.0
273.00	647.0
274.00	1497.0
275.00	8791.0
276.00	1191.0
276.90	780.0
296.00	2608.0
296.90	360.0
303.00	244.0
314.90	289.0
315.90	171.0
323.00	729.0
334.00	496.0
351.90	237.0
354.00	266.0
365.00	1030.0
365.90	158.0
372.00	439.0
401.90	172.0
403.00	213.0
421.00	169.0
421.90	198.0
423.00	1269.0
424.00	579.0
441.00	3877.0
442.00	25840.0
443.00	5054.0
444.00	574.0

Instrument :
BNA_M
ClientSampleId :
DFTPP25

m/z	Abundance
38.00	193.0
39.00	1514.0
44.00	262.0
49.00	176.0
50.10	4747.0
51.10	17792.0
52.00	869.0
56.00	537.0
57.00	1268.0
61.00	222.0
62.00	269.0
63.00	791.0
65.00	328.0
68.00	341.0
69.00	18128.0
73.00	305.0
74.00	1961.0
75.00	2740.0
76.00	989.0
77.10	19224.0
78.10	1233.0
79.00	1346.0
80.00	1120.0
81.00	1411.0
82.00	367.0
83.00	345.0
85.00	226.0
86.00	466.0
87.00	203.0
91.00	399.0
92.00	334.0
93.00	2564.0
93.90	171.0
98.00	1747.0
99.00	1471.0
100.90	844.0
103.00	256.0
104.00	585.0
104.90	565.0
106.00	184.0
107.00	6045.0
108.00	989.0
109.10	225.0
110.00	11027.0
111.00	1638.0
111.90	184.0
116.00	351.0
117.00	5564.0
118.00	415.0
122.00	397.0
123.00	648.0
124.00	307.0
125.00	282.0
127.00	22008.0
128.00	1646.0
129.00	8334.0
130.00	776.0
130.90	167.0
134.00	212.0
135.00	699.0
135.90	236.0
137.00	373.0
141.00	1087.0
142.00	337.0
143.00	200.0
146.00	196.0
147.00	610.0
148.00	1395.0
148.90	280.0
152.90	319.0
154.00	275.0
155.00	572.0
156.00	791.0
157.20	151.0
158.00	221.0
160.00	357.0
161.00	485.0
164.90	372.0
166.00	265.0
167.00	2446.0
168.00	1125.0
168.90	201.0
171.90	232.0
173.00	259.0
174.00	449.0
175.00	924.0
176.00	301.0
177.00	435.0
179.00	1565.0
180.00	1213.0
181.00	485.0
185.00	720.0

Instrument :
BNA_M
ClientSampleId :
DFTPP25

186.00	5761.0
187.00	1928.0
188.00	151.0
189.00	405.0
190.90	229.0
192.00	566.0
193.00	606.0
196.00	1467.0
197.10	324.0
198.00	43648.0
199.00	2949.0
199.90	241.0
201.50	220.0
203.00	341.0
204.00	1555.0
205.00	2757.0
206.00	11435.0
207.00	1816.0
208.00	466.0
210.10	199.0
211.00	445.0
215.90	276.0
217.00	3243.0
218.00	411.0
221.00	2029.0
221.70	398.0
223.00	654.0
224.00	6018.0
225.10	1693.0
225.90	182.0
227.00	2627.0
228.00	329.0
228.90	651.0
230.90	237.0
233.90	170.0
235.00	241.0
236.90	268.0
242.00	343.0
243.00	388.0
244.10	5427.0
245.00	708.0
246.00	1037.0
247.00	235.0
249.00	237.0
255.00	26712.0
256.00	3967.0
256.90	359.0
258.00	1537.0
259.00	220.0
264.90	644.0
273.00	799.0
274.00	2155.0
275.00	12290.0
276.00	1752.0
277.00	964.0
277.90	176.0
284.90	209.0
292.90	242.0
296.00	3366.0
296.90	449.0
303.00	463.0
315.00	418.0
316.00	239.0
323.00	1100.0
324.00	172.0
326.90	279.0
334.00	708.0
335.00	171.0
345.90	243.0
352.00	320.0
353.00	228.0
354.00	359.0
365.00	1559.0
366.00	234.0
372.00	484.0
382.90	192.0
402.00	262.0
402.90	303.0
421.00	344.0
422.00	351.0
423.00	2371.0
423.90	584.0
441.00	6303.0
442.00	42136.0
443.00	8457.0
444.00	788.0

Instrument :
BNA_M
ClientSampleId :
DFTPP25

m/z	Abundance
39.00	729.0
44.00	309.0
50.00	2758.0
51.10	10331.0
52.10	486.0
56.10	294.0
57.00	676.0
61.90	163.0
63.00	407.0
65.00	199.0
69.00	10396.0
73.00	266.0
74.00	1215.0
75.00	1742.0
76.00	557.0
77.10	11337.0
78.00	794.0
79.00	785.0
80.00	645.0
81.00	923.0
81.90	237.0
83.00	195.0
86.00	291.0
90.90	188.0
92.00	243.0
93.00	1424.0
98.00	1191.0
98.90	724.0
100.90	444.0
102.90	176.0
103.90	298.0
105.00	329.0
107.00	3960.0
108.00	565.0
110.00	6784.0
111.00	928.0
116.00	197.0
117.00	3348.0
117.90	222.0
121.90	304.0
123.00	387.0
123.90	188.0
124.80	154.0
127.00	13735.0
128.00	975.0
129.00	5201.0
129.90	462.0
134.00	169.0
135.00	459.0
137.00	189.0
141.00	685.0
141.90	236.0
143.00	189.0
147.00	407.0
148.00	888.0
148.90	201.0
153.00	184.0
154.00	175.0
155.00	394.0
156.00	540.0
158.00	151.0
160.00	243.0
161.00	387.0
165.00	247.0
165.90	223.0
167.00	1476.0
168.00	693.0
173.00	172.0
174.00	277.0
175.00	564.0
175.90	151.0
176.90	296.0
178.90	1160.0
180.00	798.0
180.90	345.0
185.00	597.0
186.00	4035.0
187.00	1069.0
189.00	225.0
191.00	181.0
191.90	370.0
193.00	481.0
196.00	885.0
197.10	240.0
198.00	30088.0
199.00	1959.0
200.00	165.0
201.40	170.0
203.00	206.0
204.00	1069.0
205.00	1921.0
206.00	7987.0

Instrument :
BNA_M
ClientSampleId :
DFTPP25

207.00	1321.0
208.00	327.0
210.20	155.0
211.00	334.0
215.90	162.0
217.00	2265.0
217.90	278.0
221.00	1268.0
221.70	326.0
223.00	408.0
224.00	4562.0
225.00	1142.0
227.00	1913.0
227.90	262.0
229.00	451.0
235.00	206.0
237.00	159.0
242.00	247.0
243.00	215.0
244.00	3520.0
245.00	533.0
246.00	729.0
246.90	178.0
248.90	190.0
254.20	157.0
255.00	19488.0
256.00	2851.0
256.90	263.0
258.00	1007.0
259.00	177.0
264.90	528.0
273.00	639.0
274.00	1563.0
275.00	9073.0
276.00	1260.0
277.00	692.0
293.00	169.0
296.00	2556.0
296.90	318.0
303.00	284.0
315.00	288.0
316.00	158.0
323.00	832.0
324.00	199.0
326.90	180.0
334.00	531.0
345.90	204.0
351.90	231.0
352.90	167.0
354.00	248.0
365.00	1353.0
365.80	174.0
372.00	470.0
402.00	161.0
403.00	370.0
421.00	285.0
422.00	244.0
423.00	2033.0
424.00	559.0
441.00	5724.0
442.00	38136.0
443.00	7205.0
443.90	726.0

Instrument :
BNA_M
ClientSampleId :
DFTPP25