
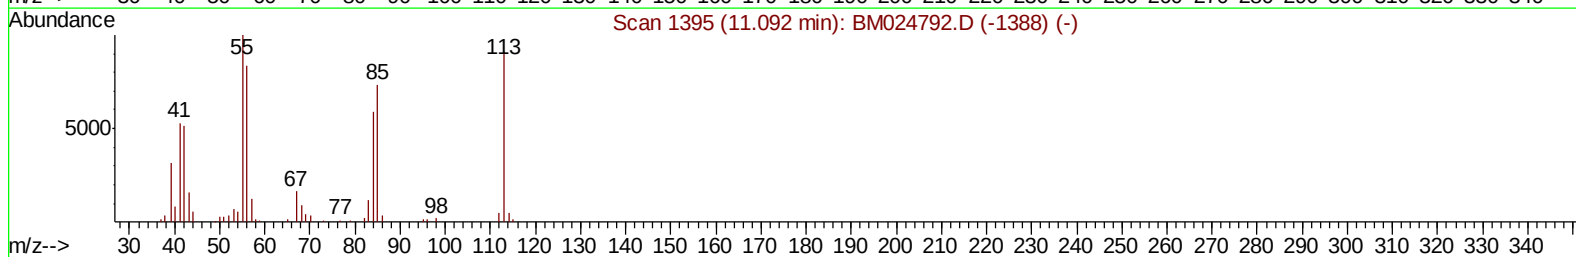
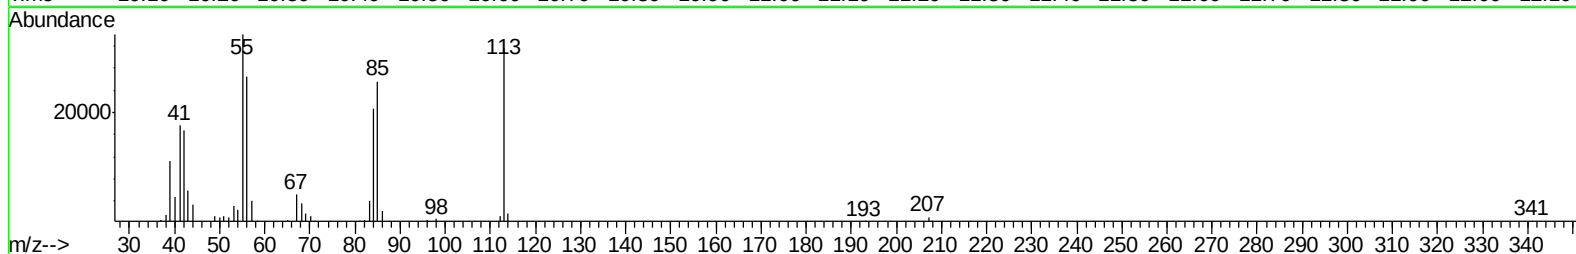


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM021020\
Data File : BM024813.D
Acq On : 10 Feb 2020 18:04
Operator : CG/JU
Sample : SSTDCCC020
Misc :
ALS Vial : 2 Sample Multiplier: 1

Quant Time: Feb 11 03:47:05 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM020620MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Feb 07 07:38:13 2020
Response via : Initial Calibration

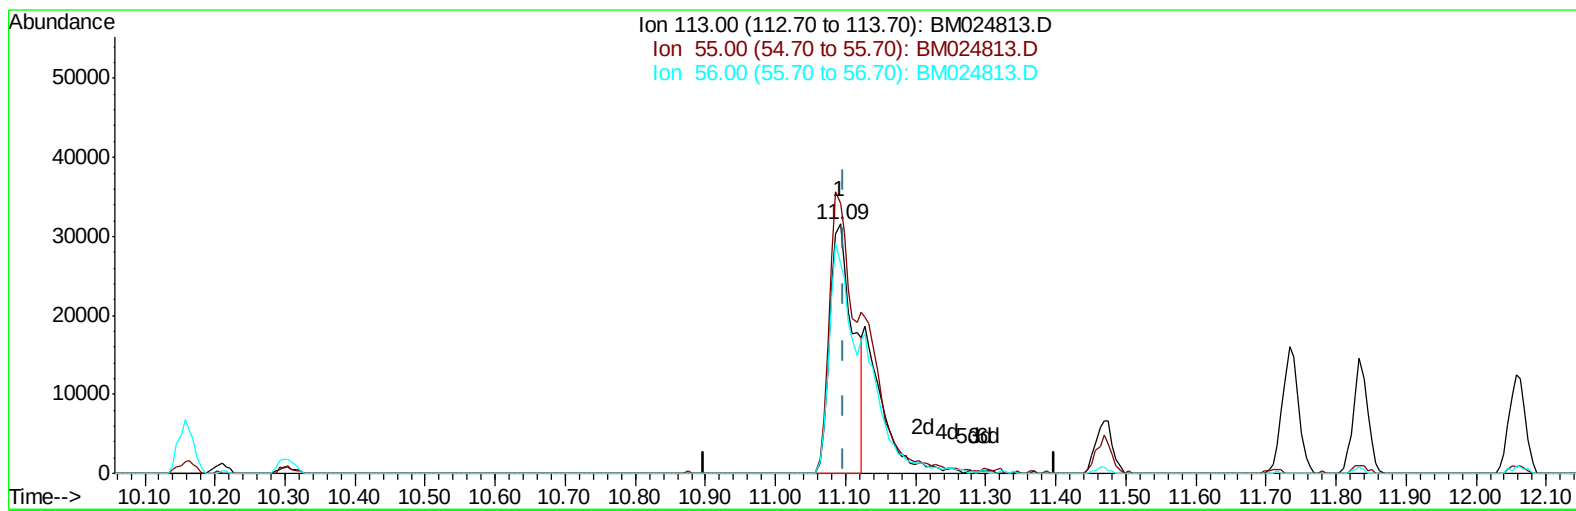

TIC: BM024813.D

(32) Caprolactam

11.092min (-0.006) 13.48ng/ul

response 72238

Ion	Exp%	Act%
113.00	100	100
55.00	107.70	108.03
56.00	89.90	84.15
0.00	0.00	0.00