
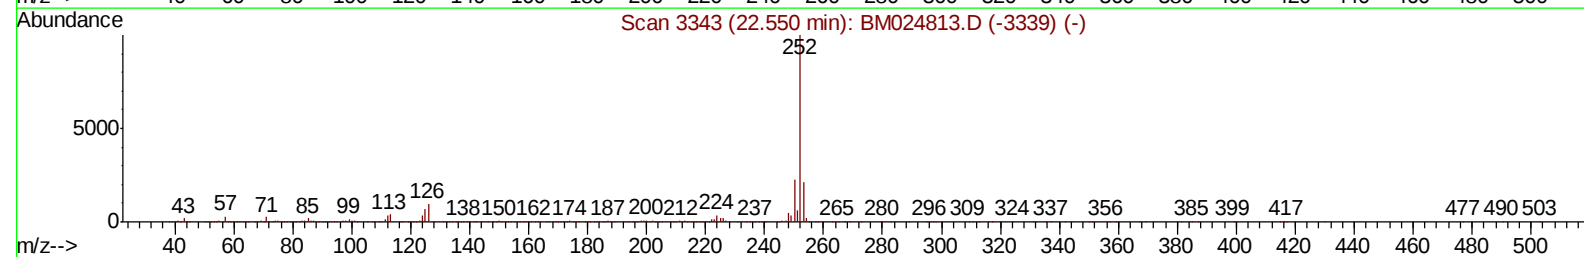
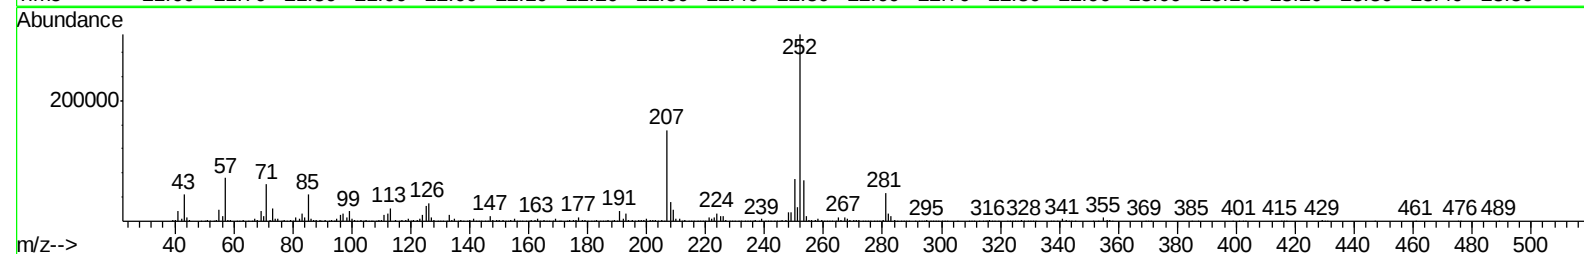


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM021020\
Data File : BM024821.D
Acq On : 10 Feb 2020 22:53
Operator : CG/JU
Sample : L1402-14
Misc :
ALS Vial : 18 Sample Multiplier: 1

Quant Time: Feb 11 03:48:30 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM020620MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Feb 07 07:38:13 2020
Response via : Initial Calibration

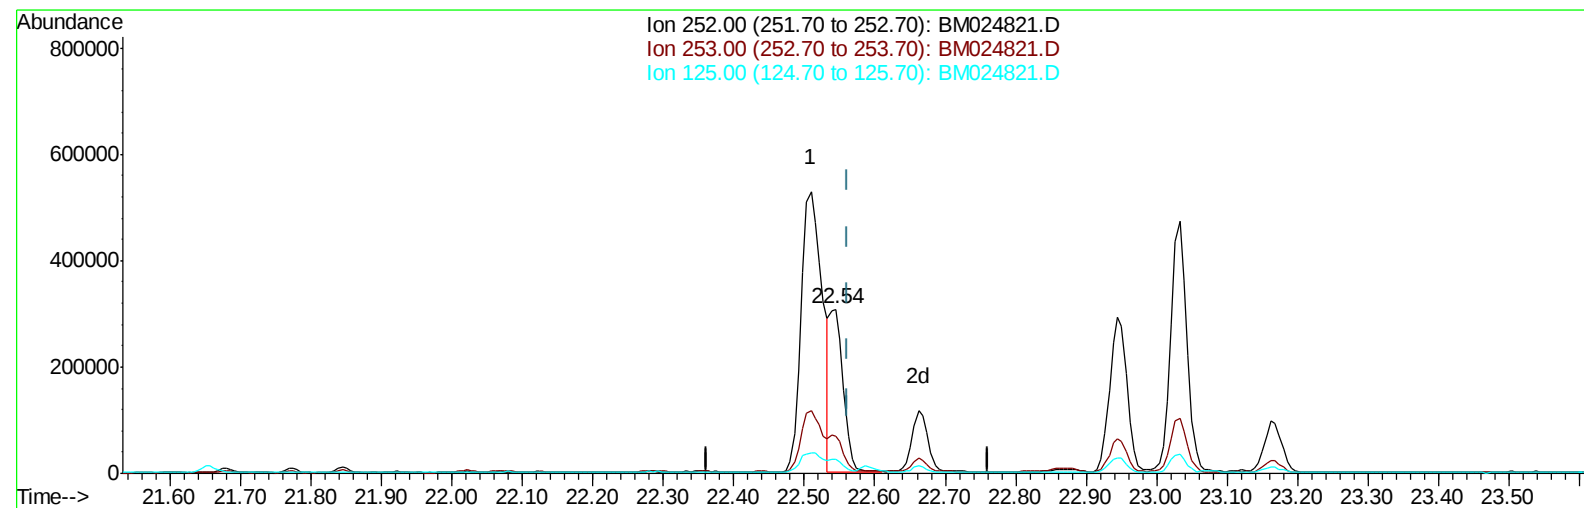

TIC: BM024821.D

(89) Benzo(k)fluoranthene

22.545min (-0.017) 3.95ng/ul m

response 400260

Ion	Exp%	Act%
252.00	100	100
253.00	21.70	22.30
125.00	6.40	8.45#
0.00	0.00	0.00