
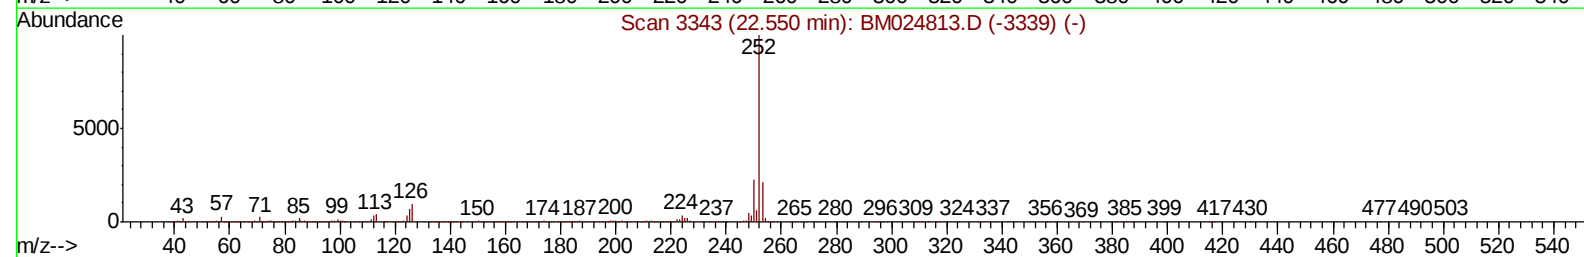
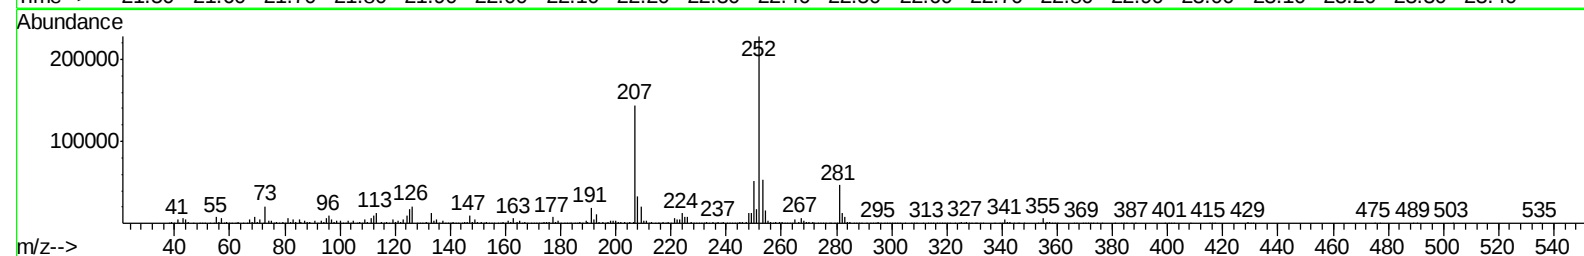


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM021020\
Data File : BM024825.D
Acq On : 11 Feb 2020 01:17
Operator : CG/JU
Sample : L1402-18
Misc :
ALS Vial : 22 Sample Multiplier: 1

Quant Time: Feb 11 03:49:10 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM020620MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Feb 07 07:38:13 2020
Response via : Initial Calibration

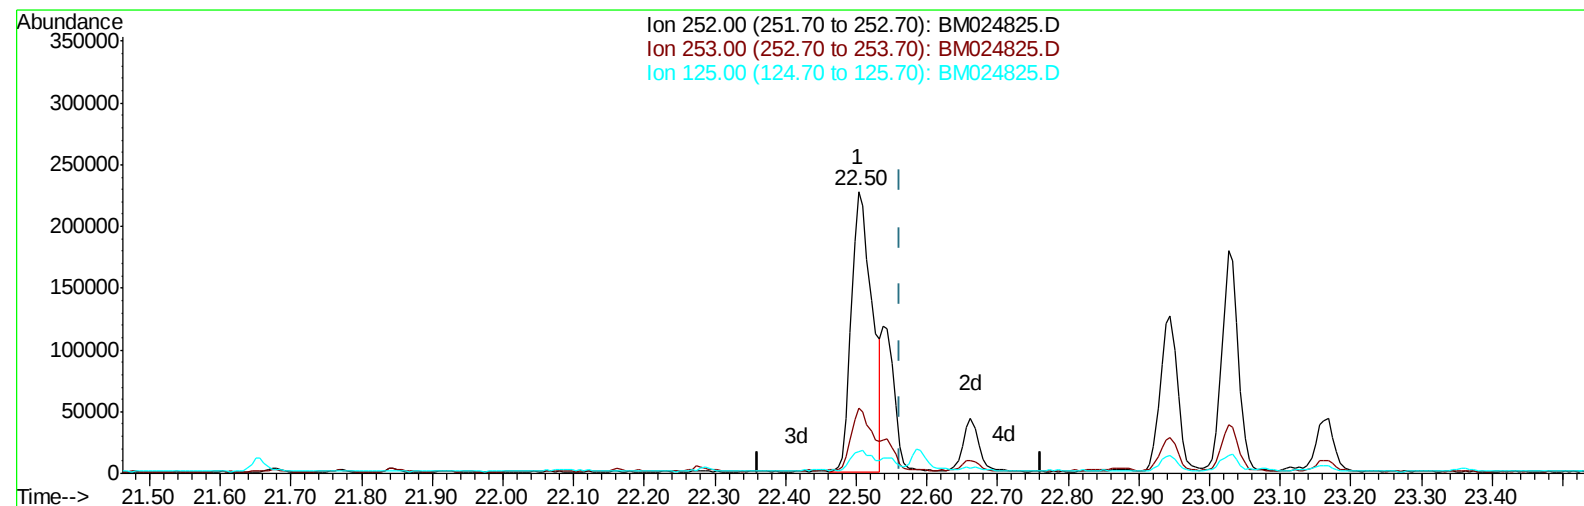

TIC: BM024825.D

(89) Benzo(k)fluoranthene

22.503min (-0.059) 4.86ng/ul

response 468656

Ion	Exp%	Act%
252.00	100	100
253.00	21.70	23.16
125.00	6.40	7.62
0.00	0.00	0.00